


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU121418\
Data File : VU028665.D
Acq On : 13 Dec 2018 08:34
Operator : MD/SY
Sample : BFB
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U112618DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Tue Nov 27 01:03:50 2018

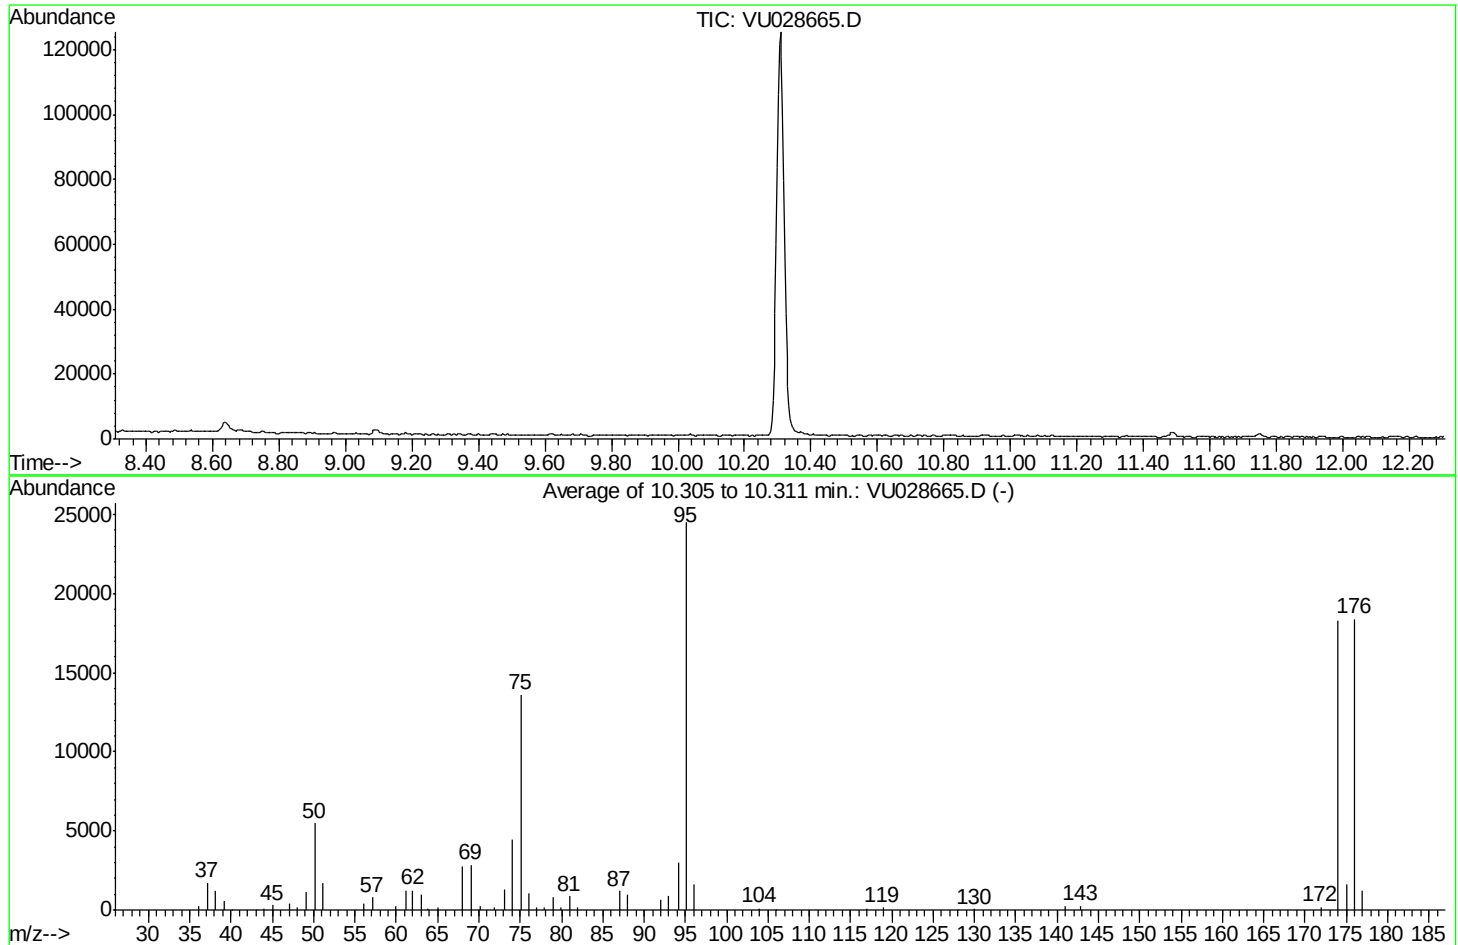

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.3	5466	PASS
75	95	30	60	55.6	13614	PASS
95	95	100	100	100.0	24501	PASS
96	95	5	9	6.5	1594	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	74.8	18320	PASS
175	174	5	9	8.9	1637	PASS
176	174	95	101	100.4	18386	PASS
177	176	5	9	6.7	1228	PASS