


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU121420\
Data File : VU041622.D
Acq On : 14 Dec 2020 19:49
Operator : SY/MD
Sample : L5027-20
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB1J9

Manual Integrations
APPROVED

apatel
12/16/2020 8:56:29 AM

Quant Time: Dec 15 02:27:53 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 15 00:46:25 2020
Response via : Initial Calibration

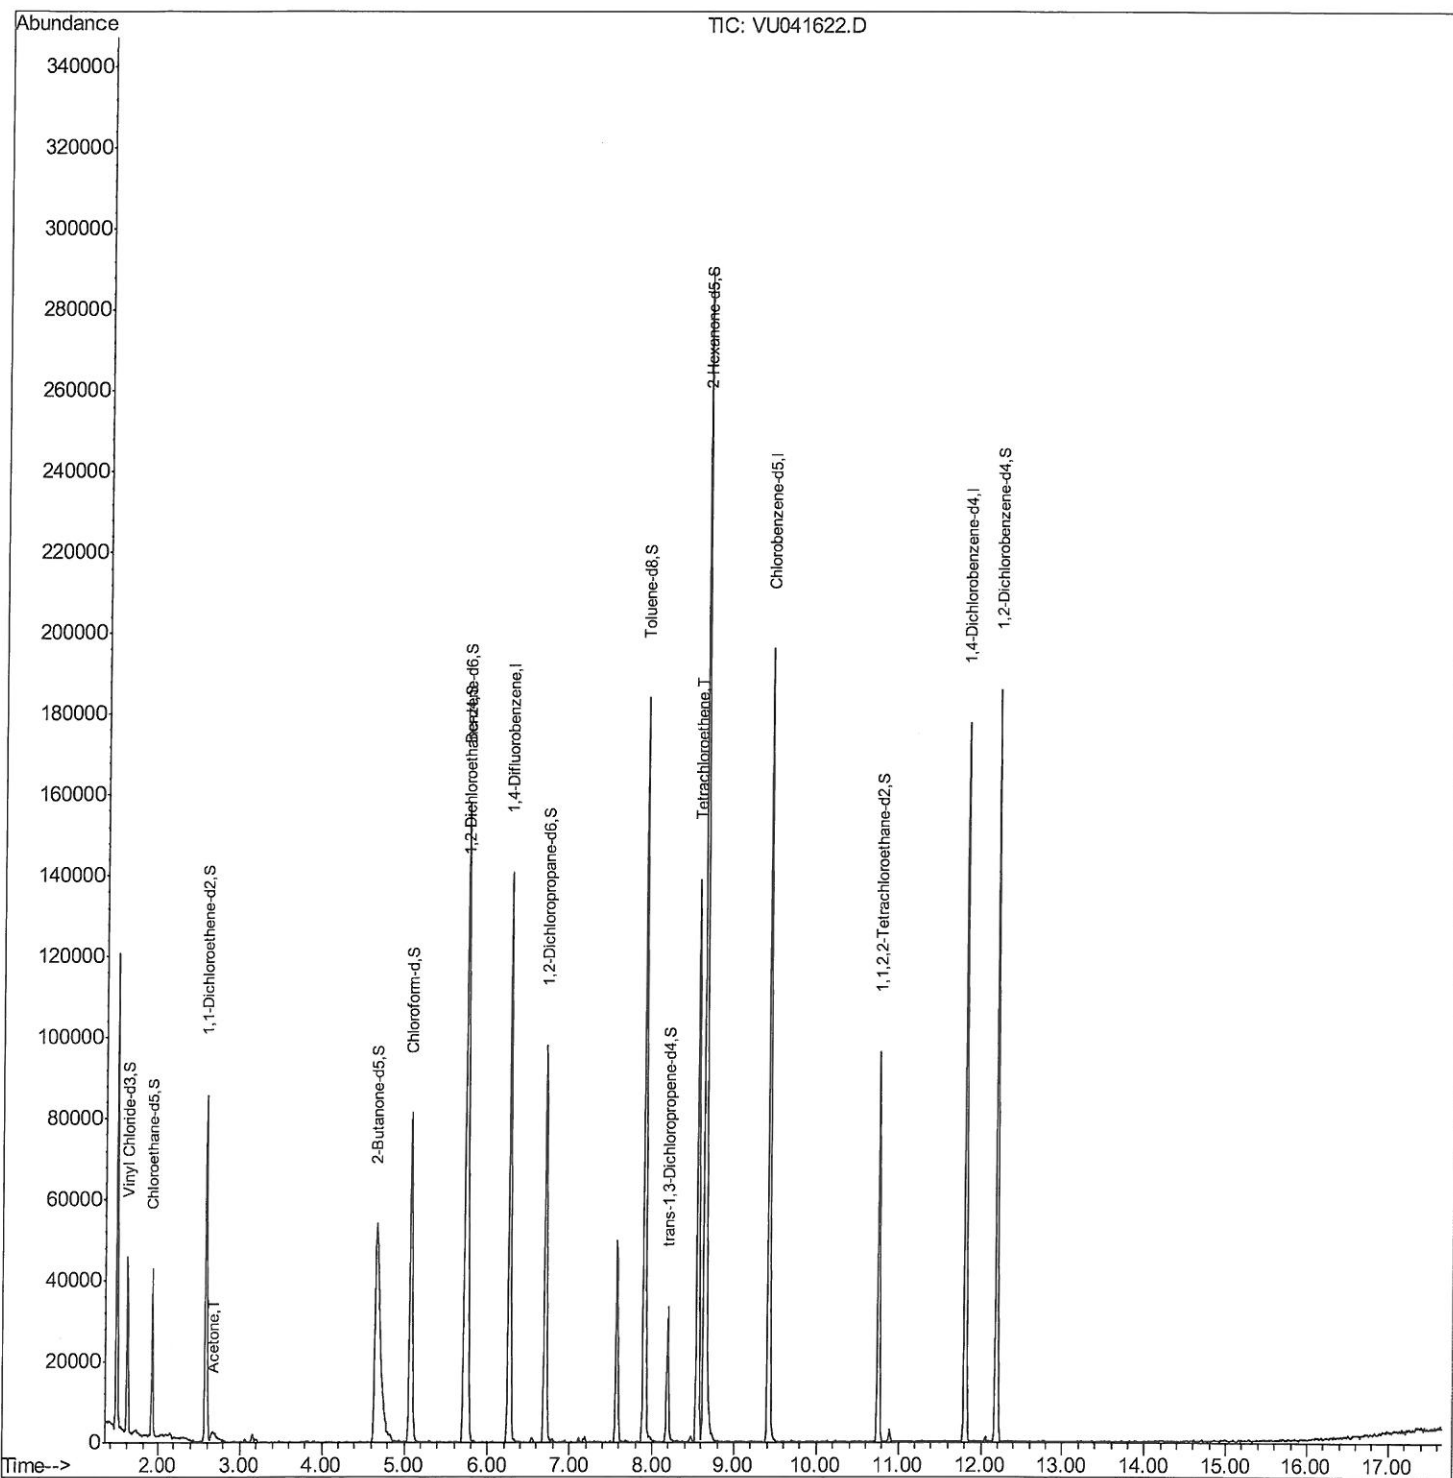

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU121420\
 Data File : VU041622.D
 Acq On : 14 Dec 2020 19:49
 Operator : SY/MD
 Sample : L5027-20
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GB1J9

Manual Integrations
 APPROVED

apatel
 12/16/2020 8:56:29 AM

Quant Time: Dec 15 00:50:27 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Dec 15 00:46:25 2020
 Response via : Initial Calibration

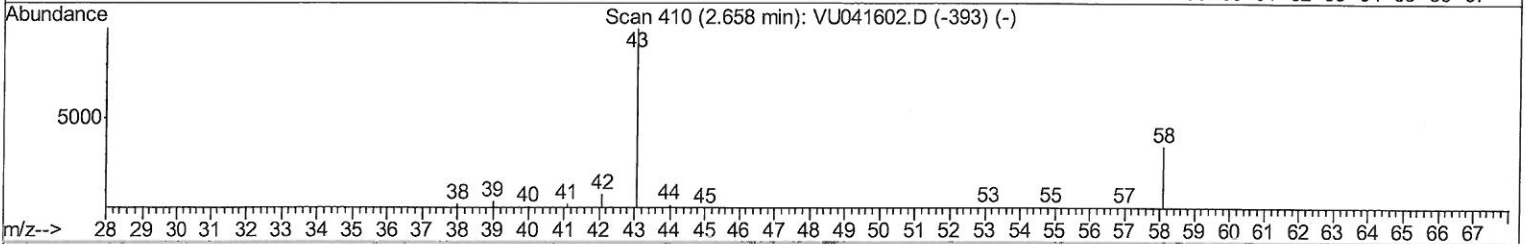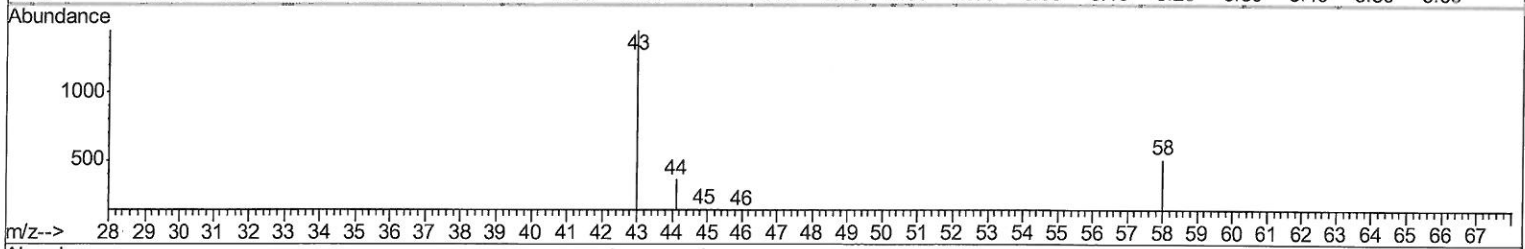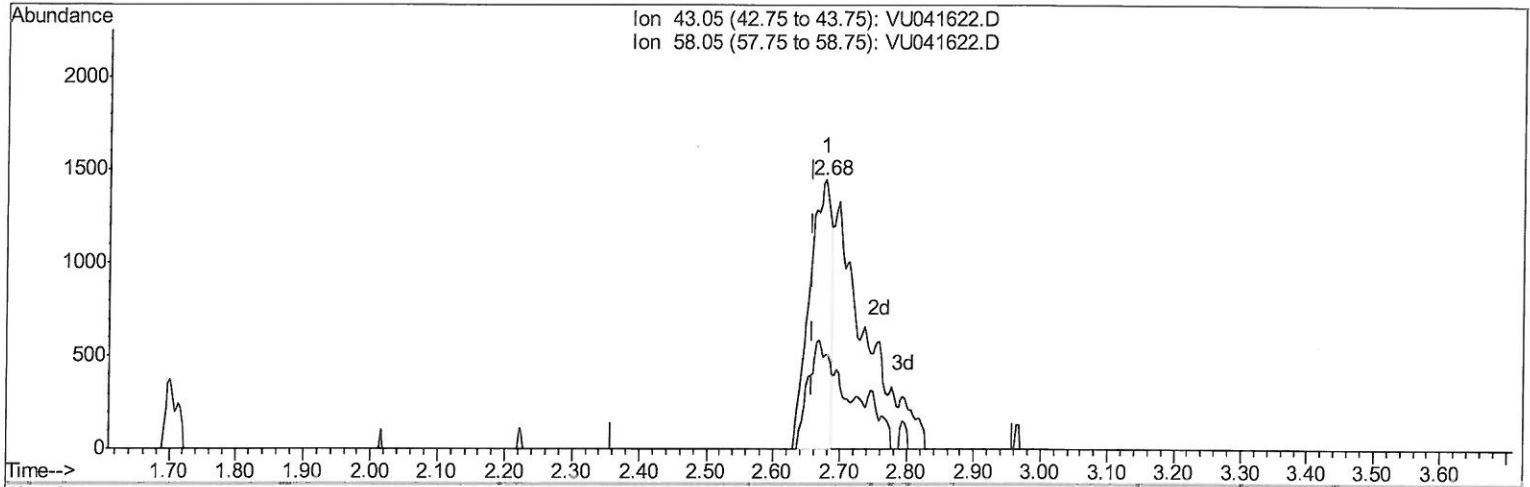

TIC: VU041622.D

(13) Acetone (T)

2.677min (+0.019) 1.92ug/L

response 3281

Ion	Exp%	Act%
43.05	100	100
58.05	36.60	40.93
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU121420\
 Data File : VU041622.D
 Acq On : 14 Dec 2020 19:49
 Operator : SY/MD
 Sample : L5027-20
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GB1J9

Manual Integrations
 APPROVED

apatel
 12/16/2020 8:56:29 AM

Quant Time: Dec 15 00:50:27 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Dec 15 00:46:25 2020
 Response via : Initial Calibration

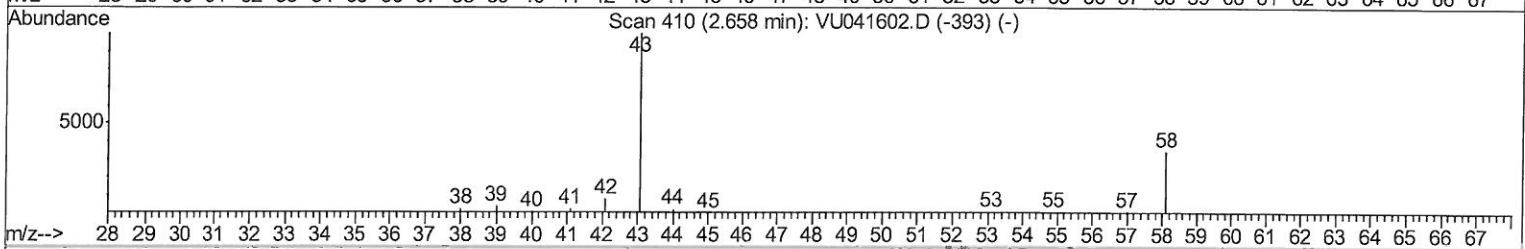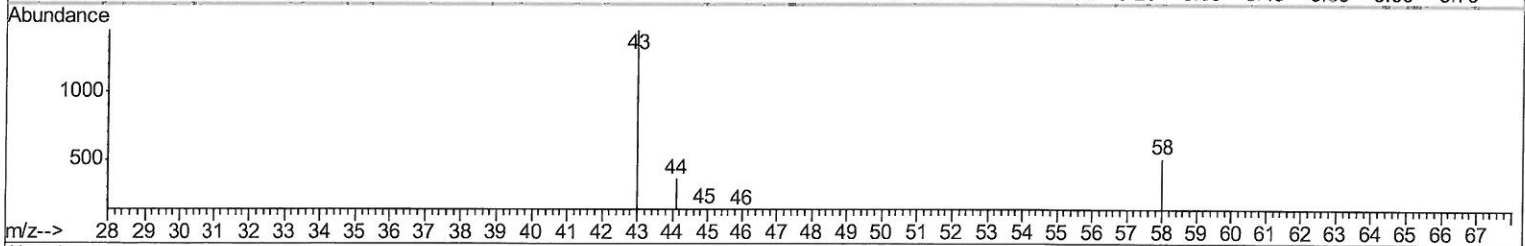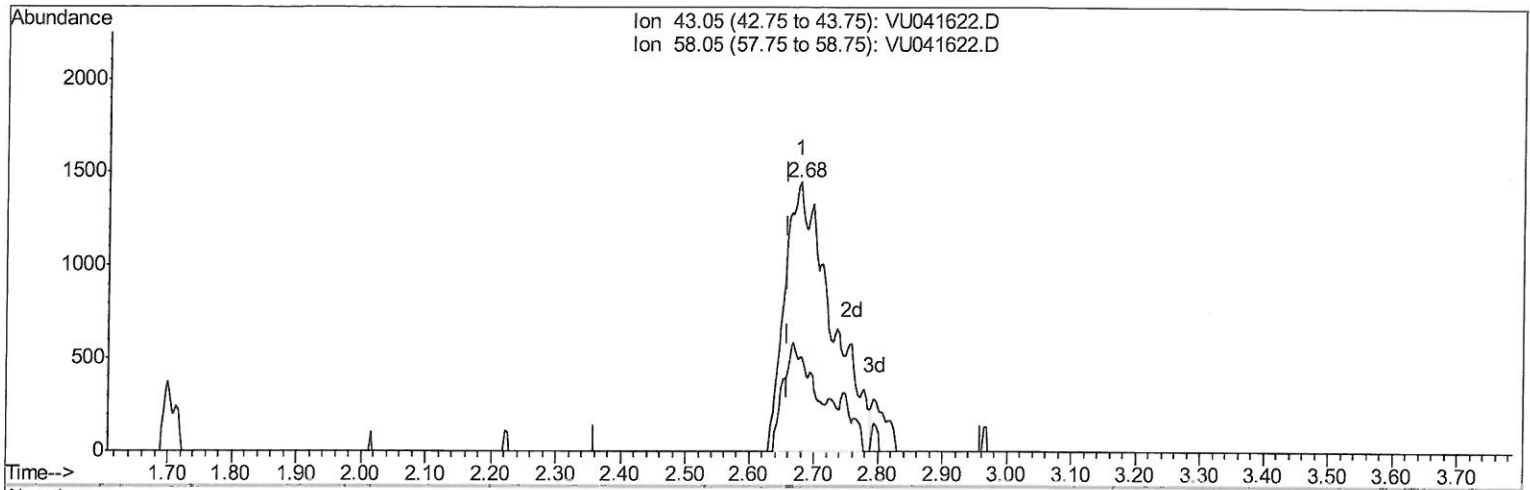

(13) Acetone (T)

2.677min (+0.019) 4.26ug/L m

response 7270

Ion Exp% Act%

43.05 100 100

58.05 36.60 18.47

0.00 0.00 0.00

0.00 0.00 0.00

7 ME
12/18/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU121420\
 Data File : VU041622.D
 Acq On : 14 Dec 2020 19:49
 Operator : SY/MD
 Sample : L5027-20
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GB1J9

Manual Integrations
 APPROVED

apatel
 12/16/2020 8:56:29 AM

Quant Time: Dec 15 02:27:53 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Dec 15 00:46:25 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	6.26	114	119454	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	111233	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	47830	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	29194	3.13	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	62.60%
7) Chloroethane-d5	1.92	69	30125	4.17	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	83.40%
11) 1,1-Dichloroethene-d2	2.58	63	51741	3.01	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	60.20%
20) 2-Butanone-d5	4.66	46	146816	54.73	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	109.46%
24) Chloroform-d	5.08	84	75966	4.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.00%
26) 1,2-Dichloroethane-d4	5.72	65	44972	4.96	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.20%
32) Benzene-d6	5.74	84	147448	4.63	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.60%
36) 1,2-Dichloropropane-d6	6.70	67	48870	4.89	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.80%
41) Toluene-d8	7.91	98	127036	4.42	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.40%
43) trans-1,3-Dichloropropene-	8.19	79	19932	4.44	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.80%
46) 2-Hexanone-d5	8.64	63	112818	45.96	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.92%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	48617	5.36	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	107.20%
64) 1,2-Dichlorobenzene-d4	12.19	152	48981	5.76	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	115.20%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
13) Acetone	2.68	43	7270m	4.261	ug/L	
47) Tetrachloroethene	8.56	164	30873	4.934	ug/L	99

ME
 12/18/20

(#) = qualifier out of range (m) = manual integration (+) = signals summed