

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U121420\
 Data File : VU041606.D
 Acq On : 14 Dec 2020 12:33
 Operator : SY/MD
 Sample : L5060-02
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B00

Quant Time: Dec 15 00:58:44 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Dec 15 00:46:25 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	134690	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	131135	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	65390	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	48447	4.60	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.00%
7) Chloroethane-d5	1.92	69	39412	4.84	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.80%
11) 1,1-Dichloroethene-d2	2.58	63	68024	3.51	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.20%
20) 2-Butanone-d5	4.66	46	159411	52.70	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	105.40%
24) Chloroform-d	5.08	84	84486	4.68	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.60%
26) 1,2-Dichloroethane-d4	5.72	65	50048	4.89	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.80%
32) Benzene-d6	5.74	84	173122	4.61	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.20%
36) 1,2-Dichloropropane-d6	6.70	67	55022	4.67	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.40%
41) Toluene-d8	7.91	98	152523	4.50	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.00%
43) trans-1,3-Dichloropropene-	8.19	79	23994	4.53	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.60%
46) 2-Hexanone-d5	8.64	63	138805	47.96	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.92%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	51683	4.83	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.60%
64) 1,2-Dichlorobenzene-d4	12.19	152	57930	4.98	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.60%


Target Compounds					Ovalue
13) Acetone	2.66	43	12355	6.422 ug/L	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU121420\
Data File : VU041606.D
Acq On : 14 Dec 2020 12:33
Operator : SY/MD
Sample : L5060-02
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B00

Quant Time: Dec 15 00:58:44 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 15 00:46:25 2020
Response via : Initial Calibration

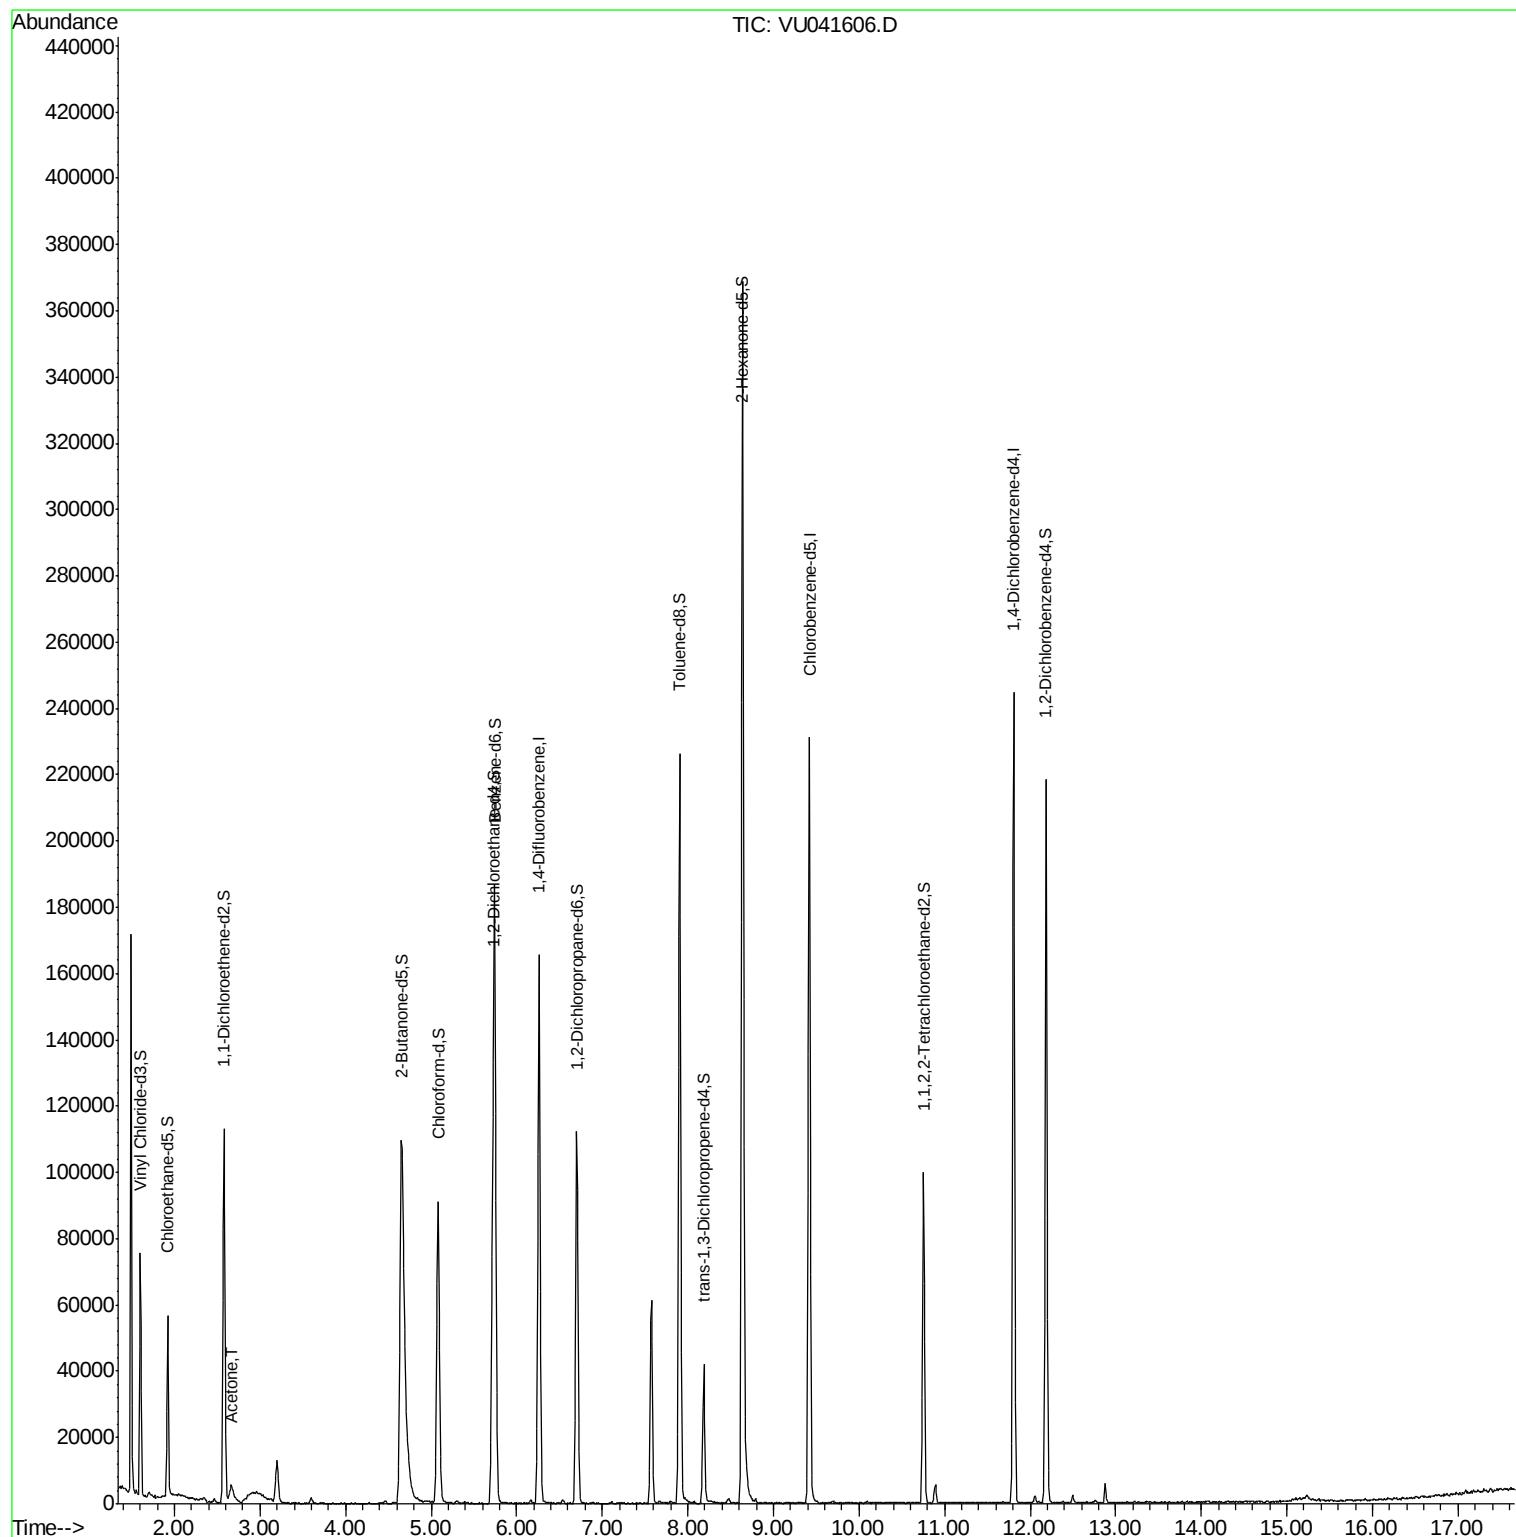

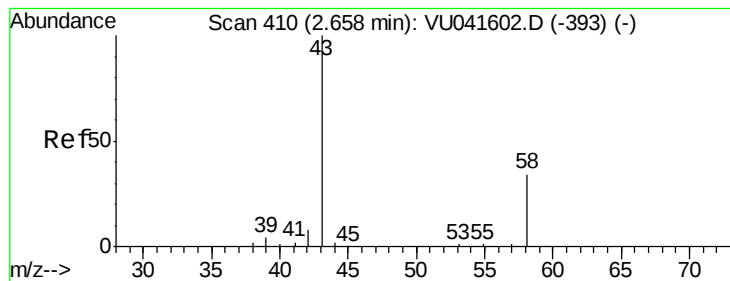

#13
 Acetone
 Concen: 6.422 ug/L
 RT: 2.66 min Scan# 412
 Delta R.T. 0.01 min
 Lab File: VU041606.D
 Acq: 14 Dec 2020 12:33

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B00

Tot Ion: 43 Resp: 12355
 Ion Ratio Lower Upper
 43 100
 58 26.2 0.0 73.2

