


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU121420\
Data File : VU041601.D
Acq On : 14 Dec 2020 09:21
Operator : SY/MD
Sample : BFB24
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB24

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
Title : TRACE VOA SOM01.0
Last Update : Tue Dec 15 00:46:25 2020

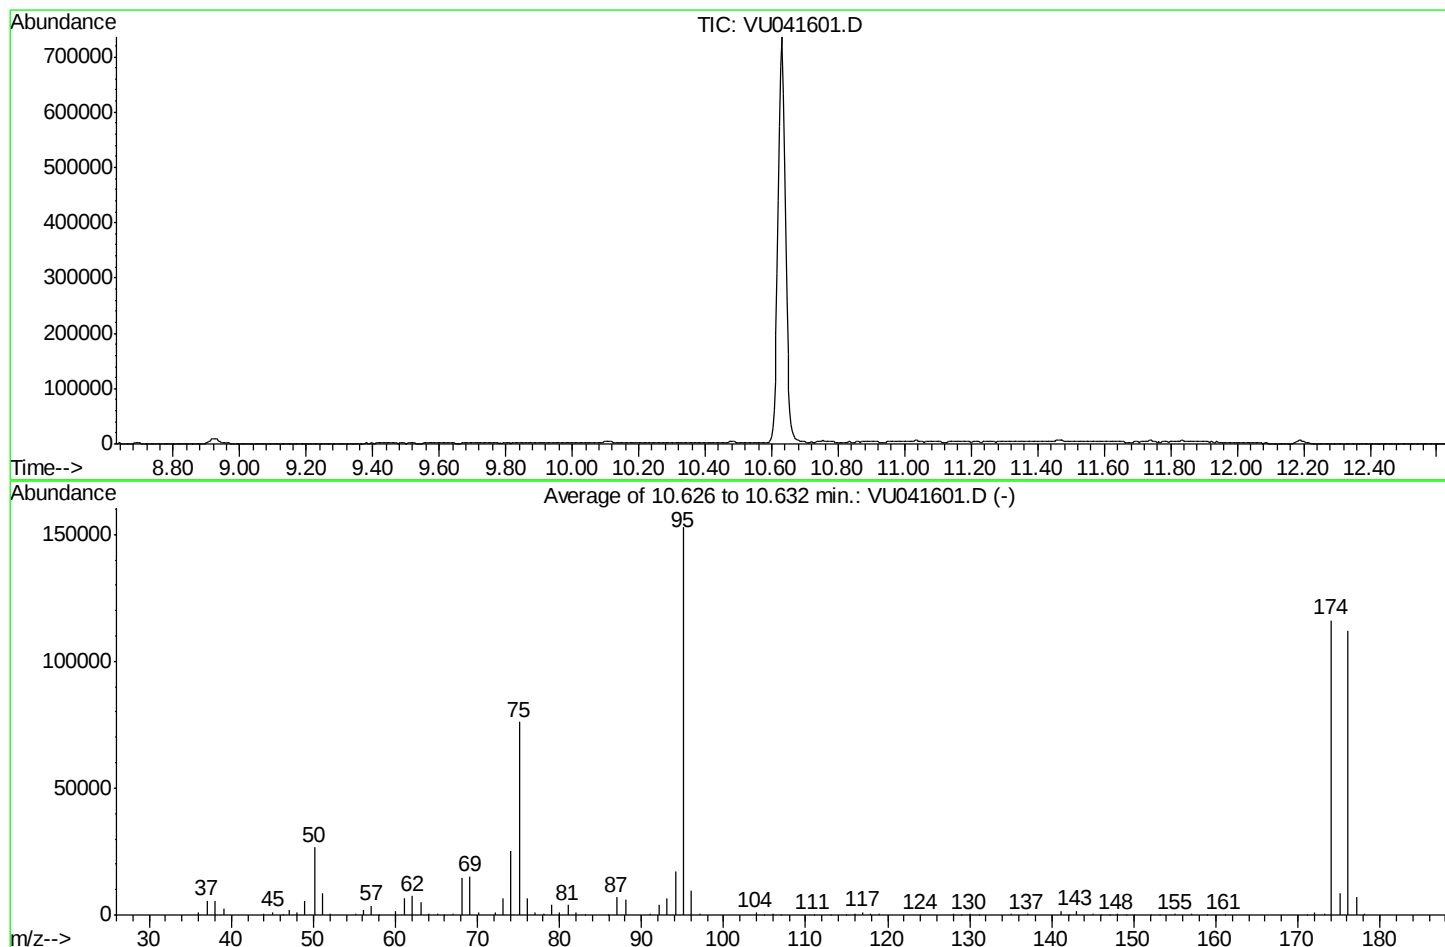

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2874

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	26706	PASS
75	95	30	80	49.7	76010	PASS
95	95	100	100	100.0	152832	PASS
96	95	5	9	6.2	9541	PASS
173	174	0.00	2	0.4	490	PASS
174	95	50	120	76.0	116114	PASS
175	174	5	9	7.3	8445	PASS
176	174	95	101	96.3	111848	PASS
177	176	5	9	6.3	7053	PASS

Scan 2874 (10.581 min): VU041601.D
BFB24

m/z	Abundance
44.00	263.0
65.10	142.0
75.90	136.0
104.00	147.0
105.00	200.0
121.10	120.0
149.10	1056.0
150.10	119.0
177.20	236.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24

m/z	Abundance
36.00	1169.0
37.00	5537.0
38.00	5610.0
39.10	2256.0
44.00	956.0
45.10	1262.0
46.30	152.0
47.10	1956.0
48.00	901.0
49.00	5633.0
50.10	26320.0
51.10	8257.0
52.10	530.0
55.10	284.0
56.10	1831.0
57.10	3653.0
58.00	193.0
60.00	1322.0
61.10	6394.0
62.10	7452.0
63.10	5194.0
64.00	564.0
65.10	807.0
66.00	100.0
67.10	426.0
68.10	14530.0
69.10	15205.0
70.10	1052.0
72.10	712.0
73.10	6721.0
74.10	25344.0
75.10	76000.0
76.10	6770.0
77.00	1036.0
78.10	647.0
79.00	4044.0
80.00	1321.0
81.00	3788.0
82.00	838.0
83.00	106.0
85.90	181.0
87.00	6971.0
88.10	6253.0
91.00	527.0
92.10	4024.0
93.10	6395.0
94.10	17776.0
95.10	152896.0
96.10	9587.0
97.10	243.0
104.00	947.0
104.90	235.0
106.00	466.0
107.00	101.0
110.90	124.0
113.00	152.0
116.00	475.0
117.00	1081.0
118.00	497.0
119.00	559.0
124.00	140.0
128.00	464.0
129.00	302.0
130.00	464.0
131.10	191.0
135.00	263.0
137.00	314.0
141.10	1283.0
142.10	161.0
143.00	1696.0
145.00	313.0
146.00	138.0
147.90	400.0
149.20	1336.0
149.90	203.0
152.00	115.0
153.10	107.0
155.10	368.0
157.10	285.0
159.00	117.0
161.00	129.0
171.10	139.0
172.10	949.0
173.20	1470.0
174.10	118840.0
175.10	8409.0
176.10	114960.0
177.10	7423.0
178.00	282.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24

m/z	Abundance
36.00	1126.0
37.00	5648.0
38.00	5549.0
39.00	2412.0
44.10	864.0
45.00	1077.0
47.10	2001.0
48.00	883.0
49.00	5576.0
50.10	26128.0
51.10	8327.0
52.00	368.0
55.10	323.0
56.00	2129.0
57.10	3586.0
58.00	149.0
60.00	1404.0
61.10	6451.0
62.10	7057.0
63.10	5123.0
64.00	662.0
65.10	792.0
66.00	111.0
67.10	442.0
68.10	14177.0
69.10	14555.0
70.10	1027.0
72.10	833.0
73.10	6659.0
74.10	24464.0
75.10	73216.0
76.10	6782.0
77.00	869.0
78.10	539.0
79.00	3886.0
80.00	1067.0
81.00	3936.0
82.00	846.0
86.00	205.0
87.00	6475.0
88.10	5882.0
91.00	554.0
92.10	4115.0
93.10	6398.0
94.10	16332.0
95.10	147456.0
96.10	9262.0
97.10	340.0
104.10	881.0
104.90	277.0
106.00	599.0
111.00	111.0
114.90	109.0
116.00	437.0
117.00	1106.0
117.90	442.0
119.00	723.0
128.00	433.0
129.00	229.0
130.00	452.0
131.10	189.0
135.00	272.0
137.00	247.0
141.10	1442.0
142.10	189.0
143.00	1566.0
145.00	326.0
146.00	152.0
147.00	123.0
148.00	355.0
149.20	1169.0
150.00	225.0
155.00	286.0
157.10	283.0
158.90	107.0
161.20	149.0
171.10	134.0
172.10	1005.0
174.10	109488.0
175.10	8204.0
176.10	104968.0
177.10	6972.0
178.20	260.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24

m/z	Abundance
36.00	1173.0
37.00	5920.0
38.00	5903.0
39.10	2438.0
44.10	926.0
45.00	1202.0
46.30	153.0
47.10	2067.0
48.00	928.0
49.00	5899.0
50.10	27672.0
51.10	8678.0
52.10	428.0
55.10	314.0
56.00	2131.0
57.10	3740.0
58.00	168.0
60.00	1389.0
61.10	6760.0
62.10	7608.0
63.10	5335.0
64.00	652.0
65.10	848.0
66.00	110.0
67.10	451.0
68.10	15276.0
69.10	15620.0
70.10	1113.0
72.10	798.0
73.10	7070.0
74.10	26488.0
75.10	78816.0
76.10	7002.0
77.00	948.0
78.10	647.0
79.00	4148.0
80.00	1245.0
81.00	4062.0
82.00	848.0
83.10	119.0
86.00	201.0
87.00	7196.0
88.10	6328.0
91.00	578.0
92.10	4345.0
93.10	6573.0
94.10	18064.0
95.10	158144.0
96.10	9776.0
97.10	305.0
104.00	949.0
104.90	279.0
106.00	572.0
110.90	116.0
113.00	115.0
116.00	480.0
117.00	1151.0
117.90	468.0
119.00	622.0
124.00	137.0
128.00	451.0
129.00	257.0
130.00	506.0
131.10	195.0
135.00	285.0
137.10	310.0
141.10	1445.0
142.10	184.0
143.00	1729.0
145.00	329.0
146.00	144.0
147.00	116.0
148.00	434.0
149.20	1267.0
149.90	217.0
152.00	100.0
153.10	112.0
155.10	329.0
157.10	320.0
159.00	122.0
161.10	135.0
171.10	145.0
172.10	1047.0
174.10	120016.0
175.10	8722.0
176.10	115616.0
177.10	7473.0
178.10	287.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24