


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121421\
 Data File : VU046345.D
 Acq On : 14 Dec 2021 10:44
 Operator : SY/MD
 Sample : BFB031
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis
 Last Update : Mon Dec 20 00:25:10 2021

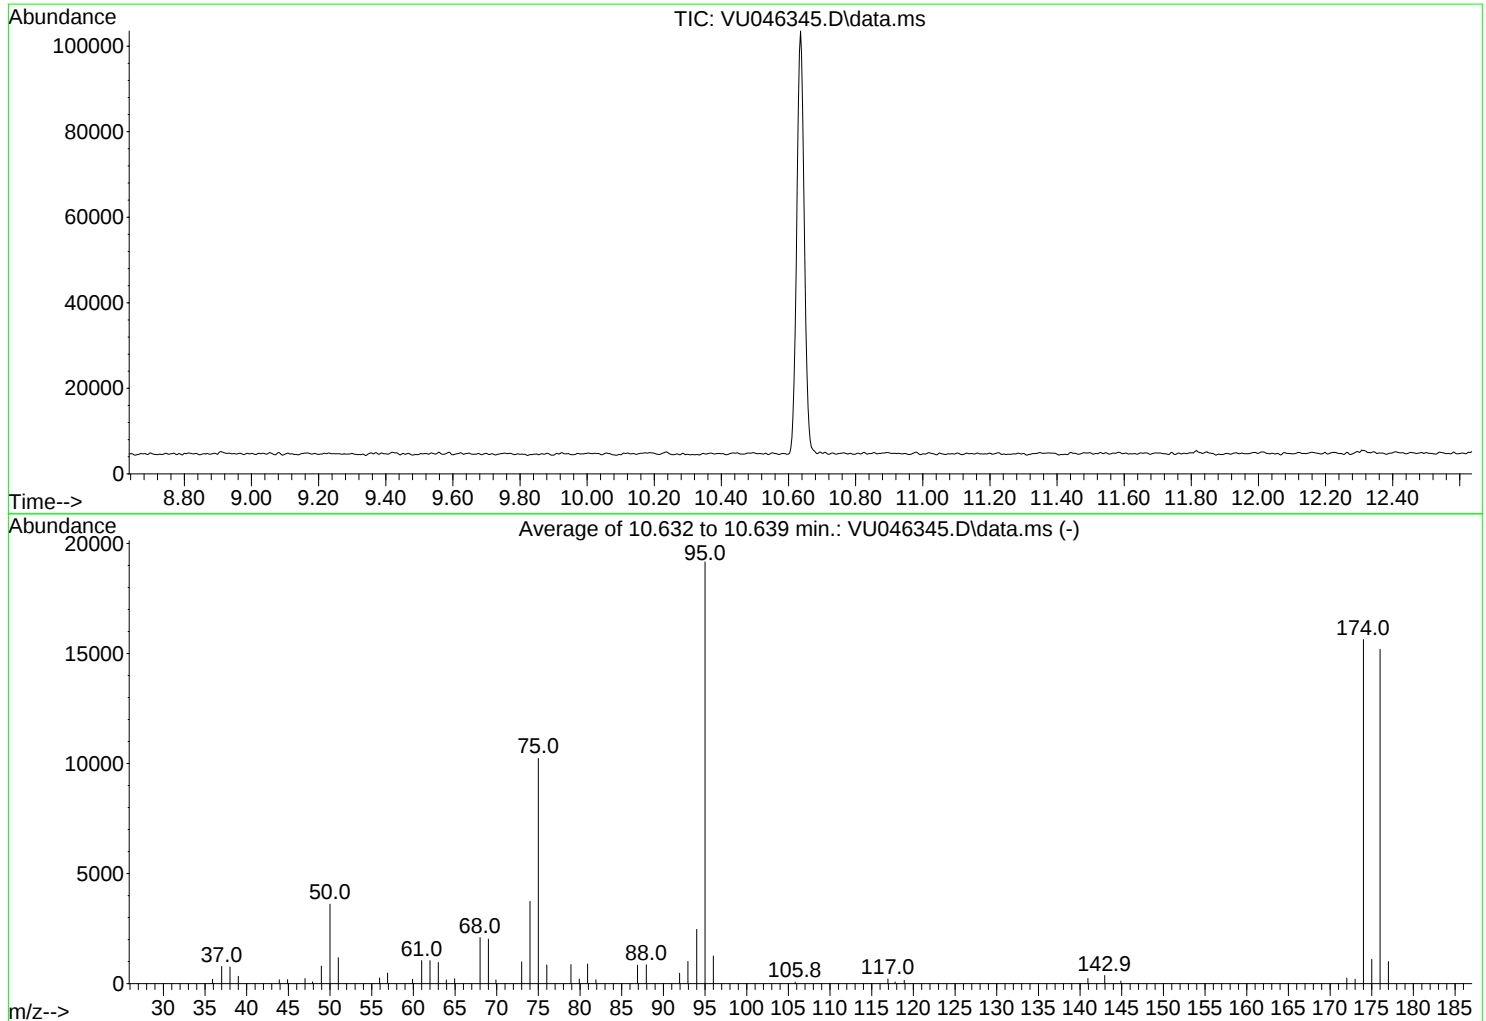

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	3610	PASS
75	95	30	80	53.4	10238	PASS
95	95	100	100	100.0	19163	PASS
96	95	5	9	6.6	1256	PASS
173	174	0.00	2	1.3	205	PASS
174	95	50	120	81.6	15629	PASS
175	174	5	9	7.0	1096	PASS
176	174	95	101	97.2	15187	PASS
177	176	5	9	6.6	1004	PASS

Scan 2879 (10.597 min): VU046345.D\data.ms
BFB031

m/z	Abundance
39.90	4418.0
43.90	183.0

Scan 2890 (10.632 min): VU046345.D\data.ms
BFB031

m/z	Abundance
35.90	186.0
37.00	820.0
38.00	752.0
39.00	296.0
40.00	4444.0
43.90	299.0
44.90	168.0
47.00	262.0
47.90	119.0
49.00	821.0
50.00	3718.0
51.00	1158.0
56.00	265.0
56.90	489.0
59.90	184.0
61.00	1048.0
62.00	1099.0
63.00	878.0
64.00	148.0
64.90	236.0
68.00	1996.0
69.00	2054.0
69.90	171.0
73.00	929.0
74.00	3621.0
75.00	10122.0
76.00	883.0
78.90	854.0
79.90	198.0
80.90	908.0
81.90	182.0
86.90	741.0
88.00	836.0
91.90	481.0
93.00	1002.0
94.00	2404.0
95.00	18952.0
96.00	1304.0
117.00	197.0
117.80	120.0
118.90	154.0
141.00	233.0
143.00	386.0
144.80	135.0
172.00	240.0
173.00	216.0
174.00	15078.0
175.00	1051.0
176.00	14770.0
177.00	946.0

Scan 2891 (10.636 min): VU046345.D\data.ms
BFB031

m/z	Abundance
35.90	214.0
37.00	800.0
38.00	784.0
39.00	323.0
40.00	4278.0
44.00	379.0
44.90	181.0
47.00	246.0
47.90	117.0
49.00	829.0
50.00	3741.0
51.00	1224.0
55.90	264.0
56.90	490.0
59.90	205.0
61.00	1083.0
62.00	1063.0
63.00	985.0
63.90	164.0
65.00	239.0
68.00	2168.0
69.00	2076.0
69.90	186.0
73.00	1020.0
74.00	3880.0
75.00	10588.0
76.00	885.0
78.90	895.0
79.90	208.0
80.90	904.0
81.90	175.0
86.90	873.0
87.90	888.0
91.90	493.0
92.90	1049.0
94.00	2586.0
95.00	19872.0
96.00	1283.0
105.80	106.0
116.90	211.0
117.80	111.0
118.90	162.0
140.90	249.0
143.00	389.0
144.90	113.0
172.00	253.0
173.00	206.0
174.00	16173.0
175.00	1138.0
176.00	15715.0
177.00	1052.0

m/z	Abundance
35.00	191.0
37.00	718.0
38.00	741.0
39.00	375.0
40.00	4190.0
44.00	388.0
44.90	187.0
47.00	190.0
48.90	749.0
50.00	3370.0
51.00	1160.0
55.90	251.0
56.90	460.0
59.90	197.0
61.00	1015.0
62.00	974.0
63.00	1016.0
63.90	188.0
65.00	212.0
68.00	2116.0
69.00	1932.0
69.90	151.0
73.00	1016.0
74.00	3719.0
75.00	10004.0
76.00	794.0
78.90	849.0
79.90	219.0
80.90	879.0
81.90	164.0
86.90	889.0
87.90	852.0
92.00	435.0
92.90	989.0
94.00	2400.0
95.00	18664.0
96.00	1182.0
105.80	121.0
116.90	218.0
118.90	144.0
140.90	245.0
142.90	328.0
145.00	100.0
172.00	273.0
173.00	194.0
174.00	15635.0
175.00	1098.0
176.00	15075.0
177.00	1014.0