

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU121422\  
 Data File : VU052400.D  
 Acq On : 14 Dec 2022 15:10  
 Operator : JC/MD  
 Sample : N6034-04  
 Misc : 25.0mL/MSVOA\_U/WATER  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 BGPL2

Quant Time: Dec 14 21:39:55 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR111822WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Wed Dec 14 21:38:14 2022  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon  | Response | Conc     | Units | Dev(Min) |
|-------------------------------|--------|-------|----------|----------|-------|----------|
| -----                         |        |       |          |          |       |          |
| Internal Standards            |        |       |          |          |       |          |
| 1) 1,4-Difluorobenzene        | 6.247  | 114   | 249019   | 5.000    | ug/L  | 0.00     |
| 28) Chlorobenzene-d5          | 9.414  | 117   | 258415   | 5.000    | ug/L  | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.809 | 152   | 111142   | 5.000    | ug/L  | 0.00     |
|                               |        |       |          |          |       |          |
| System Monitoring Compounds   |        |       |          |          |       |          |
| 4) Vinyl Chloride-d3          | 1.600  | 65    | 75829    | 3.131    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 40 - 130 | Recovery | =     | 62.600%  |
| 7) Chloroethane-d5            | 1.915  | 69    | 72514    | 3.854    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 65 - 130 | Recovery | =     | 77.000%  |
| 11) 1,1-Dichloroethene-d2     | 2.568  | 65    | 31674    | 3.648    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 60 - 125 | Recovery | =     | 73.000%  |
| 20) 2-Butanone-d5             | 4.639  | 46    | 258052   | 58.774   | ug/L  | 0.00     |
| Spiked Amount                 | 50.000 | Range | 40 - 130 | Recovery | =     | 117.540% |
| 24) Chloroform-d              | 5.060  | 84    | 168220   | 4.727    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =     | 94.600%  |
| 26) 1,2-Dichloroethane-d4     | 5.700  | 65    | 87757    | 4.882    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =     | 97.600%  |
| 32) Benzene-d6                | 5.726  | 84    | 328350   | 4.280    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =     | 85.600%  |
| 36) 1,2-Dichloropropane-d6    | 6.687  | 67    | 112782   | 4.750    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 60 - 140 | Recovery | =     | 95.000%  |
| 41) Toluene-d8                | 7.896  | 98    | 257934   | 3.716    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =     | 74.400%  |
| 43) trans-1,3-Dichloroprop... | 8.176  | 79    | 34570    | 3.996    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 55 - 130 | Recovery | =     | 80.000%  |
| 46) 2-Hexanone-d5             | 8.632  | 63    | 183019   | 49.915   | ug/L  | 0.00     |
| Spiked Amount                 | 50.000 | Range | 45 - 130 | Recovery | =     | 99.820%  |
| 56) 1,1,2,2-Tetrachloroeth... | 10.751 | 84    | 103175   | 5.012    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 65 - 120 | Recovery | =     | 100.200% |
| 66) 1,2-Dichlorobenzene-d4    | 12.188 | 152   | 105639   | 4.965    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 80 - 120 | Recovery | =     | 99.200%  |
|                               |        |       |          |          |       |          |
| Target Compounds              |        |       |          |          |       | Qvalue   |
| 13) Acetone                   | 2.655  | 43    | 57543    | 19.300   | ug/L  | 100      |
| -----                         |        |       |          |          |       |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU121422\  
Data File : VU052400.D  
Acq On : 14 Dec 2022 15:10  
Operator : JC/MD  
Sample : N6034-04  
Misc : 25.0mL/MSVOA\_U/WATER  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
BGPL2

Quant Time: Dec 14 21:39:55 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR111822WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Wed Dec 14 21:38:14 2022  
Response via : Initial Calibration

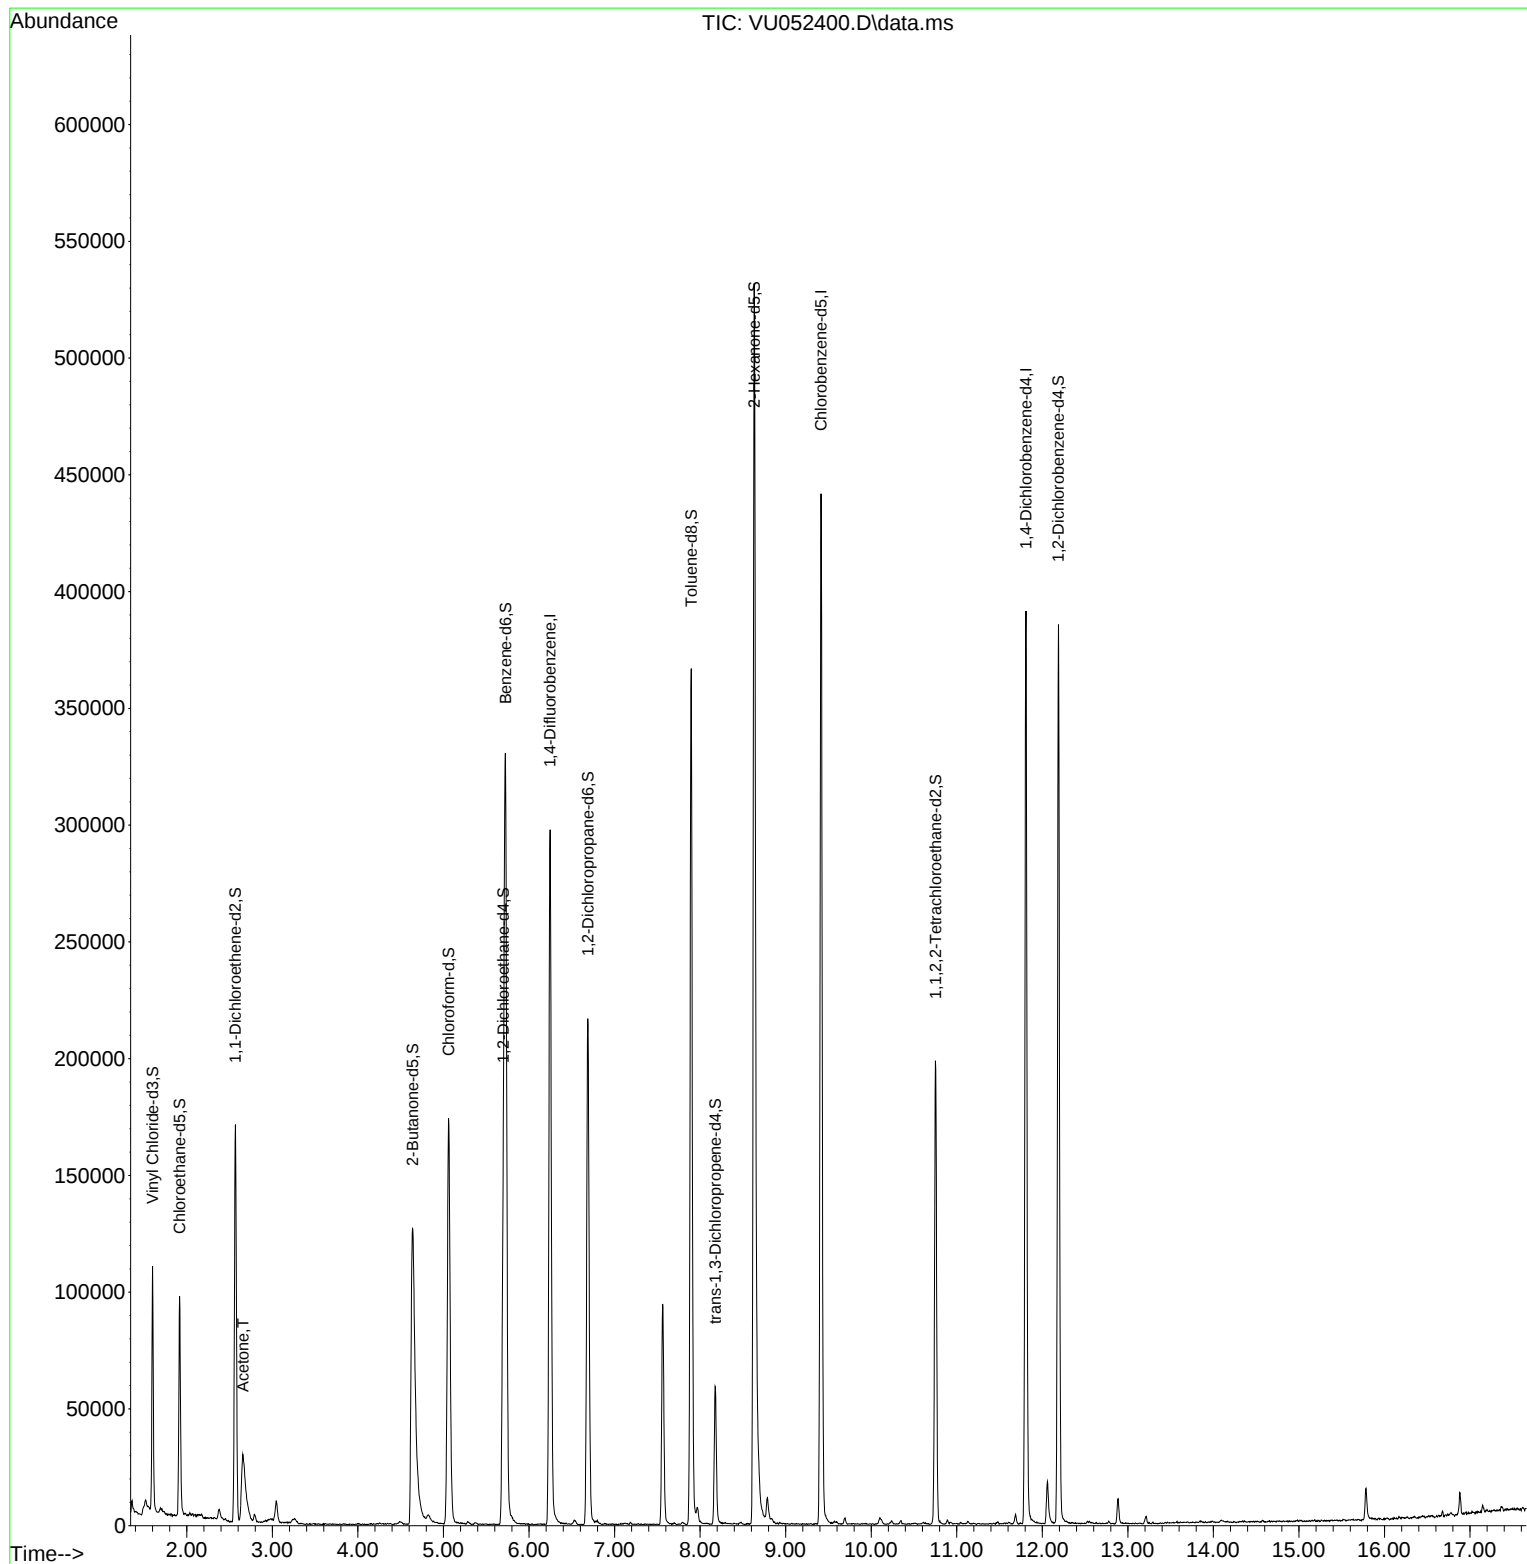

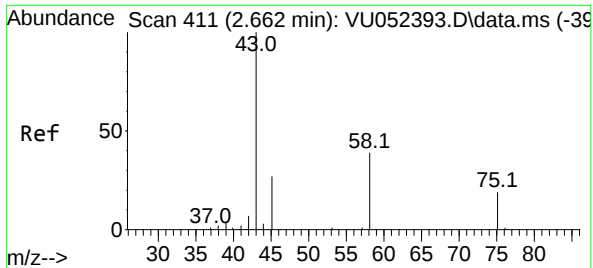

#13

Acetone

Concen: 19.300 ug/L

RT: 2.655 min Scan# 409

Delta R.T. -0.007 min

Lab File: VU052400.D

Acq: 14 Dec 2022 15:10

Instrument :

MSVOA\_U

ClientSampleId :

BGPL2

Tgt Ion: 43 Resp: 57543

Ion Ratio Lower Upper

43 100

58 37.8 0.0 76.0

