

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121422\
 Data File : VU052405.D
 Acq On : 14 Dec 2022 17:08
 Operator : JC/MD
 Sample : N6034-10
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGPK1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052405.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	95	rVB	94539	111868	11.69%	1.496%
2	1.916	170	179	194	rVB	83708	113615	11.87%	1.519%
3	2.568	370	382	398	rBV	149733	243903	25.49%	3.261%
4	3.366	613	630	648	rVB3	17531	41521	4.34%	0.555%
5	4.636	1011	1025	1069	rBV2	139179	500306	52.28%	6.690%
6	5.060	1140	1157	1181	rBV	152068	344232	35.97%	4.603%
7	5.722	1342	1363	1383	rBV2	288218	771648	80.64%	10.318%
8	6.247	1510	1526	1545	rBV	266764	511412	53.44%	6.838%
9	6.539	1602	1617	1642	rVB2	54804	106461	11.12%	1.423%
10	6.687	1649	1663	1693	rBV	193061	381390	39.85%	5.100%
11	7.562	1921	1935	1952	rBV	82009	145822	15.24%	1.950%
12	7.896	2020	2039	2064	rBV	311129	544077	56.85%	7.275%
13	8.179	2116	2127	2143	rBV	50741	86457	9.03%	1.156%
14	8.549	2229	2242	2257	rBV	339843	585577	61.19%	7.830%
15	8.632	2257	2268	2297	rVV2	483695	956964	100.00%	12.796%
16	9.414	2498	2511	2537	rBV	393316	663473	69.33%	8.871%
17	10.751	2913	2927	2947	rBV	182146	293220	30.64%	3.921%
18	11.809	3240	3256	3273	rBV	342553	554447	57.94%	7.413%
19	12.188	3362	3374	3391	rBV	316450	522517	54.60%	6.987%




Sum of corrected areas: 7478910

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121422\
Data File : VU052405.D
Acq On : 14 Dec 2022 17:08
Operator : JC/MD
Sample : N6034-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGPK1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

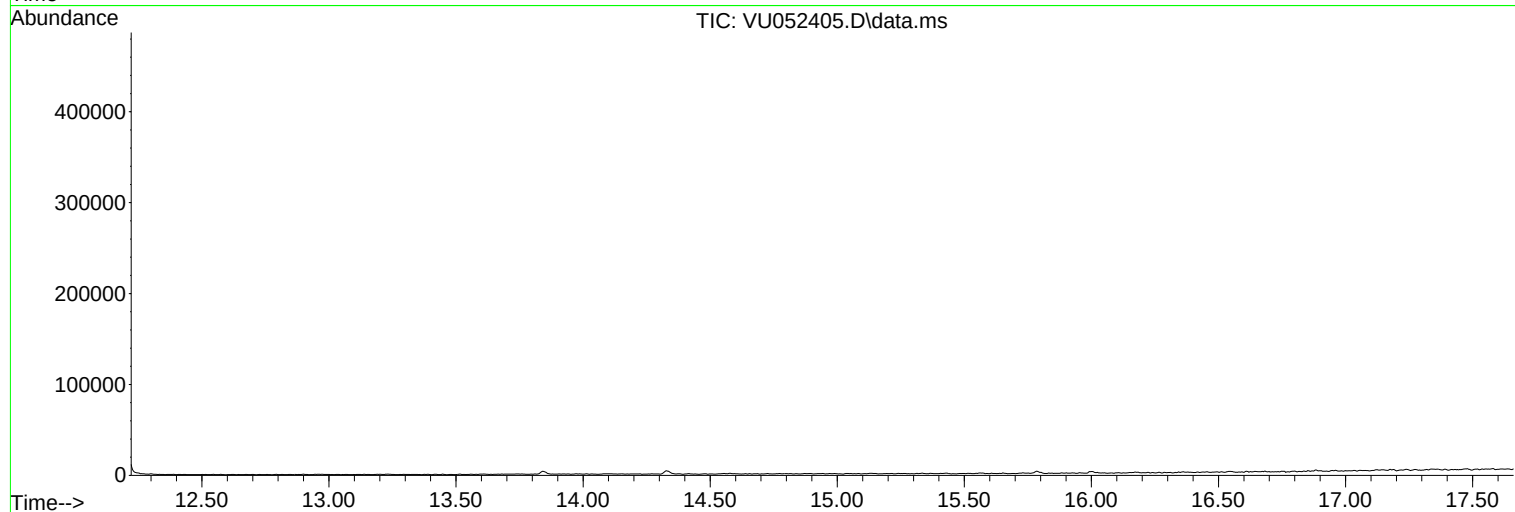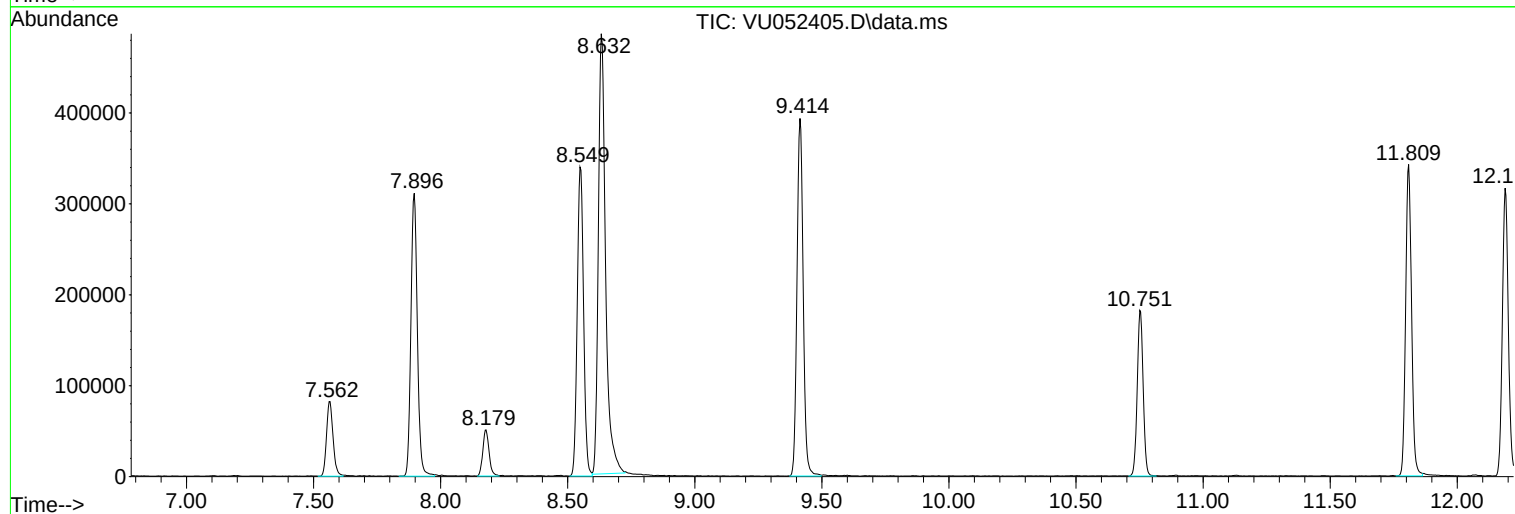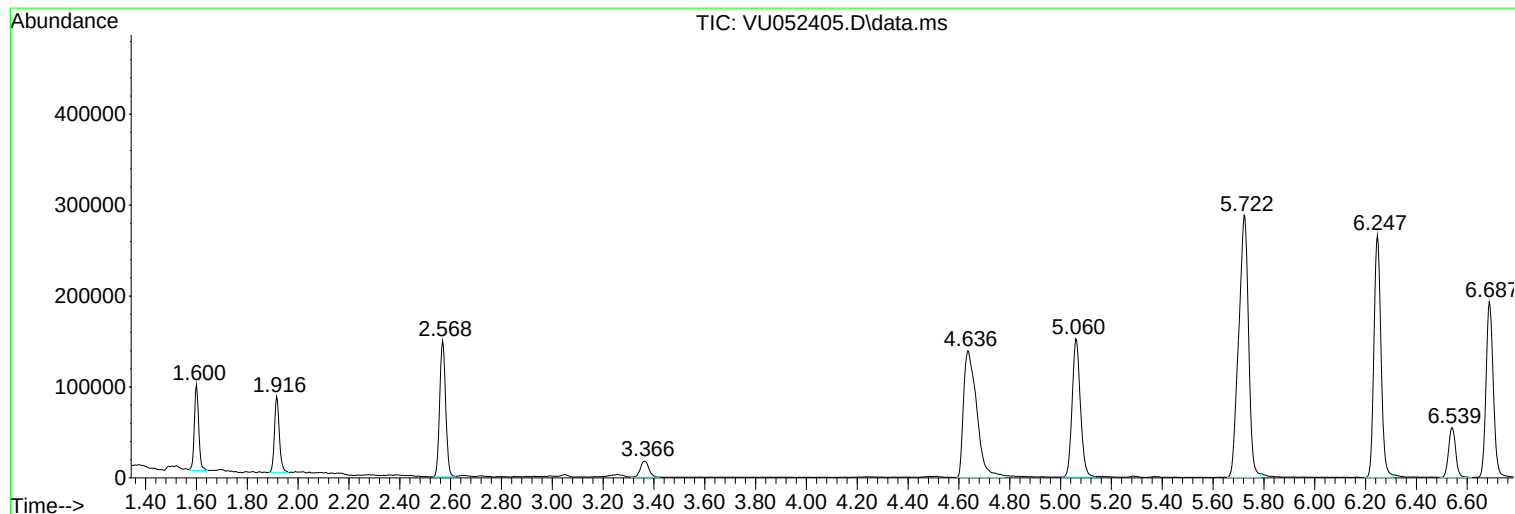

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121422\
Data File : VU052405.D
Acq On : 14 Dec 2022 17:08
Operator : JC/MD
Sample : N6034-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGPK1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121422\
Data File : VU052405.D
Acq On : 14 Dec 2022 17:08
Operator : JC/MD
Sample : N6034-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGPK1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc