


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121422\
 Data File : VU052392.D
 Acq On : 14 Dec 2022 10:19
 Operator : JC/MD
 Sample : BFB179
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB179

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Dec 14 21:38:14 2022

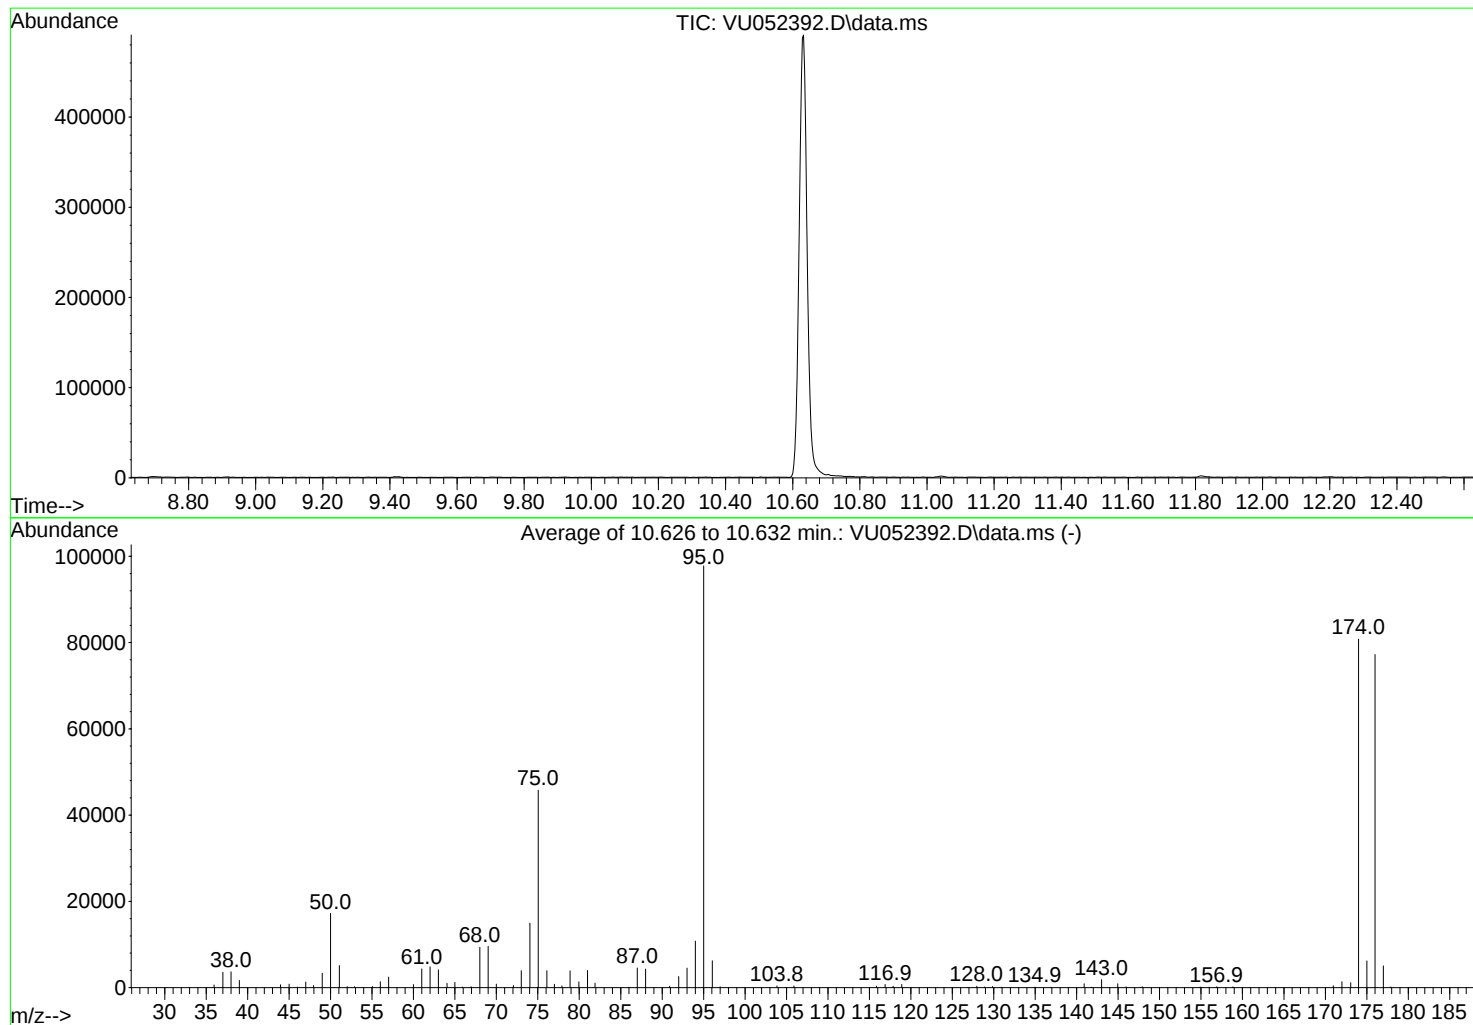

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	17206	PASS
75	95	30	80	46.8	45781	PASS
95	95	100	100	100.0	97792	PASS
96	95	5	9	6.4	6234	PASS
173	174	0.00	2	1.4	1171	PASS
174	95	50	120	82.6	80797	PASS
175	174	5	9	7.7	6187	PASS
176	174	95	101	95.6	77216	PASS
177	176	5	9	6.5	5035	PASS

Scan 2875 (10.584 min): VU052392.D\data.ms
BFB179

m/z	Abundance
39.90	344.0
43.90	393.0

Instrument :
MSVOA_U
ClientSampleId :
BFB179

m/z	Abundance
36.00	688.0
37.00	3435.0
38.00	3601.0
39.00	1605.0
39.90	279.0
44.00	957.0
45.00	806.0
46.00	167.0
47.00	1227.0
47.90	452.0
49.00	3159.0
50.00	16201.0
51.00	4831.0
52.00	191.0
52.90	194.0
55.10	287.0
56.00	1378.0
57.00	2164.0
60.00	729.0
61.00	4164.0
62.00	4426.0
63.00	3812.0
64.00	899.0
65.00	1267.0
65.90	123.0
66.90	194.0
68.00	9011.0
69.00	8987.0
70.00	751.0
72.00	487.0
73.00	3713.0
74.00	14357.0
75.10	43720.0
76.10	3813.0
77.00	673.0
77.90	439.0
78.90	3875.0
79.90	1204.0
81.00	3596.0
81.90	1005.0
85.90	117.0
87.00	4258.0
88.00	3904.0
90.90	327.0
92.00	2479.0
93.00	4214.0
94.00	9913.0
95.00	91600.0
96.10	5771.0
97.00	186.0
103.80	373.0
105.90	377.0
115.90	374.0
116.90	636.0
117.90	344.0
118.90	692.0
128.00	333.0
128.90	131.0
129.90	257.0
130.90	110.0
135.00	131.0
136.90	139.0
140.90	824.0
141.70	109.0
143.00	1814.0
144.90	918.0
145.90	208.0
147.90	202.0
154.90	211.0
156.00	134.0
156.90	192.0
158.90	133.0
160.90	105.0
170.90	389.0
172.00	1203.0
173.00	1050.0
174.00	74120.0
175.00	5556.0
176.00	71440.0
177.00	4544.0
177.90	155.0

Instrument :
MSVOA_U
ClientSampleId :
BFB179

m/z	Abundance
35.90	649.0
37.00	3719.0
38.00	3782.0
39.00	1690.0
39.90	256.0
44.00	1083.0
45.00	848.0
46.00	156.0
47.00	1336.0
48.00	479.0
49.00	3423.0
50.00	17808.0
51.10	5298.0
52.00	243.0
52.90	225.0
54.00	113.0
55.10	274.0
56.00	1435.0
57.00	2567.0
60.00	701.0
61.00	4412.0
62.00	5008.0
63.00	4288.0
64.00	1012.0
65.00	1251.0
65.90	148.0
67.00	213.0
68.00	9704.0
69.00	9777.0
70.00	872.0
72.10	522.0
73.00	4003.0
74.00	15317.0
75.10	46880.0
76.10	4073.0
77.00	812.0
77.90	432.0
78.90	3979.0
80.00	1342.0
81.00	4106.0
81.90	1079.0
85.90	124.0
87.00	4634.0
88.00	4401.0
90.90	319.0
92.00	2657.0
93.00	4725.0
94.00	11150.0
95.00	101064.0
96.10	6494.0
97.00	206.0
103.80	410.0
104.90	103.0
105.90	419.0
115.80	343.0
116.90	772.0
117.80	350.0
118.90	782.0
128.00	350.0
128.90	148.0
129.80	251.0
130.90	135.0
134.90	122.0
136.90	131.0
140.90	918.0
141.70	115.0
143.00	1887.0
144.90	910.0
145.90	192.0
147.90	220.0
154.90	237.0
156.00	132.0
156.90	241.0
158.90	177.0
170.90	446.0
172.00	1412.0
173.00	1238.0
174.00	83016.0
175.00	6440.0
176.00	79344.0
177.00	5117.0
177.90	140.0

Instrument :
MSVOA_U
ClientSampleId :
BFB179

m/z	Abundance
36.00	616.0
37.00	3580.0
38.00	3584.0
39.00	1674.0
40.00	262.0
44.00	1141.0
45.00	808.0
46.00	146.0
47.00	1389.0
48.00	494.0
49.00	3491.0
50.00	17608.0
51.10	5263.0
52.00	278.0
52.90	214.0
54.00	136.0
55.00	203.0
56.00	1311.0
57.00	2666.0
60.00	722.0
61.00	4472.0
62.00	5043.0
63.00	4305.0
64.10	1069.0
65.00	1123.0
65.90	180.0
66.90	237.0
68.00	9347.0
69.00	9913.0
70.00	869.0
72.10	469.0
73.00	4060.0
74.10	15220.0
75.00	46744.0
76.10	3918.0
77.00	827.0
77.90	326.0
78.90	3847.0
79.90	1450.0
81.00	4158.0
81.90	1078.0
86.10	132.0
87.00	4815.0
88.00	4563.0
90.90	348.0
92.00	2574.0
93.00	4692.0
94.00	11286.0
95.00	100712.0
96.00	6437.0
97.00	192.0
103.90	440.0
104.80	119.0
105.90	414.0
115.80	322.0
116.90	820.0
117.80	330.0
118.90	747.0
126.90	111.0
127.90	340.0
128.90	163.0
129.80	305.0
130.90	142.0
134.90	113.0
136.90	102.0
140.90	906.0
141.80	114.0
143.00	1846.0
145.00	811.0
146.00	205.0
147.90	226.0
155.10	258.0
155.90	125.0
156.90	213.0
158.80	222.0
171.00	477.0
172.00	1570.0
173.10	1224.0
174.00	85256.0
175.00	6564.0
176.00	80864.0
177.00	5445.0
177.90	127.0

Instrument :
MSVOA_U
ClientSampleId :
BFB179