

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU121520\
 Data File : VU041642.D
 Acq On : 15 Dec 2020 17:32
 Operator : SY/MD
 Sample : L5029-04DL 250X
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GB1K4DL

Quant Time: Dec 16 05:49:33 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Dec 16 04:34:43 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	113962	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	115188	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	50418	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	28547	3.20	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	64.00%
7) Chloroethane-d5	1.92	69	31204	4.52	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.40%
11) 1,1-Dichloroethene-d2	2.58	63	49679	3.03	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	60.60%
20) 2-Butanone-d5	4.66	46	139988	54.70	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	109.40%
24) Chloroform-d	5.08	84	75338	4.94	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.80%
26) 1,2-Dichloroethane-d4	5.72	65	45153	5.21	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.20%
32) Benzene-d6	5.74	84	147269	4.47	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.40%
36) 1,2-Dichloropropane-d6	6.70	67	47778	4.62	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.40%
41) Toluene-d8	7.90	98	122955	4.13	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.60%
43) trans-1,3-Dichloropropene-	8.18	79	19311	4.15	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.00%
46) 2-Hexanone-d5	8.64	63	110484	43.46	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.92%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	48393	5.15	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.00%
64) 1,2-Dichlorobenzene-d4	12.19	152	49036	5.47	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	109.40%


Target Compounds					Ovalue
47) Tetrachloroethene	8.56	164	45234	6.980 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU121520\
Data File : VU041642.D
Acq On : 15 Dec 2020 17:32
Operator : SY/MD
Sample : L5029-04DL 250X
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB1K4DL

Quant Time: Dec 16 05:49:33 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Dec 16 04:34:43 2020
Response via : Initial Calibration

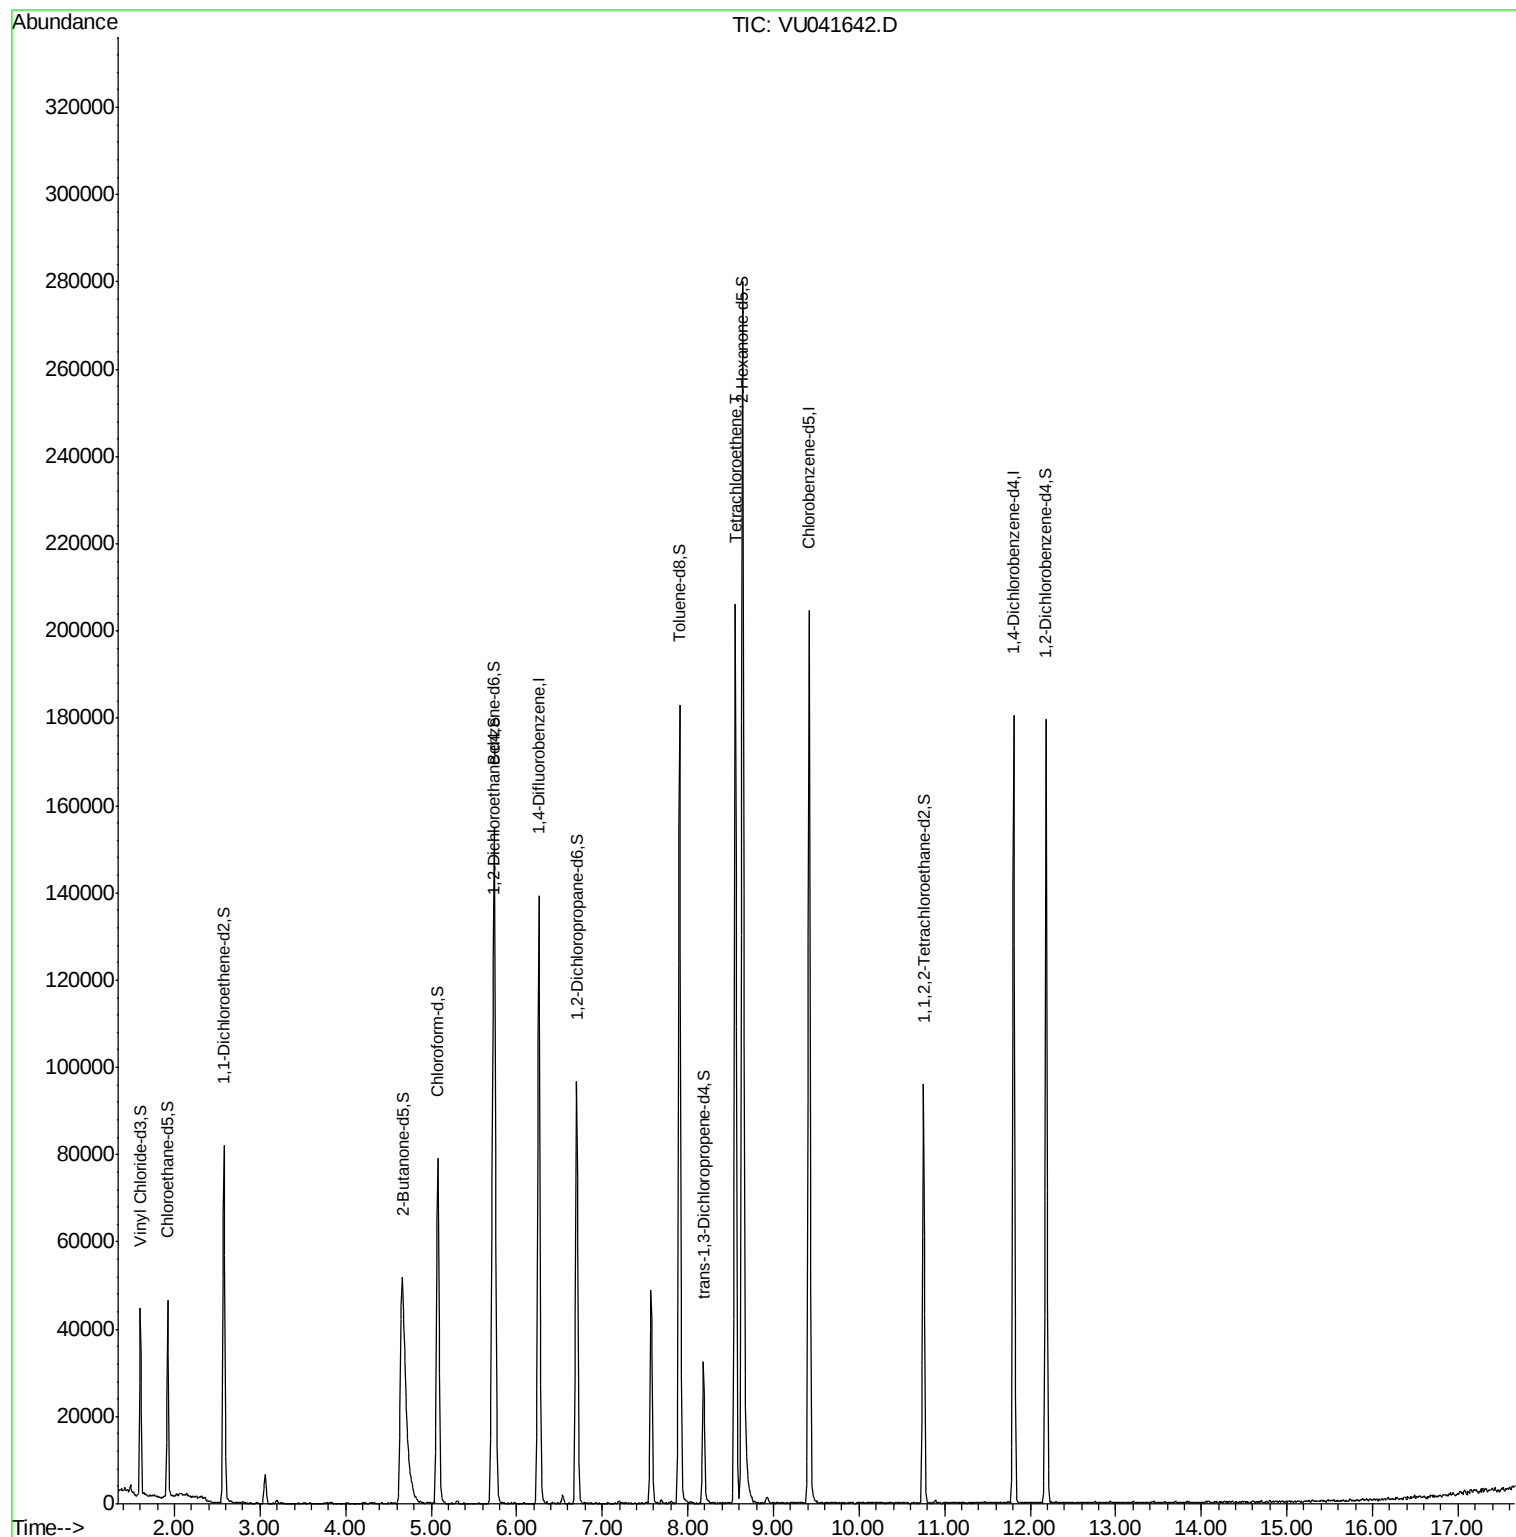

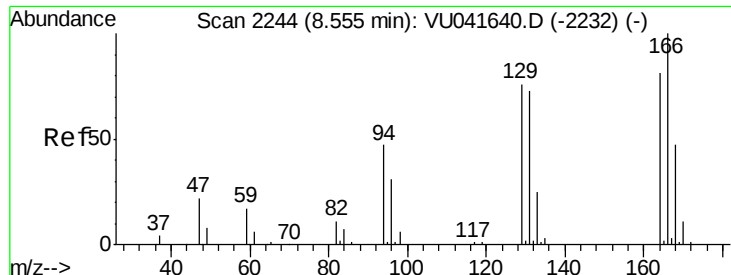

#47

Tetrachloroethene

Concen: 6.980 ug/L

RT: 8.56 min Scan# 2244

Delta R.T. 0.00 min

Lab File: VU041642.D


Acq: 15 Dec 2020 17:32

Instrument :

MSVOA_U

ClientSampleId :

GB1K4DL

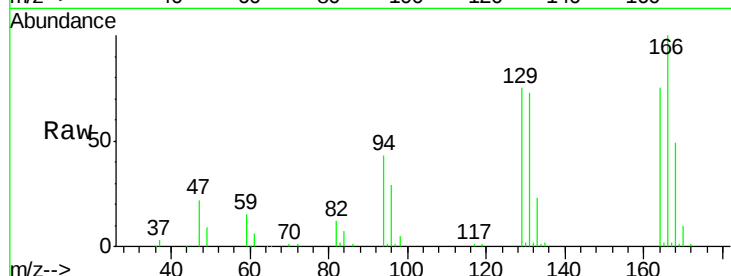

Tot Ion:164 Resp: 45234

Ion Ratio Lower Upper

164 100

129 100.2 72.2 134.0

131 97.2 66.9 124.3

166 133.6 89.6 166.4

Abundance Ion 163.90 (163.60 to 164.60): V

Ion 128.95 (128.65 to 129.65): V

Ion 130.95 (130.65 to 131.65): V

Ion 165.90 (165.60 to 166.60): V

