


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU121520\
 Data File : VU041625.D
 Acq On : 15 Dec 2020 09:00
 Operator : SY/MD
 Sample : BFB25
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB25

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Dec 16 04:34:43 2020

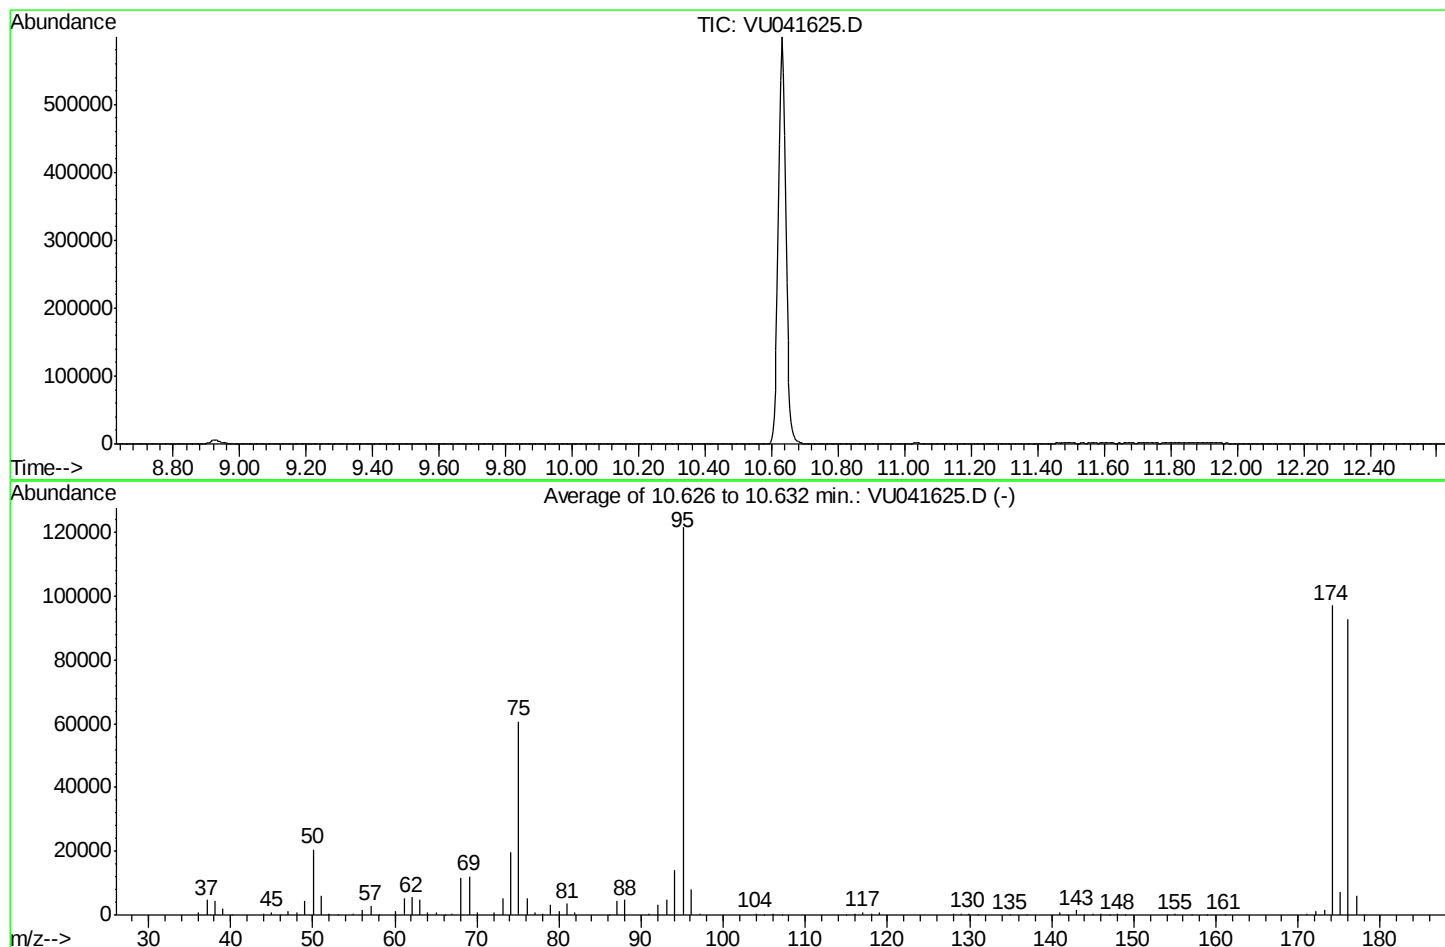

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	20658	PASS
75	95	30	80	50.0	60824	PASS
95	95	100	100	100.0	121629	PASS
96	95	5	9	6.5	7910	PASS
173	174	0.00	2	1.6	1587	PASS
174	95	50	120	79.8	97077	PASS
175	174	5	9	7.3	7115	PASS
176	174	95	101	95.6	92802	PASS
177	176	5	9	6.6	6079	PASS

m/z	Abundance
36.10	879.0
37.10	4393.0
38.00	4041.0
39.00	1784.0
40.10	175.0
44.00	569.0
45.00	955.0
46.10	209.0
47.00	1167.0
48.00	670.0
49.00	4305.0
50.10	19800.0
51.10	5732.0
52.00	269.0
53.10	125.0
55.00	254.0
56.10	1517.0
57.10	2940.0
58.10	154.0
60.10	1065.0
61.10	5009.0
62.10	5196.0
63.10	4682.0
64.00	705.0
65.10	893.0
66.20	123.0
67.00	390.0
68.10	10578.0
69.10	11594.0
70.00	771.0
72.00	566.0
73.10	5112.0
74.10	18280.0
75.10	56352.0
76.10	5209.0
77.10	761.0
78.00	526.0
79.00	3269.0
80.00	1118.0
81.00	3382.0
81.90	841.0
86.10	200.0
87.00	4447.0
88.10	4421.0
91.00	467.0
92.10	3196.0
93.10	4665.0
94.10	12933.0
95.10	115624.0
96.10	7475.0
97.20	192.0
104.00	491.0
104.90	174.0
106.00	483.0
107.10	102.0
116.00	410.0
117.00	778.0
118.00	329.0
119.00	828.0
128.00	372.0
129.00	168.0
129.90	358.0
131.00	160.0
134.90	148.0
136.90	100.0
141.10	920.0
143.10	1380.0
144.00	115.0
145.10	421.0
146.00	234.0
148.00	258.0
155.00	301.0
157.00	139.0
158.90	179.0
161.00	153.0
171.00	198.0
172.10	1231.0
173.20	1443.0
174.10	87912.0
175.10	6457.0
176.10	84216.0
177.10	5494.0
178.10	143.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25

m/z	Abundance
36.10	1042.0
37.10	4826.0
38.10	4333.0
39.00	1971.0
40.10	163.0
44.00	594.0
45.00	975.0
46.10	224.0
47.10	1390.0
48.00	776.0
49.10	4790.0
50.10	21208.0
51.10	6333.0
52.00	315.0
53.00	126.0
55.00	280.0
56.10	1692.0
57.10	3094.0
58.00	169.0
60.00	1125.0
61.10	5372.0
62.10	5568.0
63.10	5033.0
64.00	719.0
65.10	953.0
66.10	141.0
67.00	405.0
68.10	11730.0
69.10	12544.0
70.00	815.0
72.10	654.0
73.10	5488.0
74.10	20600.0
75.10	62712.0
76.10	5342.0
77.10	817.0
78.00	597.0
79.00	3525.0
80.00	1146.0
81.00	3519.0
82.00	918.0
86.10	146.0
87.00	4705.0
88.10	4811.0
91.00	549.0
92.10	3453.0
93.10	5018.0
94.10	14321.0
95.10	125552.0
96.10	8128.0
97.10	214.0
104.00	527.0
104.90	178.0
106.00	499.0
116.00	442.0
117.00	861.0
118.10	367.0
119.00	821.0
128.00	412.0
129.00	245.0
129.90	437.0
131.00	169.0
134.90	198.0
136.90	131.0
141.00	1031.0
141.90	109.0
143.00	1547.0
144.00	107.0
145.10	416.0
146.00	233.0
147.00	103.0
148.00	328.0
149.00	104.0
154.00	122.0
155.10	315.0
157.10	158.0
159.00	204.0
161.00	155.0
171.00	238.0
172.10	1352.0
173.20	1643.0
174.10	100192.0
175.10	7422.0
176.10	95624.0
177.10	6274.0
178.00	155.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25

m/z	Abundance
36.10	1041.0
37.10	4760.0
38.10	4481.0
39.00	1984.0
40.10	162.0
44.00	627.0
45.00	854.0
46.10	200.0
47.10	1508.0
48.00	781.0
49.10	4703.0
50.10	20968.0
51.10	6406.0
52.00	307.0
52.90	117.0
55.00	304.0
56.00	1781.0
57.10	3003.0
58.00	150.0
60.00	1139.0
61.10	5430.0
62.10	5571.0
63.10	4931.0
64.00	707.0
65.10	1086.0
66.10	136.0
67.00	309.0
68.10	12190.0
69.10	12651.0
70.00	769.0
72.10	698.0
73.10	5606.0
74.10	20616.0
75.10	63408.0
76.10	5020.0
77.10	764.0
78.00	538.0
79.00	3379.0
80.00	1085.0
81.00	3511.0
82.00	886.0
86.00	106.0
87.00	4649.0
88.00	4870.0
91.00	539.0
92.10	3626.0
93.10	5083.0
94.10	14519.0
95.10	123712.0
96.10	8129.0
97.00	248.0
104.00	510.0
104.90	160.0
106.00	467.0
115.00	125.0
116.00	463.0
117.00	823.0
118.10	404.0
119.00	743.0
128.00	437.0
129.00	255.0
129.90	493.0
131.00	179.0
134.90	192.0
136.90	157.0
141.00	1046.0
142.00	110.0
143.00	1573.0
145.10	380.0
146.00	189.0
147.00	118.0
148.00	362.0
148.90	109.0
154.00	143.0
155.10	329.0
157.10	156.0
159.00	204.0
161.10	110.0
171.00	243.0
172.20	1357.0
173.20	1675.0
174.10	103128.0
175.10	7468.0
176.10	98568.0
177.10	6469.0
178.00	155.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25

m/z	Abundance
43.90	250.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25