

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121521\
 Data File : VU046389.D
 Acq On : 15 Dec 2021 11:59
 Operator : SY/MD
 Sample : VU1215WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK065

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046389.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	99	rBV	97558	116074	16.93%	2.234%
2	1.919	171	180	201	rBV	64159	93541	13.64%	1.800%
3	2.308	297	301	305	rBV	249	207	0.03%	0.004%
4	2.382	321	324	331	rBV2	187	273	0.04%	0.005%
5	2.430	335	339	341	rBV2	177	130	0.02%	0.003%
6	2.575	370	384	424	rVV	157595	263034	38.35%	5.062%
7	2.797	447	453	455	rBV	346	395	0.06%	0.008%
8	2.932	491	495	497	rBB	143	121	0.02%	0.002%
9	2.977	506	509	514	rBB	154	176	0.03%	0.003%
10	3.044	527	530	533	rBV2	361	306	0.04%	0.006%
11	3.060	533	535	540	rVB2	452	400	0.06%	0.008%
12	3.089	540	544	547	rBB	148	147	0.02%	0.003%
13	3.166	565	568	569	rBV	285	179	0.03%	0.003%
14	3.195	572	577	584	rVB2	719	1162	0.17%	0.022%
15	3.369	626	631	633	rBV	137	137	0.02%	0.003%
16	4.642	1012	1027	1062	rBV	48781	155204	22.63%	2.987%
17	4.813	1078	1080	1085	rVB	210	119	0.02%	0.002%
18	4.899	1104	1107	1112	rBB2	216	189	0.03%	0.004%
19	5.070	1143	1160	1181	rBV	124526	271906	39.65%	5.232%
20	5.215	1200	1205	1208	rBB	205	215	0.03%	0.004%
21	5.250	1212	1216	1219	rBV	179	206	0.03%	0.004%
22	5.729	1344	1365	1395	rBV2	254034	685795	100.00%	13.197%
23	5.832	1395	1397	1404	rVB2	238	188	0.03%	0.004%
24	6.253	1514	1528	1551	rBV	192489	358013	52.20%	6.889%
25	6.362	1560	1562	1567	rVB2	181	128	0.02%	0.002%
26	6.539	1611	1617	1620	rBV3	534	535	0.08%	0.010%
27	6.694	1652	1665	1685	rBV	155431	300587	43.83%	5.784%
28	6.816	1699	1703	1707	rBB	275	229	0.03%	0.004%
29	7.186	1815	1818	1825	rVB	306	323	0.05%	0.006%
30	7.568	1925	1937	1954	rBV	85098	149536	21.80%	2.878%
31	7.658	1963	1965	1969	rVB	222	134	0.02%	0.003%
32	7.687	1972	1974	1981	rBB2	322	261	0.04%	0.005%
33	7.903	2027	2041	2055	rBV	315923	546220	79.65%	10.511%
34	7.970	2058	2062	2072	rVB	3983	6347	0.93%	0.122%
35	8.095	2099	2101	2105	rBV	125	130	0.02%	0.003%
36	8.182	2116	2128	2140	rBV	60858	99775	14.55%	1.920%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121521\
 Data File : VU046389.D
 Acq On : 15 Dec 2021 11:59
 Operator : SY/MD
 Sample : VU1215WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK065

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	8.478	2212	2220	2221	rBV	439	488	0.07%	0.009%
38	8.636	2257	2269	2294	rBV	192544	327360	47.73%	6.299%
39	8.816	2322	2325	2329	rVV2	214	179	0.03%	0.003%
40	8.835	2329	2331	2337	rVB	168	189	0.03%	0.004%
41	8.912	2352	2355	2356	rBV	271	170	0.02%	0.003%
42	8.922	2356	2358	2361	rVB2	264	149	0.02%	0.003%
43	9.063	2395	2402	2405	rBB	149	202	0.03%	0.004%
44	9.169	2432	2435	2440	rBB	157	177	0.03%	0.003%
45	9.269	2463	2466	2469	rBV	125	135	0.02%	0.003%
46	9.288	2469	2472	2475	rVB	167	133	0.02%	0.003%
47	9.420	2499	2513	2533	rBV	290338	471714	68.78%	9.077%
48	9.652	2581	2585	2589	rBB	159	188	0.03%	0.004%
49	9.697	2594	2599	2604	rBB2	522	593	0.09%	0.011%
50	9.944	2673	2676	2678	rBV	137	119	0.02%	0.002%
51	10.028	2697	2702	2707	rBV	173	282	0.04%	0.005%
52	10.066	2711	2714	2716	rBV	136	118	0.02%	0.002%
53	10.140	2734	2737	2740	rBB	146	123	0.02%	0.002%
54	10.160	2740	2743	2747	rBB	183	169	0.02%	0.003%
55	10.195	2751	2754	2756	rBV	145	126	0.02%	0.002%
56	10.330	2793	2796	2800	rBB	143	141	0.02%	0.003%
57	10.353	2800	2803	2808	rBB	161	183	0.03%	0.004%
58	10.462	2833	2837	2842	rBB	137	161	0.02%	0.003%
59	10.494	2843	2847	2853	rBB	176	254	0.04%	0.005%
60	10.526	2855	2857	2861	rBB	145	122	0.02%	0.002%
61	10.562	2866	2868	2872	rBV	146	149	0.02%	0.003%
62	10.671	2895	2902	2913	rBV4	1472	2221	0.32%	0.043%
63	10.758	2917	2929	2948	rVB	215556	342162	49.89%	6.584%
64	10.867	2960	2963	2966	rVV2	311	201	0.03%	0.004%
65	10.902	2969	2974	2976	rVV2	331	283	0.04%	0.005%
66	11.034	3013	3015	3018	rBV	157	134	0.02%	0.003%
67	11.102	3030	3036	3038	rBB	143	144	0.02%	0.003%
68	11.121	3039	3042	3045	rBV	143	147	0.02%	0.003%
69	11.192	3061	3064	3067	rBV	136	140	0.02%	0.003%
70	11.256	3081	3084	3086	rBV	181	147	0.02%	0.003%
71	11.320	3101	3104	3106	rBV	167	136	0.02%	0.003%
72	11.455	3140	3146	3157	rBV4	912	1338	0.20%	0.026%
73	11.703	3216	3223	3225	rBV3	502	459	0.07%	0.009%
74	11.751	3231	3238	3240	rVB2	365	400	0.06%	0.008%
75	11.812	3244	3257	3275	rVV	313997	485715	70.83%	9.347%
76	11.944	3291	3298	3301	rBV2	444	457	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121521\
 Data File : VU046389.D
 Acq On : 15 Dec 2021 11:59
 Operator : SY/MD
 Sample : VU1215WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK065

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.976	3304	3308	3316	rVB3	871	891	0.13%	0.017%
78	12.025	3321	3323	3327	rBV	131	140	0.02%	0.003%
79	12.195	3364	3376	3391	rVV	316757	500302	72.95%	9.627%
80	12.275	3396	3401	3404	rBV	162	171	0.02%	0.003%
81	12.639	3510	3514	3518	rVB2	288	279	0.04%	0.005%
82	12.664	3518	3522	3524	rBV	170	164	0.02%	0.003%
83	12.774	3552	3556	3560	rBV	228	264	0.04%	0.005%
84	13.044	3637	3640	3647	rVB	121	132	0.02%	0.003%
85	13.838	3883	3887	3888	rBV2	319	199	0.03%	0.004%
86	14.092	3960	3966	3975	rBV	430	771	0.11%	0.015%
87	14.336	4038	4042	4048	rVB	425	470	0.07%	0.009%
88	14.581	4112	4118	4121	rBV2	241	256	0.04%	0.005%
89	15.436	4381	4384	4387	rBV	211	122	0.02%	0.002%
90	15.510	4403	4407	4415	rVB2	280	297	0.04%	0.006%
91	15.565	4421	4424	4428	rVV2	194	200	0.03%	0.004%
92	15.719	4470	4472	4476	rVB2	240	137	0.02%	0.003%
93	15.745	4476	4480	4482	rBV	163	158	0.02%	0.003%
94	15.764	4482	4486	4491	rVB	287	291	0.04%	0.006%
95	15.790	4491	4494	4498	rBV2	216	163	0.02%	0.003%
96	15.819	4499	4503	4505	rBV	266	208	0.03%	0.004%
97	15.877	4518	4521	4525	rBV	260	161	0.02%	0.003%
98	15.931	4535	4538	4543	rBV	219	175	0.03%	0.003%
99	16.487	4709	4711	4717	rBV2	239	209	0.03%	0.004%
100	16.610	4745	4749	4758	rVB2	353	428	0.06%	0.008%




Sum of corrected areas: 5196618

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121521\
Data File : VU046389.D
Acq On : 15 Dec 2021 11:59
Operator : SY/MD
Sample : VU1215WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK065

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

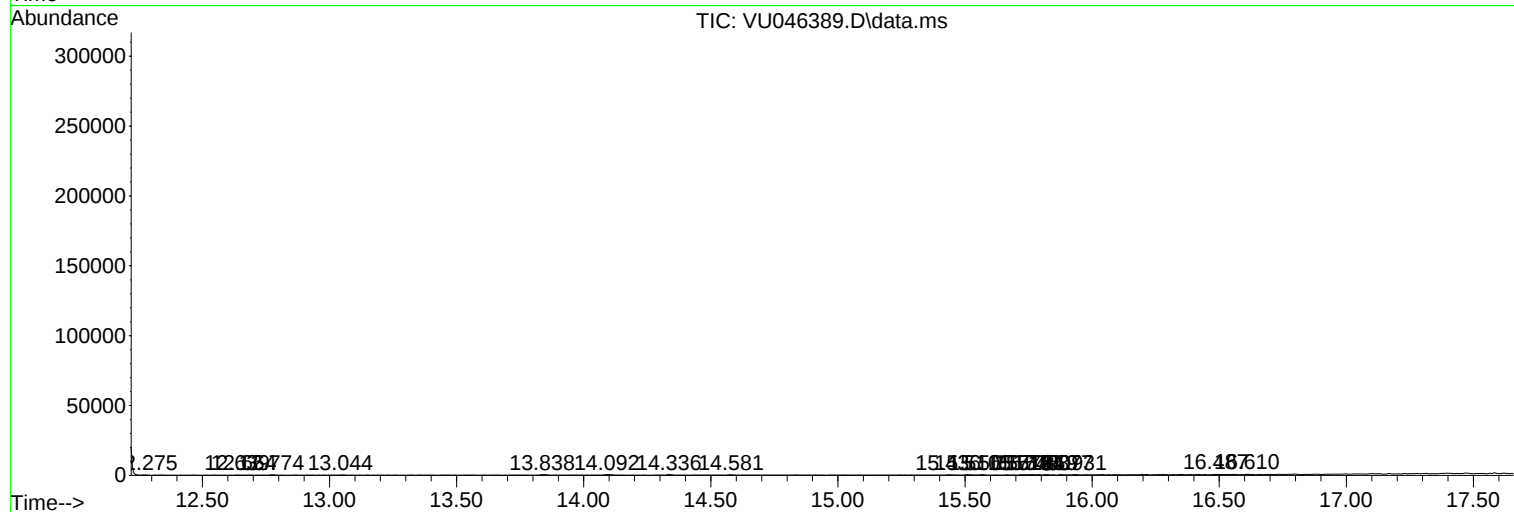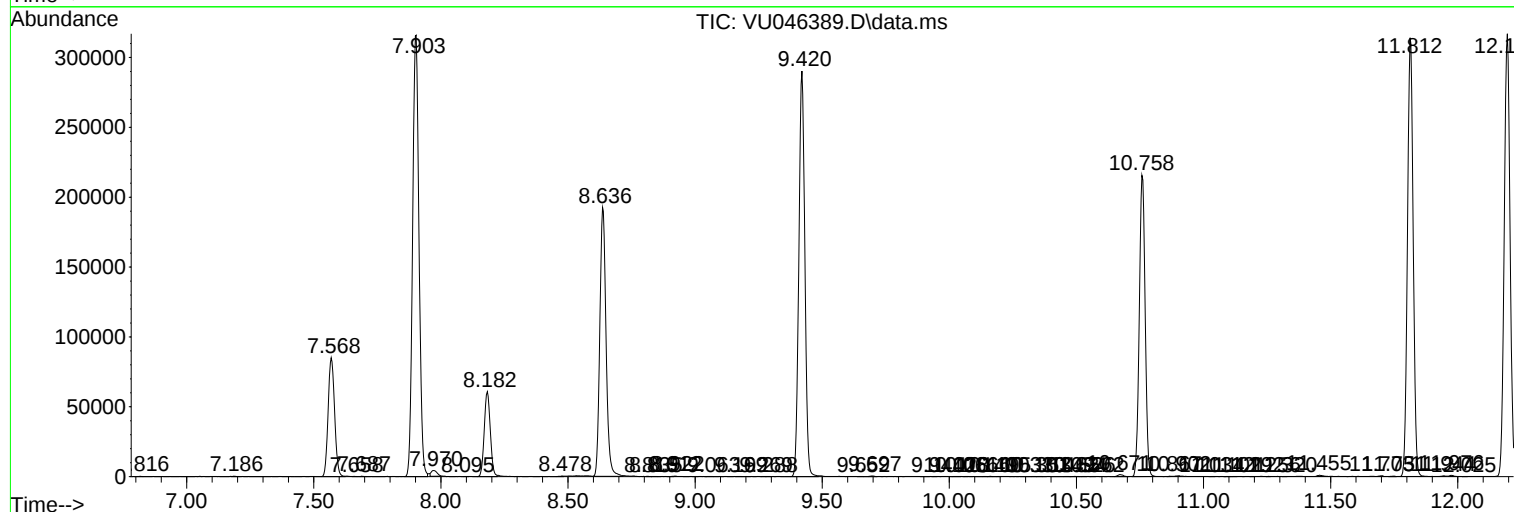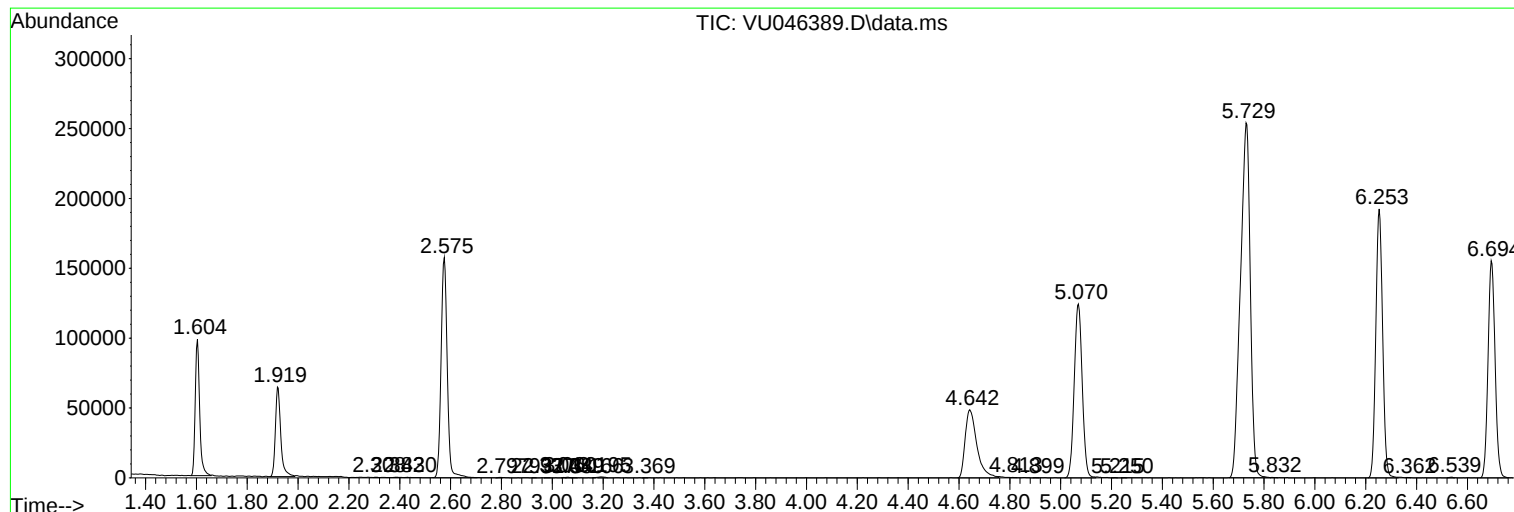

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121521\
Data File : VU046389.D
Acq On : 15 Dec 2021 11:59
Operator : SY/MD
Sample : VU1215WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK065

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121521\
Data File : VU046389.D
Acq On : 15 Dec 2021 11:59
Operator : SY/MD
Sample : VU1215WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK065

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc