

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121521\
 Data File : VU046397.D
 Acq On : 15 Dec 2021 15:07
 Operator : SY/MD
 Sample : VIBLK013
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK013

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046397.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	99	rBV	85094	100718	16.84%	2.148%
2	1.919	171	180	204	rBV	55260	77843	13.01%	1.660%
3	2.472	350	352	357	rVB	196	165	0.03%	0.004%
4	2.575	369	384	405	rBV	133748	222550	37.21%	4.746%
5	2.941	494	498	502	rBV	156	172	0.03%	0.004%
6	3.054	526	533	541	rVB3	922	1310	0.22%	0.028%
7	3.144	557	561	563	rBV	144	144	0.02%	0.003%
8	3.179	569	572	573	rBV2	217	124	0.02%	0.003%
9	3.456	655	658	660	rBV	140	115	0.02%	0.002%
10	3.517	674	677	681	rBV	143	167	0.03%	0.004%
11	3.572	692	694	698	rBB	130	119	0.02%	0.003%
12	3.883	780	791	799	rBB2	625	1301	0.22%	0.028%
13	3.954	810	813	816	rBB	166	126	0.02%	0.003%
14	4.144	868	872	874	rBB	163	139	0.02%	0.003%
15	4.446	964	966	969	rBV	133	117	0.02%	0.002%
16	4.636	1011	1025	1056	rBV2	49152	153024	25.58%	3.263%
17	4.793	1073	1074	1079	rVB	326	142	0.02%	0.003%
18	4.822	1081	1083	1088	rVB2	255	211	0.04%	0.004%
19	4.864	1094	1096	1098	rVB	245	136	0.02%	0.003%
20	5.067	1142	1159	1186	rBV	107915	237191	39.66%	5.058%
21	5.163	1186	1189	1191	rVV	205	145	0.02%	0.003%
22	5.179	1191	1194	1196	rVV	228	147	0.02%	0.003%
23	5.729	1344	1365	1392	rBV2	222761	598123	100.00%	12.756%
24	5.961	1434	1437	1440	rBB	139	117	0.02%	0.002%
25	6.250	1514	1527	1546	rBV	185121	350783	58.65%	7.481%
26	6.543	1612	1618	1625	rBB3	905	1112	0.19%	0.024%
27	6.694	1651	1665	1684	rBV	138890	264542	44.23%	5.642%
28	6.761	1684	1686	1690	rVB2	237	177	0.03%	0.004%
29	6.787	1691	1694	1697	rBB	139	117	0.02%	0.002%
30	6.803	1697	1699	1702	rBB	252	138	0.02%	0.003%
31	6.870	1716	1720	1722	rBV	130	138	0.02%	0.003%
32	7.047	1771	1775	1779	rBB	162	187	0.03%	0.004%
33	7.182	1814	1817	1822	rBV	201	230	0.04%	0.005%
34	7.372	1871	1876	1881	rBB	160	221	0.04%	0.005%
35	7.568	1924	1937	1950	rBV	73402	128810	21.54%	2.747%
36	7.694	1974	1976	1979	rBB	220	126	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121521\
 Data File : VU046397.D
 Acq On : 15 Dec 2021 15:07
 Operator : SY/MD
 Sample : VIBLK013
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK013

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	7.899	2027	2040	2056	rBV	277761	475303	79.47%	10.137%
38	7.970	2057	2062	2073	rVV2	3646	6160	1.03%	0.131%
39	8.015	2074	2076	2079	rVB	428	194	0.03%	0.004%
40	8.182	2116	2128	2144	rBV	52598	87458	14.62%	1.865%
41	8.298	2162	2164	2167	rVB	260	146	0.02%	0.003%
42	8.353	2178	2181	2183	rBV	231	157	0.03%	0.003%
43	8.382	2188	2190	2193	rBV	141	114	0.02%	0.002%
44	8.472	2211	2218	2220	rBV2	523	683	0.11%	0.015%
45	8.636	2257	2269	2293	rBV	173974	292686	48.93%	6.242%
46	8.809	2319	2323	2326	rBB	155	151	0.03%	0.003%
47	9.417	2497	2512	2537	rBV	279152	459586	76.84%	9.801%
48	9.578	2554	2562	2565	rBB2	407	539	0.09%	0.011%
49	9.694	2592	2598	2600	rVV2	652	716	0.12%	0.015%
50	9.722	2604	2607	2616	rVV	151	263	0.04%	0.006%
51	9.793	2625	2629	2633	rBB	155	153	0.03%	0.003%
52	9.816	2634	2636	2639	rBV	122	111	0.02%	0.002%
53	9.957	2678	2680	2683	rVB	184	124	0.02%	0.003%
54	10.060	2709	2712	2714	rBV	188	148	0.02%	0.003%
55	10.112	2726	2728	2732	rVB2	210	116	0.02%	0.002%
56	10.179	2743	2749	2753	rBV	175	258	0.04%	0.006%
57	10.221	2759	2762	2764	rBV	126	111	0.02%	0.002%
58	10.317	2789	2792	2795	rBV	149	147	0.02%	0.003%
59	10.353	2800	2803	2806	rVV	159	164	0.03%	0.003%
60	10.382	2810	2812	2816	rBB	120	107	0.02%	0.002%
61	10.478	2836	2842	2849	rBV	168	335	0.06%	0.007%
62	10.587	2872	2876	2878	rBV	157	162	0.03%	0.003%
63	10.607	2879	2882	2885	rVB	210	156	0.03%	0.003%
64	10.645	2891	2894	2896	rBV	153	128	0.02%	0.003%
65	10.671	2896	2902	2909	rVV3	1420	1792	0.30%	0.038%
66	10.758	2917	2929	2946	rBV	191174	304317	50.88%	6.490%
67	10.902	2970	2974	2980	rVB3	719	841	0.14%	0.018%
68	11.002	2997	3005	3011	rVV2	617	1086	0.18%	0.023%
69	11.089	3029	3032	3037	rVB	426	378	0.06%	0.008%
70	11.240	3075	3079	3081	rBV	166	172	0.03%	0.004%
71	11.298	3089	3097	3101	rVB2	390	612	0.10%	0.013%
72	11.324	3101	3105	3108	rBV	178	188	0.03%	0.004%
73	11.465	3139	3149	3158	rBV3	2309	3539	0.59%	0.075%
74	11.700	3219	3222	3228	rVB2	336	311	0.05%	0.007%
75	11.758	3236	3240	3245	rVB	149	112	0.02%	0.002%
76	11.812	3245	3257	3275	rBV	302730	471268	78.79%	10.050%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121521\
 Data File : VU046397.D
 Acq On : 15 Dec 2021 15:07
 Operator : SY/MD
 Sample : VIBLK013
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK013

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.880	3275	3278	3279	rBV	240	128	0.02%	0.003%
78	11.899	3279	3284	3288	rVB	484	470	0.08%	0.010%
79	11.970	3302	3306	3313	rVB4	925	1131	0.19%	0.024%
80	12.066	3331	3336	3338	rBV	205	226	0.04%	0.005%
81	12.192	3363	3375	3393	rBV	274307	431482	72.14%	9.202%
82	12.330	3416	3418	3421	rBV	239	116	0.02%	0.002%
83	12.481	3460	3465	3468	rBV	140	139	0.02%	0.003%
84	12.764	3550	3553	3554	rBV	198	135	0.02%	0.003%
85	13.816	3875	3880	3882	rBV	127	117	0.02%	0.002%
86	14.092	3960	3966	3974	rVB	387	658	0.11%	0.014%
87	14.571	4111	4115	4116	rBV2	159	120	0.02%	0.003%
88	15.211	4311	4314	4317	rVB	204	103	0.02%	0.002%
89	15.391	4366	4370	4375	rBV2	185	231	0.04%	0.005%
90	15.417	4375	4378	4381	rBV	194	103	0.02%	0.002%
91	15.606	4433	4437	4443	rVB2	274	263	0.04%	0.006%
92	15.645	4444	4449	4452	rBV2	157	148	0.02%	0.003%
93	15.684	4457	4461	4464	rBV2	180	159	0.03%	0.003%
94	15.709	4464	4469	4471	rBV2	151	135	0.02%	0.003%
95	15.767	4482	4487	4493	rBV2	266	392	0.07%	0.008%
96	15.812	4497	4501	4506	rBV	208	219	0.04%	0.005%
97	16.336	4662	4664	4668	rBV	262	144	0.02%	0.003%
98	16.446	4696	4698	4701	rBV2	220	109	0.02%	0.002%
99	16.680	4768	4771	4775	rBV2	302	223	0.04%	0.005%
100	16.790	4803	4805	4809	rVB3	341	149	0.02%	0.003%




Sum of corrected areas: 4689019

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121521\
Data File : VU046397.D
Acq On : 15 Dec 2021 15:07
Operator : SY/MD
Sample : VIBLK013
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK013

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

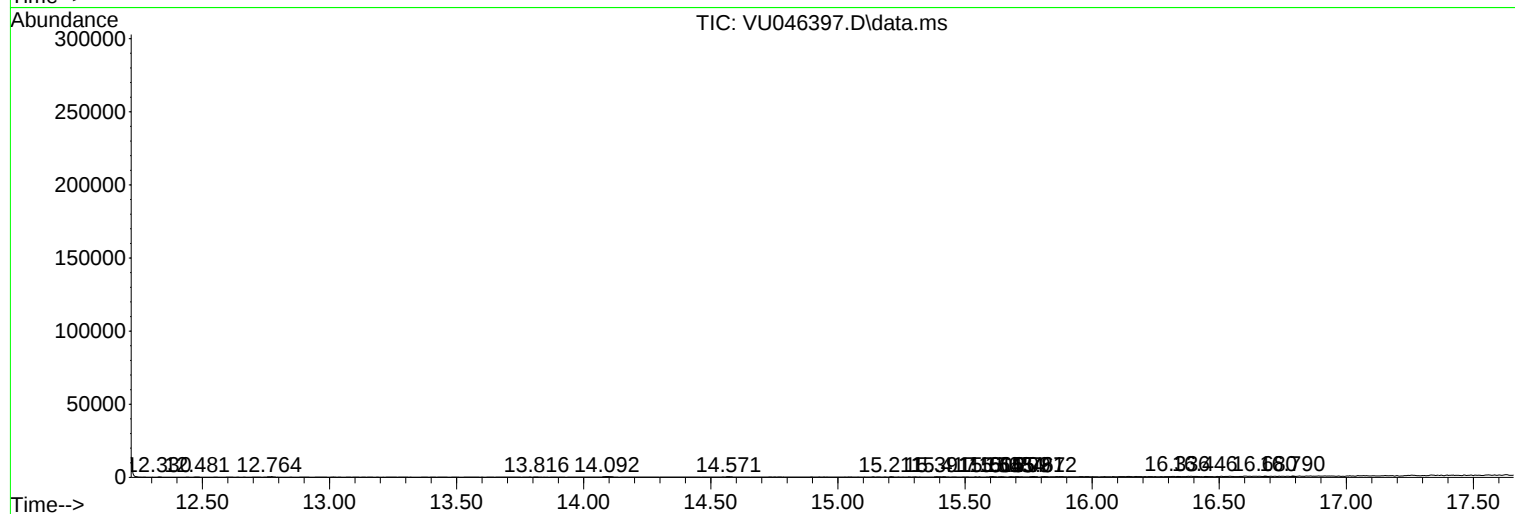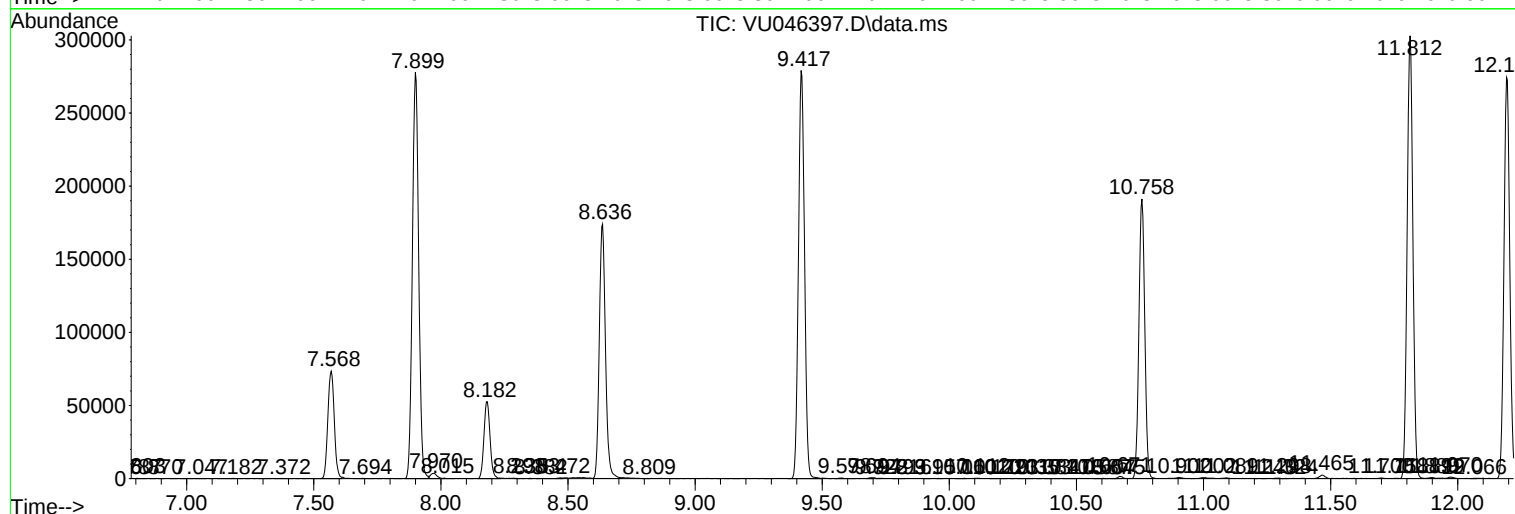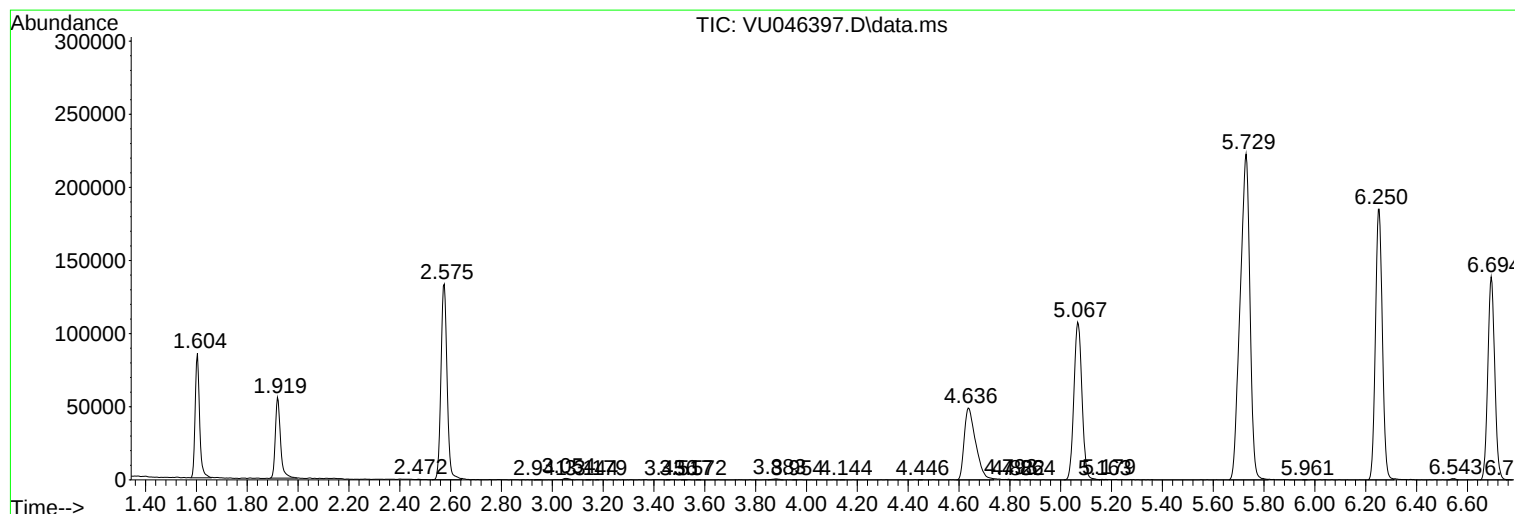

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121521\
Data File : VU046397.D
Acq On : 15 Dec 2021 15:07
Operator : SY/MD
Sample : VIBLK013
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK013

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121521\
Data File : VU046397.D
Acq On : 15 Dec 2021 15:07
Operator : SY/MD
Sample : VIBLK013
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK013

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------