

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121521\
 Data File : VU046406.D
 Acq On : 15 Dec 2021 19:09
 Operator : SY/MD
 Sample : M4983-23
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046406.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	101	rVB	82840	102006	16.51%	2.178%
2	1.919	171	180	205	rBV	55002	80005	12.95%	1.708%
3	2.308	299	301	304	rBV2	145	112	0.02%	0.002%
4	2.346	310	313	321	rVB	277	264	0.04%	0.006%
5	2.571	372	383	418	rVB	135657	229158	37.10%	4.894%
6	2.729	429	432	436	rBB	165	161	0.03%	0.003%
7	2.835	463	465	467	rBV	158	107	0.02%	0.002%
8	3.047	527	531	532	rBV	1113	699	0.11%	0.015%
9	3.150	561	563	566	rBV	121	107	0.02%	0.002%
10	3.186	571	574	578	rBV	264	220	0.04%	0.005%
11	3.269	596	600	604	rBB	157	171	0.03%	0.004%
12	3.350	623	625	628	rBV	133	116	0.02%	0.002%
13	3.417	641	646	650	rBB	127	181	0.03%	0.004%
14	4.121	862	865	868	rBB	142	121	0.02%	0.003%
15	4.346	932	935	938	rBV	130	135	0.02%	0.003%
16	4.636	1011	1025	1060	rBV	48865	142920	23.14%	3.052%
17	4.819	1079	1082	1088	rVB2	205	225	0.04%	0.005%
18	4.941	1116	1120	1122	rBB	123	111	0.02%	0.002%
19	5.067	1143	1159	1177	rBV	112633	242728	39.30%	5.183%
20	5.237	1210	1212	1215	rVV2	243	166	0.03%	0.004%
21	5.295	1227	1230	1232	rBB	237	116	0.02%	0.002%
22	5.729	1343	1365	1392	rBV2	230443	617690	100.00%	13.191%
23	5.896	1414	1417	1420	rBB	140	120	0.02%	0.003%
24	6.253	1514	1528	1554	rBV	185396	345329	55.91%	7.374%
25	6.343	1554	1556	1561	rVV	233	200	0.03%	0.004%
26	6.530	1611	1614	1618	rBB3	389	258	0.04%	0.006%
27	6.694	1652	1665	1683	rBV	140410	271058	43.88%	5.788%
28	6.812	1699	1702	1705	rBV	148	142	0.02%	0.003%
29	7.044	1771	1774	1778	rVV2	300	253	0.04%	0.005%
30	7.185	1815	1818	1821	rBV	285	289	0.05%	0.006%
31	7.484	1909	1911	1916	rBB	162	160	0.03%	0.003%
32	7.568	1925	1937	1953	rBV	76764	131645	21.31%	2.811%
33	7.780	2001	2003	2008	rBB	129	139	0.02%	0.003%
34	7.841	2020	2022	2027	rBB	159	131	0.02%	0.003%
35	7.899	2028	2040	2056	rBV	287762	487945	79.00%	10.420%
36	7.967	2058	2061	2072	rVB3	3220	4951	0.80%	0.106%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121521\
 Data File : VU046406.D
 Acq On : 15 Dec 2021 19:09
 Operator : SY/MD
 Sample : M4983-23
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	8.182	2115	2128	2143	rBV	52953	88203	14.28%	1.884%
38	8.314	2167	2169	2171	rBV	219	129	0.02%	0.003%
39	8.430	2202	2205	2207	rBV	140	115	0.02%	0.002%
40	8.462	2211	2215	2216	rBV	423	313	0.05%	0.007%
41	8.475	2216	2219	2222	rBV2	361	316	0.05%	0.007%
42	8.552	2239	2243	2251	rVB3	1027	1168	0.19%	0.025%
43	8.584	2251	2253	2257	rVB2	273	206	0.03%	0.004%
44	8.636	2257	2269	2291	rBV	173841	293616	47.53%	6.270%
45	8.777	2310	2313	2317	rVB2	173	144	0.02%	0.003%
46	8.928	2356	2360	2363	rBB	179	143	0.02%	0.003%
47	8.980	2373	2376	2380	rBB	140	141	0.02%	0.003%
48	9.066	2399	2403	2406	rBB	182	177	0.03%	0.004%
49	9.230	2451	2454	2457	rBV	164	154	0.02%	0.003%
50	9.420	2500	2513	2534	rBV	272221	446341	72.26%	9.532%
51	9.510	2538	2541	2547	rVV2	285	247	0.04%	0.005%
52	9.552	2552	2554	2557	rBV	168	141	0.02%	0.003%
53	9.616	2571	2574	2578	rBV	155	183	0.03%	0.004%
54	9.684	2591	2595	2598	rBV	309	276	0.04%	0.006%
55	9.697	2598	2599	2603	rVB	302	165	0.03%	0.004%
56	9.867	2649	2652	2654	rBV	156	129	0.02%	0.003%
57	9.973	2682	2685	2688	rBV	162	163	0.03%	0.003%
58	10.150	2737	2740	2742	rBV	137	116	0.02%	0.002%
59	10.198	2753	2755	2757	rBV	165	114	0.02%	0.002%
60	10.343	2795	2800	2802	rBV	151	150	0.02%	0.003%
61	10.401	2815	2818	2820	rBV	156	127	0.02%	0.003%
62	10.488	2841	2845	2847	rBV	151	161	0.03%	0.003%
63	10.545	2860	2863	2868	rBV	160	207	0.03%	0.004%
64	10.626	2885	2888	2891	rBV	165	158	0.03%	0.003%
65	10.674	2896	2903	2910	rVV2	1518	1893	0.31%	0.040%
66	10.758	2916	2929	2945	rVV	193242	308191	49.89%	6.581%
67	10.896	2965	2972	2980	rVV2	569	814	0.13%	0.017%
68	10.951	2985	2989	2990	rBV	167	139	0.02%	0.003%
69	10.996	3001	3003	3010	rVB	238	243	0.04%	0.005%
70	11.044	3016	3018	3021	rBV	122	108	0.02%	0.002%
71	11.192	3061	3064	3065	rBV	155	107	0.02%	0.002%
72	11.375	3118	3121	3123	rBV	177	141	0.02%	0.003%
73	11.455	3141	3146	3148	rBV2	802	755	0.12%	0.016%
74	11.574	3181	3183	3188	rVB2	191	179	0.03%	0.004%
75	11.697	3218	3221	3226	rVB2	337	279	0.05%	0.006%
76	11.812	3245	3257	3276	rVV	282535	438046	70.92%	9.354%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121521\
 Data File : VU046406.D
 Acq On : 15 Dec 2021 19:09
 Operator : SY/MD
 Sample : M4983-23
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.938	3289	3296	3297	rBV2	230	238	0.04%	0.005%
78	11.973	3302	3307	3313	rVB3	1067	1131	0.18%	0.024%
79	12.060	3331	3334	3337	rBV	233	208	0.03%	0.004%
80	12.195	3363	3376	3396	rVB	272643	431664	69.88%	9.218%
81	12.333	3414	3419	3424	rVV3	258	219	0.04%	0.005%
82	12.642	3513	3515	3520	rVB	194	122	0.02%	0.003%
83	12.774	3550	3556	3561	rBV	516	658	0.11%	0.014%
84	14.098	3964	3968	3973	rBV2	238	247	0.04%	0.005%
85	14.574	4112	4116	4124	rVB2	295	392	0.06%	0.008%
86	14.831	4192	4196	4201	rBV2	252	210	0.03%	0.004%
87	15.124	4284	4287	4291	rBV	224	133	0.02%	0.003%
88	15.391	4365	4370	4374	rVB2	164	154	0.02%	0.003%
89	15.491	4397	4401	4403	rBV2	135	108	0.02%	0.002%
90	15.510	4403	4407	4412	rVB2	184	234	0.04%	0.005%
91	15.542	4414	4417	4420	rBV2	208	161	0.03%	0.003%
92	15.645	4444	4449	4452	rBV2	303	317	0.05%	0.007%
93	15.709	4462	4469	4475	rBV2	215	318	0.05%	0.007%
94	15.770	4485	4488	4492	rBV2	140	160	0.03%	0.003%
95	15.918	4531	4534	4535	rBV	218	134	0.02%	0.003%
96	16.079	4581	4584	4590	rBV2	114	119	0.02%	0.003%
97	16.291	4647	4650	4652	rBV2	223	135	0.02%	0.003%
98	16.786	4802	4804	4808	rVB	449	274	0.04%	0.006%
99	17.571	5045	5048	5054	rBV2	724	614	0.10%	0.013%
100	17.616	5060	5062	5066	rBV3	545	277	0.04%	0.006%




Sum of corrected areas: 4682764

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121521\
Data File : VU046406.D
Acq On : 15 Dec 2021 19:09
Operator : SY/MD
Sample : M4983-23
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

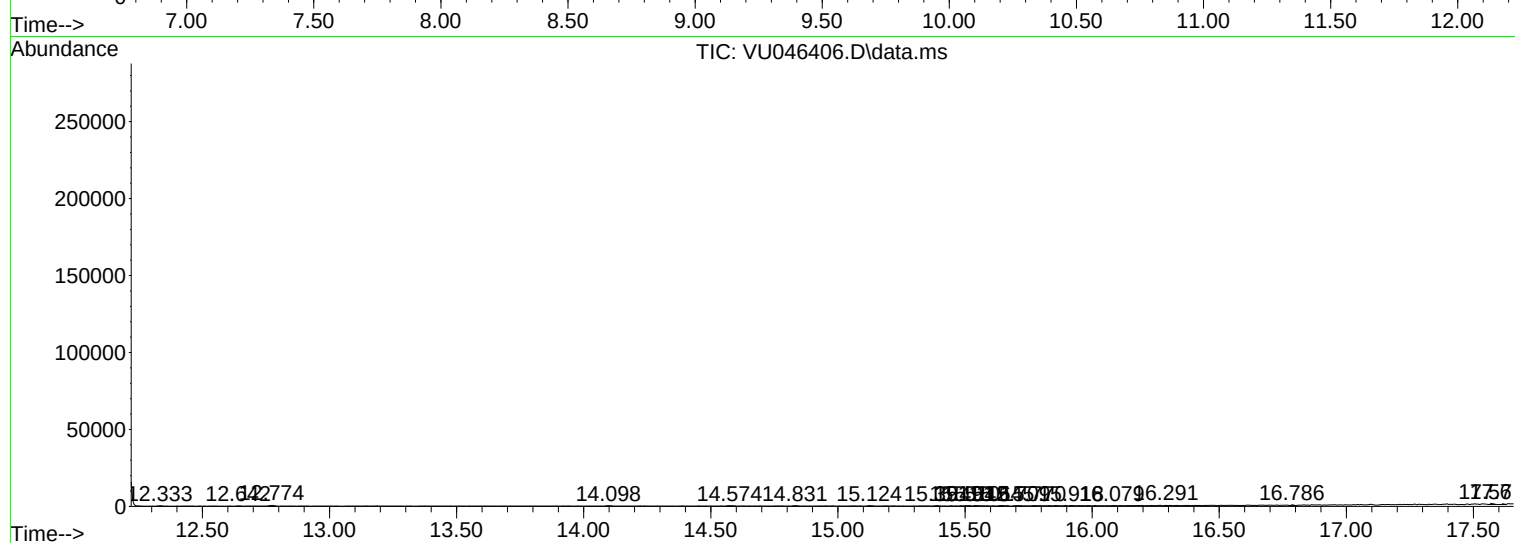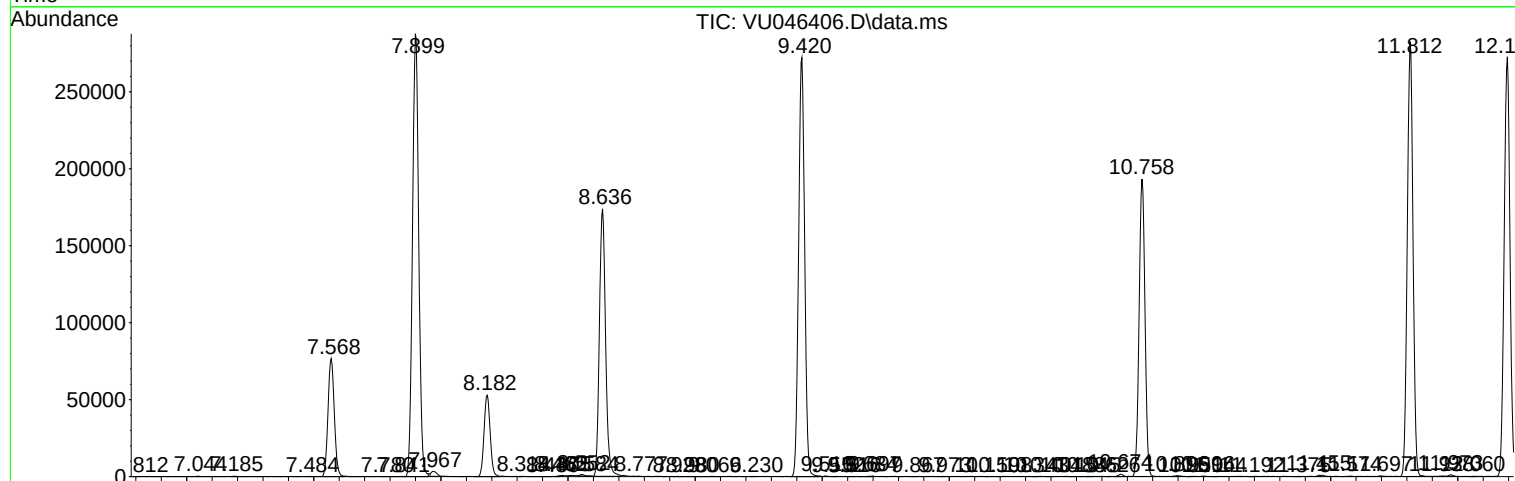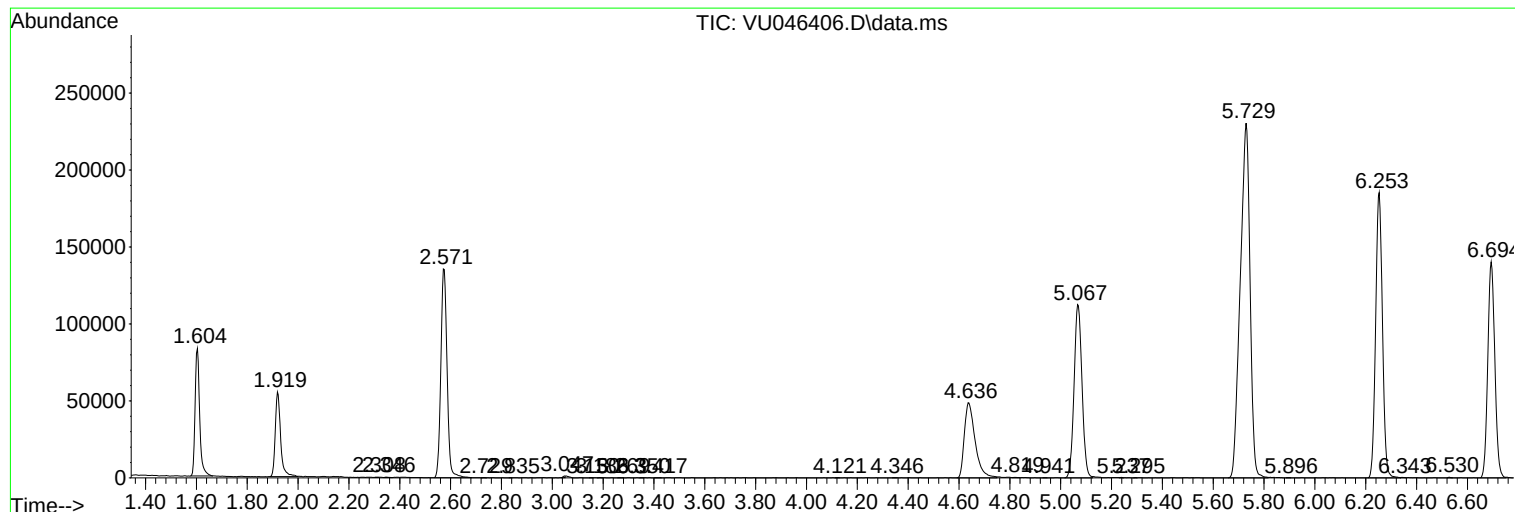

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121521\
Data File : VU046406.D
Acq On : 15 Dec 2021 19:09
Operator : SY/MD
Sample : M4983-23
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121521\
Data File : VU046406.D
Acq On : 15 Dec 2021 19:09
Operator : SY/MD
Sample : M4983-23
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc