

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121521\
 Data File : VU046407.D
 Acq On : 15 Dec 2021 19:32
 Operator : SY/MD
 Sample : M5002-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046407.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	101	rBV	81540	98345	16.32%	2.151%
2	1.919	171	180	201	rBV	53811	77893	12.93%	1.703%
3	2.314	299	303	307	rVB2	191	192	0.03%	0.004%
4	2.350	307	314	316	rBV2	175	236	0.04%	0.005%
5	2.571	371	383	402	rBV	132623	222267	36.89%	4.861%
6	2.674	413	415	418	rVB2	297	145	0.02%	0.003%
7	2.745	434	437	441	rBV	146	171	0.03%	0.004%
8	2.973	506	508	512	rBB	137	117	0.02%	0.003%
9	3.051	525	532	542	rVB4	1111	2126	0.35%	0.046%
10	3.102	545	548	551	rBB	158	126	0.02%	0.003%
11	3.182	567	573	574	rBV2	409	408	0.07%	0.009%
12	3.292	605	607	610	rBB	133	94	0.02%	0.002%
13	3.475	661	664	666	rBB	158	102	0.02%	0.002%
14	4.012	828	831	834	rBB	150	124	0.02%	0.003%
15	4.636	1011	1025	1054	rBV	51872	139949	23.23%	3.060%
16	4.825	1080	1084	1089	rVV2	169	186	0.03%	0.004%
17	4.880	1099	1101	1104	rVB2	267	167	0.03%	0.004%
18	5.067	1143	1159	1180	rBV	109753	237428	39.41%	5.192%
19	5.250	1213	1216	1220	rVB	227	209	0.03%	0.005%
20	5.288	1223	1228	1231	rBB	155	173	0.03%	0.004%
21	5.314	1234	1236	1238	rBB	230	109	0.02%	0.002%
22	5.401	1260	1263	1265	rBV	118	108	0.02%	0.002%
23	5.603	1323	1326	1329	rBB	134	114	0.02%	0.002%
24	5.636	1333	1336	1339	rVB	172	139	0.02%	0.003%
25	5.729	1342	1365	1390	rBV2	223314	602442	100.00%	13.174%
26	6.253	1514	1528	1553	rBV	175910	334155	55.47%	7.307%
27	6.536	1613	1616	1618	rVV	256	180	0.03%	0.004%
28	6.629	1642	1645	1650	rBB	140	166	0.03%	0.004%
29	6.693	1651	1665	1683	rBV	139249	266090	44.17%	5.819%
30	6.780	1689	1692	1694	rBB	233	108	0.02%	0.002%
31	6.806	1697	1700	1703	rBB2	236	133	0.02%	0.003%
32	7.182	1814	1817	1823	rBV	176	249	0.04%	0.005%
33	7.218	1826	1828	1831	rBB	163	109	0.02%	0.002%
34	7.568	1924	1937	1958	rVB	73671	128096	21.26%	2.801%
35	7.687	1972	1974	1976	rBV	148	99	0.02%	0.002%
36	7.767	1994	1999	2001	rBB	130	112	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121521\
 Data File : VU046407.D
 Acq On : 15 Dec 2021 19:32
 Operator : SY/MD
 Sample : M5002-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	7.809	2008	2012	2014	rBV	120	107	0.02%	0.002%
38	7.835	2017	2020	2022	rBB	149	100	0.02%	0.002%
39	7.899	2027	2040	2056	rBV	277155	475467	78.92%	10.398%
40	7.970	2059	2062	2074	rVB2	3552	4910	0.82%	0.107%
41	8.028	2077	2080	2083	rBB	277	182	0.03%	0.004%
42	8.127	2108	2111	2113	rBV	148	122	0.02%	0.003%
43	8.182	2117	2128	2144	rBV	52327	85791	14.24%	1.876%
44	8.295	2161	2163	2165	rVV	244	146	0.02%	0.003%
45	8.481	2212	2221	2227	rBV2	894	1373	0.23%	0.030%
46	8.523	2230	2234	2236	rBV2	377	296	0.05%	0.006%
47	8.635	2257	2269	2293	rBV	176234	292276	48.52%	6.392%
48	8.783	2312	2315	2317	rVB2	237	123	0.02%	0.003%
49	8.870	2339	2342	2346	rBB	132	114	0.02%	0.002%
50	8.915	2352	2356	2360	rVB2	537	542	0.09%	0.012%
51	8.992	2377	2380	2384	rBV	189	200	0.03%	0.004%
52	9.066	2401	2403	2405	rBV	152	107	0.02%	0.002%
53	9.121	2416	2420	2424	rBB	159	189	0.03%	0.004%
54	9.189	2438	2441	2443	rBV	134	121	0.02%	0.003%
55	9.282	2468	2470	2473	rBV	144	120	0.02%	0.003%
56	9.420	2498	2513	2529	rBV	263724	434614	72.14%	9.504%
57	9.504	2536	2539	2543	rVB2	263	204	0.03%	0.004%
58	9.574	2558	2561	2565	rBV	224	202	0.03%	0.004%
59	9.655	2583	2586	2589	rBV	157	163	0.03%	0.004%
60	9.687	2594	2596	2597	rBV	283	137	0.02%	0.003%
61	9.716	2603	2605	2610	rBB	159	153	0.03%	0.003%
62	9.851	2642	2647	2651	rBV	183	263	0.04%	0.006%
63	9.963	2678	2682	2687	rBB	188	235	0.04%	0.005%
64	9.996	2687	2692	2696	rBV	174	251	0.04%	0.005%
65	10.015	2696	2698	2701	rVB	156	106	0.02%	0.002%
66	10.041	2704	2706	2710	rVB	226	112	0.02%	0.002%
67	10.118	2727	2730	2733	rBV	128	138	0.02%	0.003%
68	10.291	2781	2784	2787	rBV	177	178	0.03%	0.004%
69	10.401	2814	2818	2821	rBB	135	139	0.02%	0.003%
70	10.426	2822	2826	2829	rBV	194	204	0.03%	0.004%
71	10.488	2840	2845	2848	rBV	150	198	0.03%	0.004%
72	10.674	2895	2903	2909	rBV2	1269	1501	0.25%	0.033%
73	10.758	2916	2929	2947	rBV2	195486	306265	50.84%	6.698%
74	10.838	2951	2954	2956	rBV	198	148	0.02%	0.003%
75	10.867	2961	2963	2968	rBV2	208	175	0.03%	0.004%
76	10.896	2968	2972	2976	rBV2	346	342	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121521\
 Data File : VU046407.D
 Acq On : 15 Dec 2021 19:32
 Operator : SY/MD
 Sample : M5002-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.266	3084	3087	3090	rBV	219	192	0.03%	0.004%
78	11.327	3103	3106	3110	rVB	191	188	0.03%	0.004%
79	11.349	3111	3113	3115	rBV	158	107	0.02%	0.002%
80	11.455	3140	3146	3147	rBV2	714	631	0.10%	0.014%
81	11.568	3178	3181	3186	rBV2	189	233	0.04%	0.005%
82	11.690	3216	3219	3222	rBV	268	233	0.04%	0.005%
83	11.812	3245	3257	3274	rVV	281236	425569	70.64%	9.307%
84	11.896	3277	3283	3287	rBB	116	119	0.02%	0.003%
85	11.944	3291	3298	3302	rBV2	313	419	0.07%	0.009%
86	11.970	3303	3306	3317	rVB4	943	1109	0.18%	0.024%
87	12.195	3363	3376	3391	rVV	263014	420330	69.77%	9.192%
88	12.259	3394	3396	3401	rVB	180	142	0.02%	0.003%
89	12.635	3508	3513	3514	rBV	141	113	0.02%	0.002%
90	12.774	3548	3556	3561	rBV2	462	745	0.12%	0.016%
91	13.034	3631	3637	3640	rBV	146	170	0.03%	0.004%
92	13.931	3913	3916	3924	rBV	117	112	0.02%	0.002%
93	14.500	4088	4093	4098	rBV	126	176	0.03%	0.004%
94	14.581	4114	4118	4122	rBV2	243	229	0.04%	0.005%
95	14.764	4172	4175	4178	rBV	129	98	0.02%	0.002%
96	15.400	4370	4373	4377	rBV	196	115	0.02%	0.003%
97	15.523	4407	4411	4416	rBV2	195	175	0.03%	0.004%
98	15.568	4421	4425	4429	rBV	168	145	0.02%	0.003%
99	15.587	4429	4431	4436	rVB	237	215	0.04%	0.005%
100	15.683	4454	4461	4465	rBV2	232	349	0.06%	0.008%




Sum of corrected areas: 4572795

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121521\
Data File : VU046407.D
Acq On : 15 Dec 2021 19:32
Operator : SY/MD
Sample : M5002-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

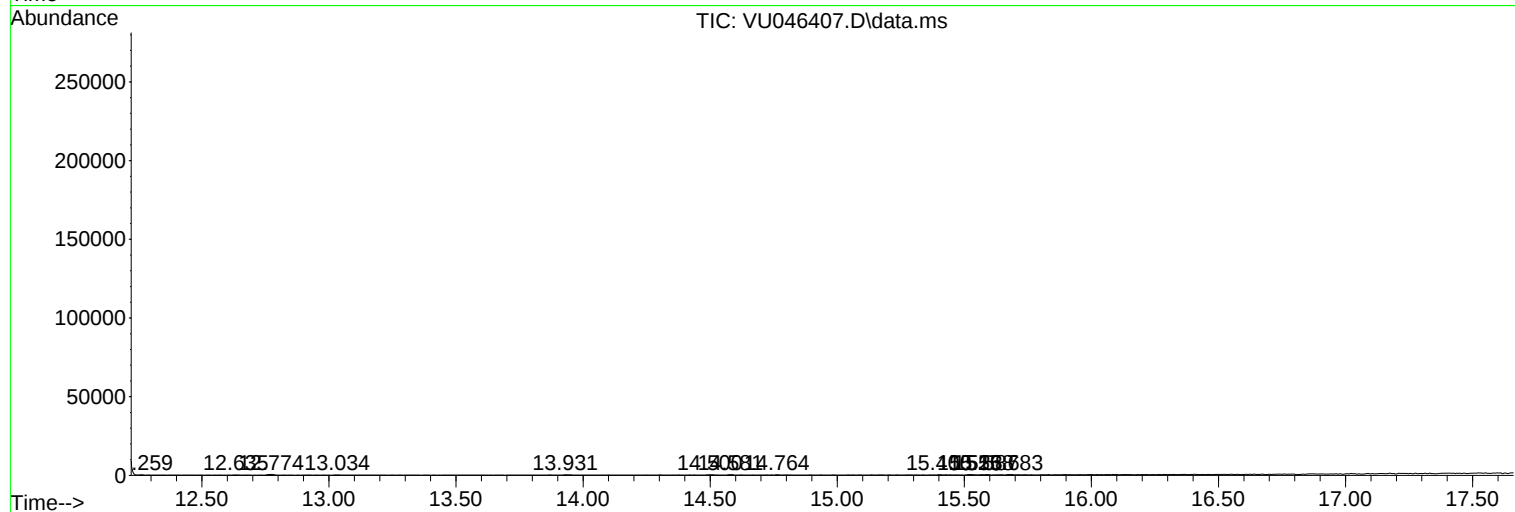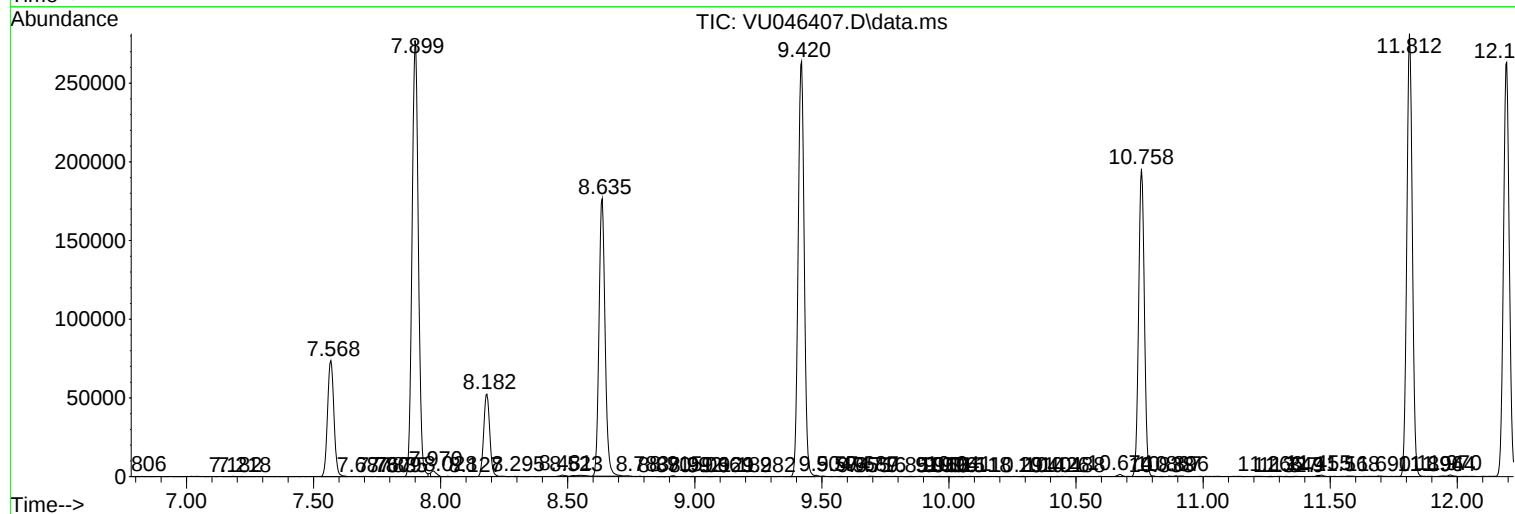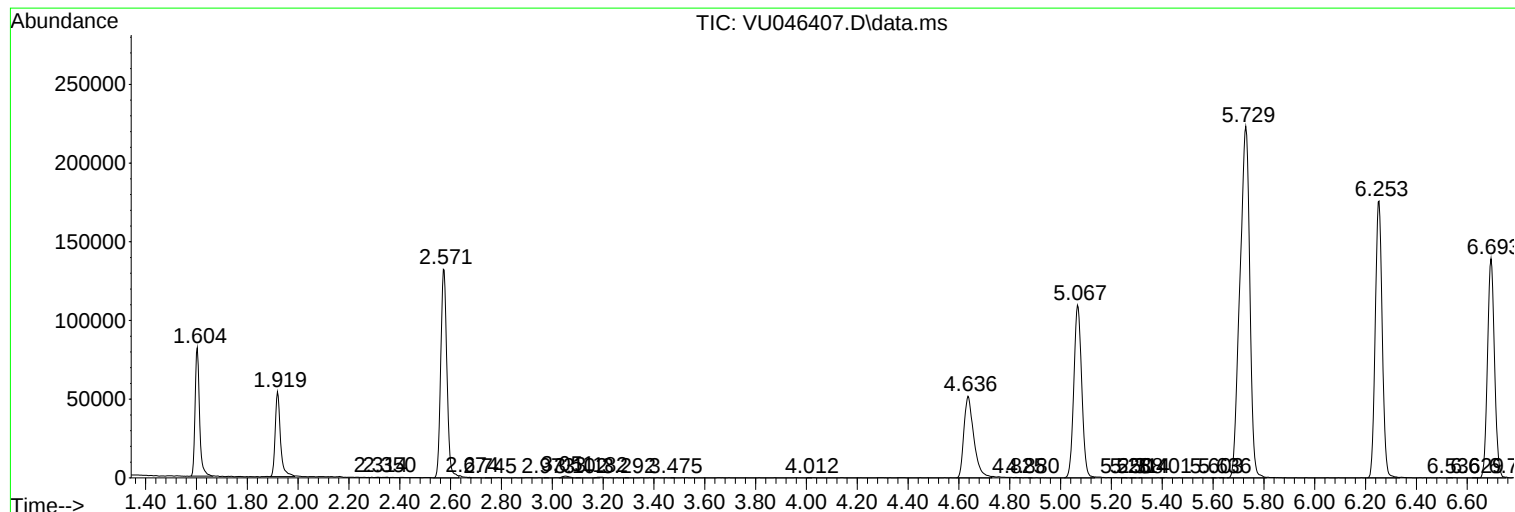

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121521\
Data File : VU046407.D
Acq On : 15 Dec 2021 19:32
Operator : SY/MD
Sample : M5002-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121521\
Data File : VU046407.D
Acq On : 15 Dec 2021 19:32
Operator : SY/MD
Sample : M5002-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc