


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121521\
Data File : VU046386.D
Acq On : 15 Dec 2021 09:33
Operator : SY/MD
Sample : BFB032
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB032

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Title : VOC Analysis
Last Update : Mon Dec 20 00:25:10 2021

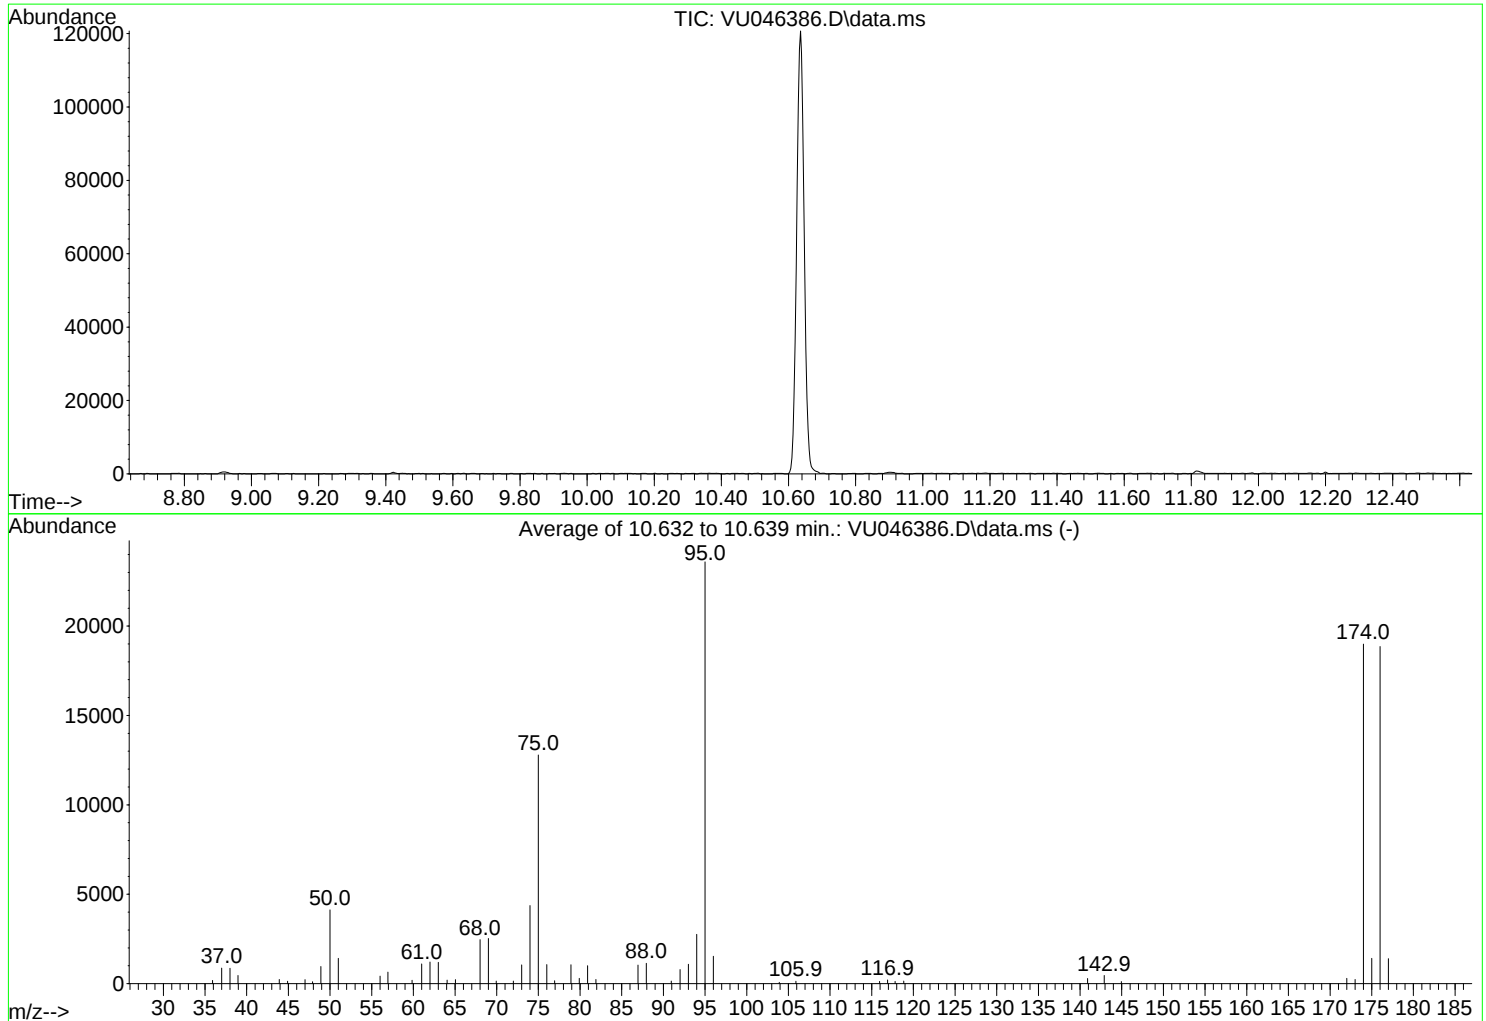

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2879

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.5	4124	PASS
75	95	30	80	54.2	12786	PASS
95	95	100	100	100.0	23592	PASS
96	95	5	9	6.5	1533	PASS
173	174	0.00	2	1.2	235	PASS
174	95	50	120	80.5	18989	PASS
175	174	5	9	7.5	1416	PASS
176	174	95	101	99.3	18861	PASS
177	176	5	9	7.4	1399	PASS

Instrument :
MSVOA_U
ClientSampleId :
BFB032

m/z	Abundance
35.90	194.0
37.00	823.0
38.00	785.0
39.00	452.0
43.90	257.0
44.80	132.0
47.00	219.0
47.90	109.0
48.90	949.0
50.00	3738.0
51.00	1361.0
56.00	391.0
57.00	646.0
59.80	177.0
61.00	1053.0
62.00	1155.0
63.00	1113.0
64.10	182.0
65.00	201.0
68.00	2341.0
69.00	2465.0
70.00	143.0
72.00	120.0
73.00	989.0
74.00	4261.0
75.00	12138.0
76.00	939.0
77.00	108.0
78.90	967.0
79.90	292.0
80.90	1018.0
81.90	252.0
87.00	969.0
87.90	1126.0
90.90	133.0
92.00	781.0
93.00	1075.0
94.00	2718.0
95.00	23224.0
96.00	1487.0
105.90	140.0
116.00	141.0
116.90	208.0
117.80	129.0
118.90	145.0
140.90	276.0
142.90	420.0
144.90	119.0
172.00	283.0
173.00	193.0
174.00	19392.0
175.00	1460.0
176.00	18816.0
177.00	1365.0

Instrument :
MSVOA_U
ClientSampleId :
BFB032

m/z	Abundance
35.90	167.0
37.00	898.0
38.00	909.0
38.90	440.0
43.90	192.0
45.00	131.0
47.00	217.0
47.90	105.0
48.90	922.0
50.00	4377.0
51.00	1416.0
56.00	432.0
56.90	649.0
59.90	199.0
61.00	1127.0
62.00	1236.0
63.00	1236.0
64.00	188.0
65.10	250.0
68.00	2491.0
69.00	2539.0
69.90	134.0
72.00	152.0
73.00	1066.0
74.00	4287.0
75.00	12990.0
76.00	1168.0
76.90	217.0
78.90	1097.0
79.90	309.0
80.90	970.0
81.90	206.0
86.90	1068.0
88.00	1093.0
91.00	155.0
92.00	764.0
93.00	1061.0
94.00	2739.0
95.00	23216.0
96.00	1537.0
103.90	111.0
105.90	123.0
115.90	101.0
116.90	198.0
117.80	111.0
118.80	147.0
140.90	296.0
142.90	467.0
145.00	114.0
172.00	287.0
173.00	271.0
174.00	17976.0
175.00	1327.0
176.00	18368.0
177.00	1383.0

Instrument :
MSVOA_U
ClientSampleId :
BFB032

m/z	Abundance
35.90	188.0
37.00	891.0
38.00	884.0
39.00	473.0
43.90	238.0
44.90	136.0
47.00	233.0
47.90	122.0
48.90	1012.0
50.00	4257.0
51.00	1475.0
56.00	429.0
56.90	643.0
59.90	176.0
61.00	1122.0
62.00	1235.0
63.00	1235.0
64.00	208.0
65.10	233.0
68.00	2556.0
69.00	2581.0
69.90	148.0
72.00	153.0
73.00	1075.0
74.00	4555.0
75.00	13230.0
76.00	1088.0
77.00	154.0
78.90	1104.0
79.90	298.0
80.90	1029.0
81.90	233.0
86.90	1064.0
87.90	1192.0
91.00	153.0
92.00	819.0
93.00	1106.0
94.00	2808.0
95.00	24336.0
96.00	1575.0
103.90	108.0
105.90	133.0
115.90	138.0
116.90	217.0
117.80	134.0
118.80	148.0
140.90	299.0
142.90	479.0
144.90	121.0
172.00	305.0
173.00	240.0
174.00	19600.0
175.00	1461.0
176.00	19400.0
177.00	1450.0

Instrument :
MSVOA_U
ClientSampleId :
BFB032