

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121522\
 Data File : VU052414.D
 Acq On : 15 Dec 2022 12:25
 Operator : JC/MD
 Sample : N6050-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 B0AA8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052414.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	92	rVB	36067	41135	4.00%	0.571%
2	1.916	171	179	193	rVB	82373	112033	10.90%	1.555%
3	2.569	371	382	400	rVB	128175	207232	20.16%	2.877%
4	4.646	1011	1028	1064	rBV	120306	446773	43.46%	6.202%
5	5.070	1141	1160	1186	rBV3	207764	661739	64.37%	9.187%
6	5.723	1343	1363	1393	rBV2	296707	801694	77.98%	11.130%
7	6.247	1509	1526	1551	rBV	244643	480323	46.72%	6.668%
8	6.687	1649	1663	1681	rBV	199643	393041	38.23%	5.456%
9	7.102	1777	1792	1807	rBV	97581	183617	17.86%	2.549%
10	7.562	1923	1935	1956	rBV	77862	139938	13.61%	1.943%
11	7.896	2026	2039	2060	rBV	237201	422052	41.05%	5.859%
12	8.179	2116	2127	2141	rBV2	52341	94267	9.17%	1.309%
13	8.636	2255	2269	2302	rBV2	495964	1028076	100.00%	14.273%
14	8.806	2308	2322	2335	rVB2	57289	99976	9.72%	1.388%
15	9.414	2498	2511	2529	rBV	380135	631673	61.44%	8.769%
16	10.752	2910	2927	2942	rBV	192286	310962	30.25%	4.317%
17	10.928	2973	2982	2995	rVB	24050	36829	3.58%	0.511%
18	11.044	3008	3018	3030	rVB3	8941	13465	1.31%	0.187%
19	11.809	3244	3256	3276	rBV	329672	538367	52.37%	7.474%
20	12.189	3361	3374	3394	rBV	341479	559980	54.47%	7.774%




Sum of corrected areas: 7203172

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121522\
Data File : VU052414.D
Acq On : 15 Dec 2022 12:25
Operator : JC/MD
Sample : N6050-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
B0AA8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

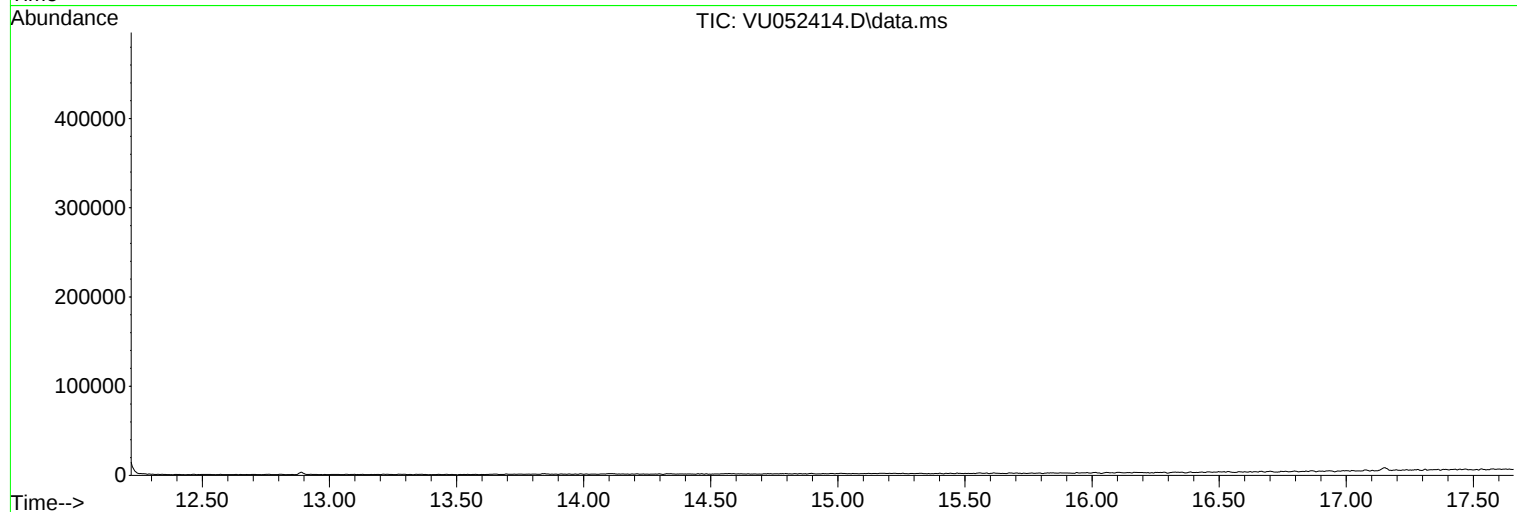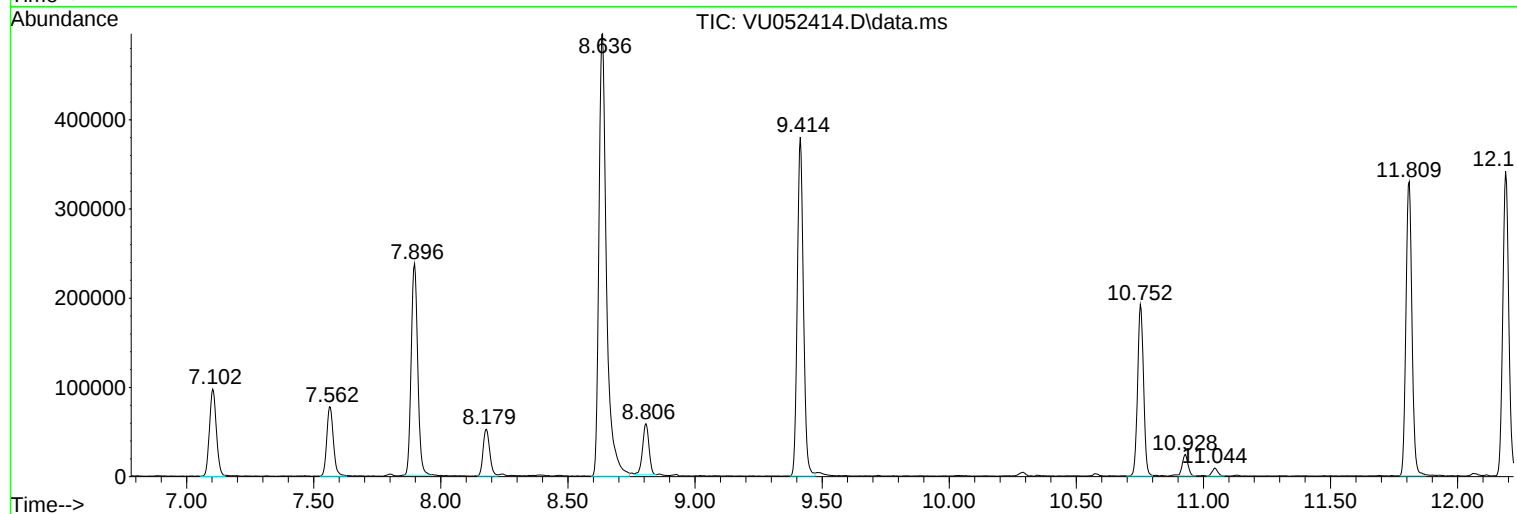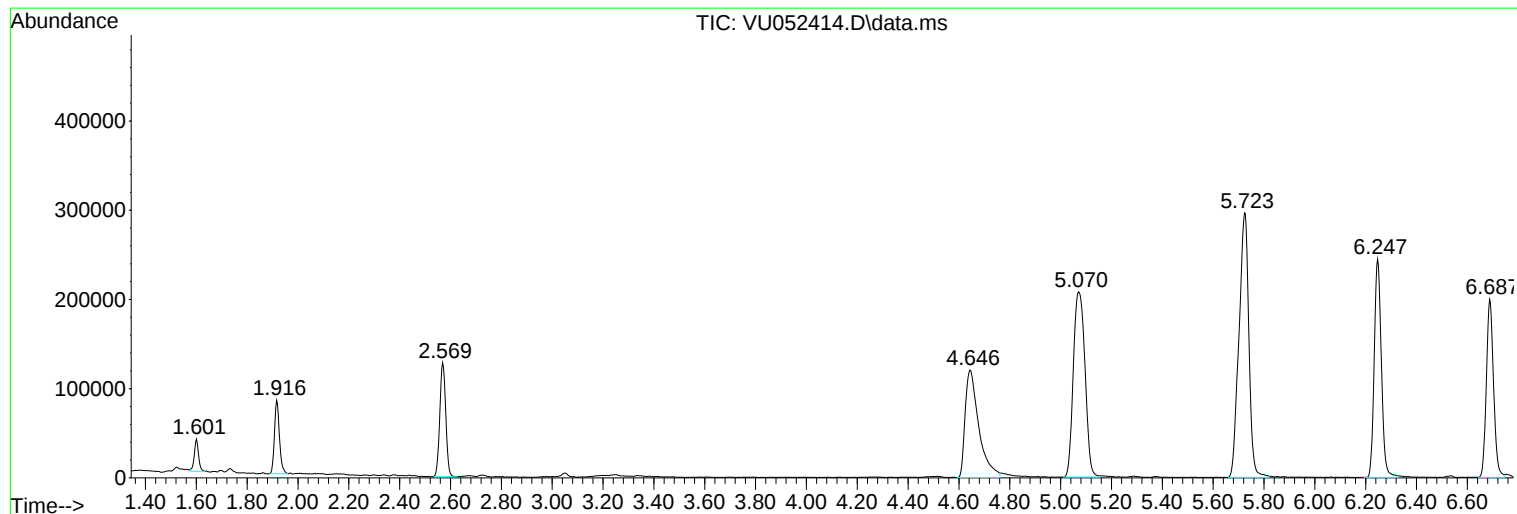

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121522\
Data File : VU052414.D
Acq On : 15 Dec 2022 12:25
Operator : JC/MD
Sample : N6050-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
B0AA8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121522\
Data File : VU052414.D
Acq On : 15 Dec 2022 12:25
Operator : JC/MD
Sample : N6050-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
B0AA8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc