

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121523\
 Data File : VU056898.D
 Acq On : 15 Dec 2023 23:15
 Operator : MD/SY
 Sample : 05809-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F7C27

Quant Time: Dec 16 00:08:01 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Dec 15 01:53:53 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	205219	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	209711	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	91244	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	78494	4.462	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.200%
7) Chloroethane-d5	1.907	69	65465	4.973	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.400%
11) 1,1-Dichloroethene-d2	2.563	65	35655	4.737	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	94.800%
20) 2-Butanone-d5	4.621	46	200091	57.598	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	115.200%
24) Chloroform-d	5.055	84	175696	5.274	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.400%
26) 1,2-Dichloroethane-d4	5.695	65	86506	5.488	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.800%
32) Benzene-d6	5.721	84	324738	4.992	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.800%
36) 1,2-Dichloropropane-d6	6.685	67	106663	5.239	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.800%
41) Toluene-d8	7.894	98	258987	4.455	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.000%
43) trans-1,3-Dichloroprop...	8.177	79	37831	4.792	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.800%
46) 2-Hexanone-d5	8.631	63	149897	50.338	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.680%
56) 1,1,2,2-Tetrachloroeth...	10.749	84	81125	5.507	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	110.200%
66) 1,2-Dichlorobenzene-d4	12.190	152	96996	5.408	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.200%
Target Compounds					Qvalue	
13) Acetone	2.631	43	18852	8.905	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121523\
Data File : VU056898.D
Acq On : 15 Dec 2023 23:15
Operator : MD/SY
Sample : 05809-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7C27

Quant Time: Dec 16 00:08:01 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Dec 15 01:53:53 2023
Response via : Initial Calibration

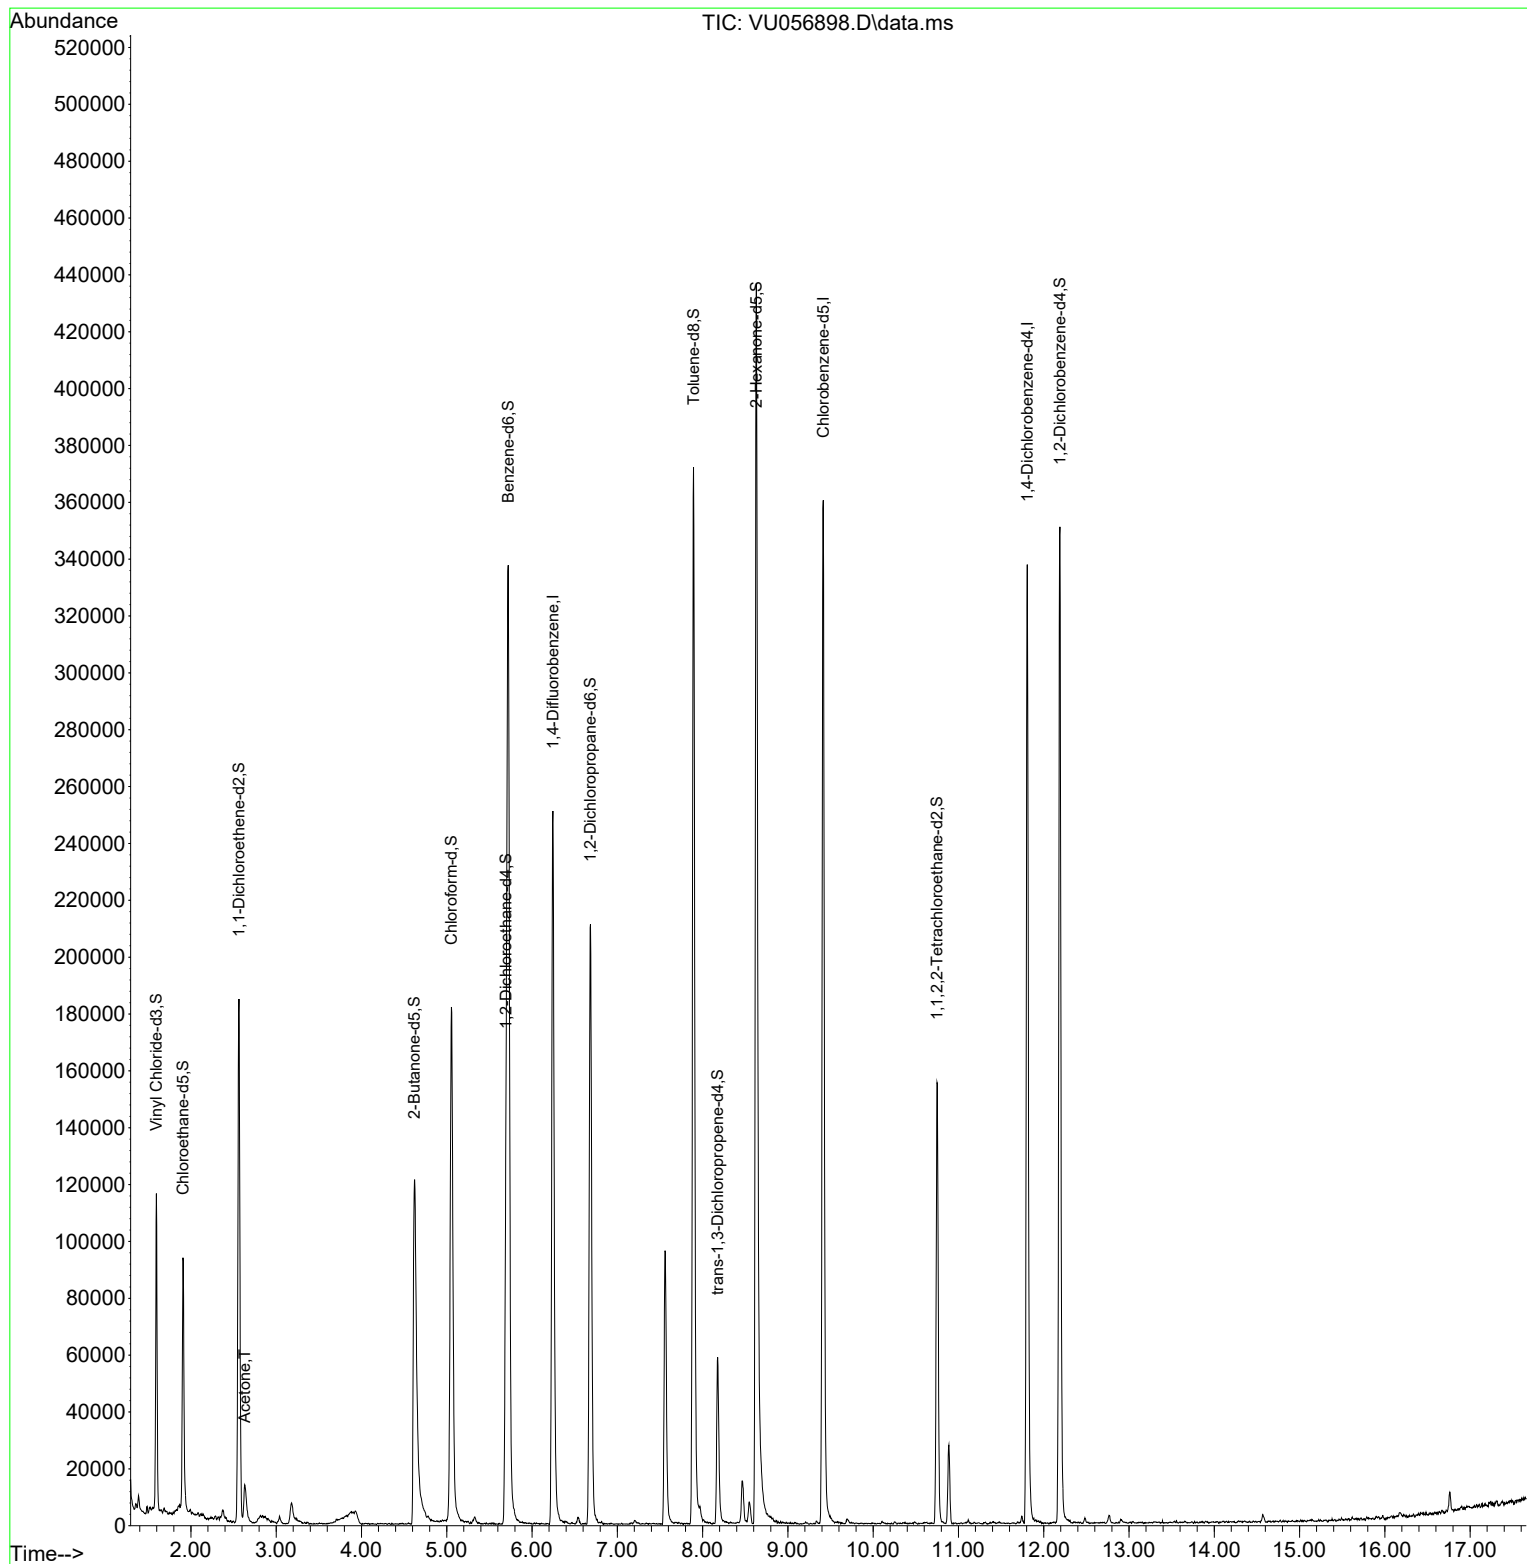

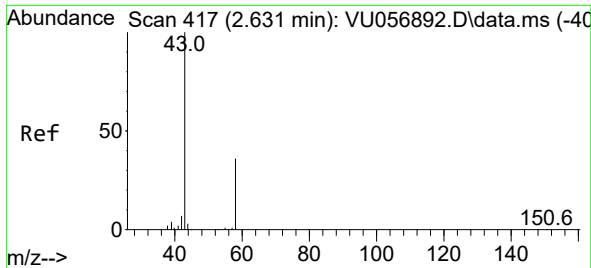

#13

Acetone

Concen: 8.905 ug/L

RT: 2.631 min Scan# 41

Delta R.T. 0.003 min

Lab File: VU056898.D

Acq: 15 Dec 2023 23:15

Instrument :

MSVOA_U

ClientSampleId :

F7C27

Tgt Ion: 43 Resp: 18852

Ion Ratio Lower Upper

43 100

58 35.9 0.0 72.6

