

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121523\
 Data File : VU056903.D
 Acq On : 16 Dec 2023 01:16
 Operator : MD/SY
 Sample : 05809-10
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F7C50

Quant Time: Dec 16 05:13:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Dec 15 01:53:53 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	207698	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	212904	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	89915	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	76116	4.275	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.600%
7) Chloroethane-d5	1.911	69	63381	4.757	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.200%
11) 1,1-Dichloroethene-d2	2.563	65	33010	4.334	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	86.600%
20) 2-Butanone-d5	4.624	46	188101	53.501	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	107.000%
24) Chloroform-d	5.055	84	167933	4.981	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.600%
26) 1,2-Dichloroethane-d4	5.695	65	82319	5.160	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.200%
32) Benzene-d6	5.721	84	308083	4.665	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.400%
36) 1,2-Dichloropropane-d6	6.685	67	100293	4.852	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.000%
41) Toluene-d8	7.894	98	244042	4.135	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.600%
43) trans-1,3-Dichloroprop...	8.177	79	34927	4.357	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.200%
46) 2-Hexanone-d5	8.630	63	141518	46.811	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.620%
56) 1,1,2,2-Tetrachloroeth...	10.749	84	75901	5.075	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	101.600%
66) 1,2-Dichlorobenzene-d4	12.190	152	88532	5.009	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.200%
Target Compounds						Qvalue
13) Acetone	2.637	43	60407	28.193	ug/L	96
21) 2-Butanone	4.734	43	5677	1.571	ug/L	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121523\
Data File : VU056903.D
Acq On : 16 Dec 2023 01:16
Operator : MD/SY
Sample : 05809-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7C50

Quant Time: Dec 16 05:13:02 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Dec 15 01:53:53 2023
Response via : Initial Calibration

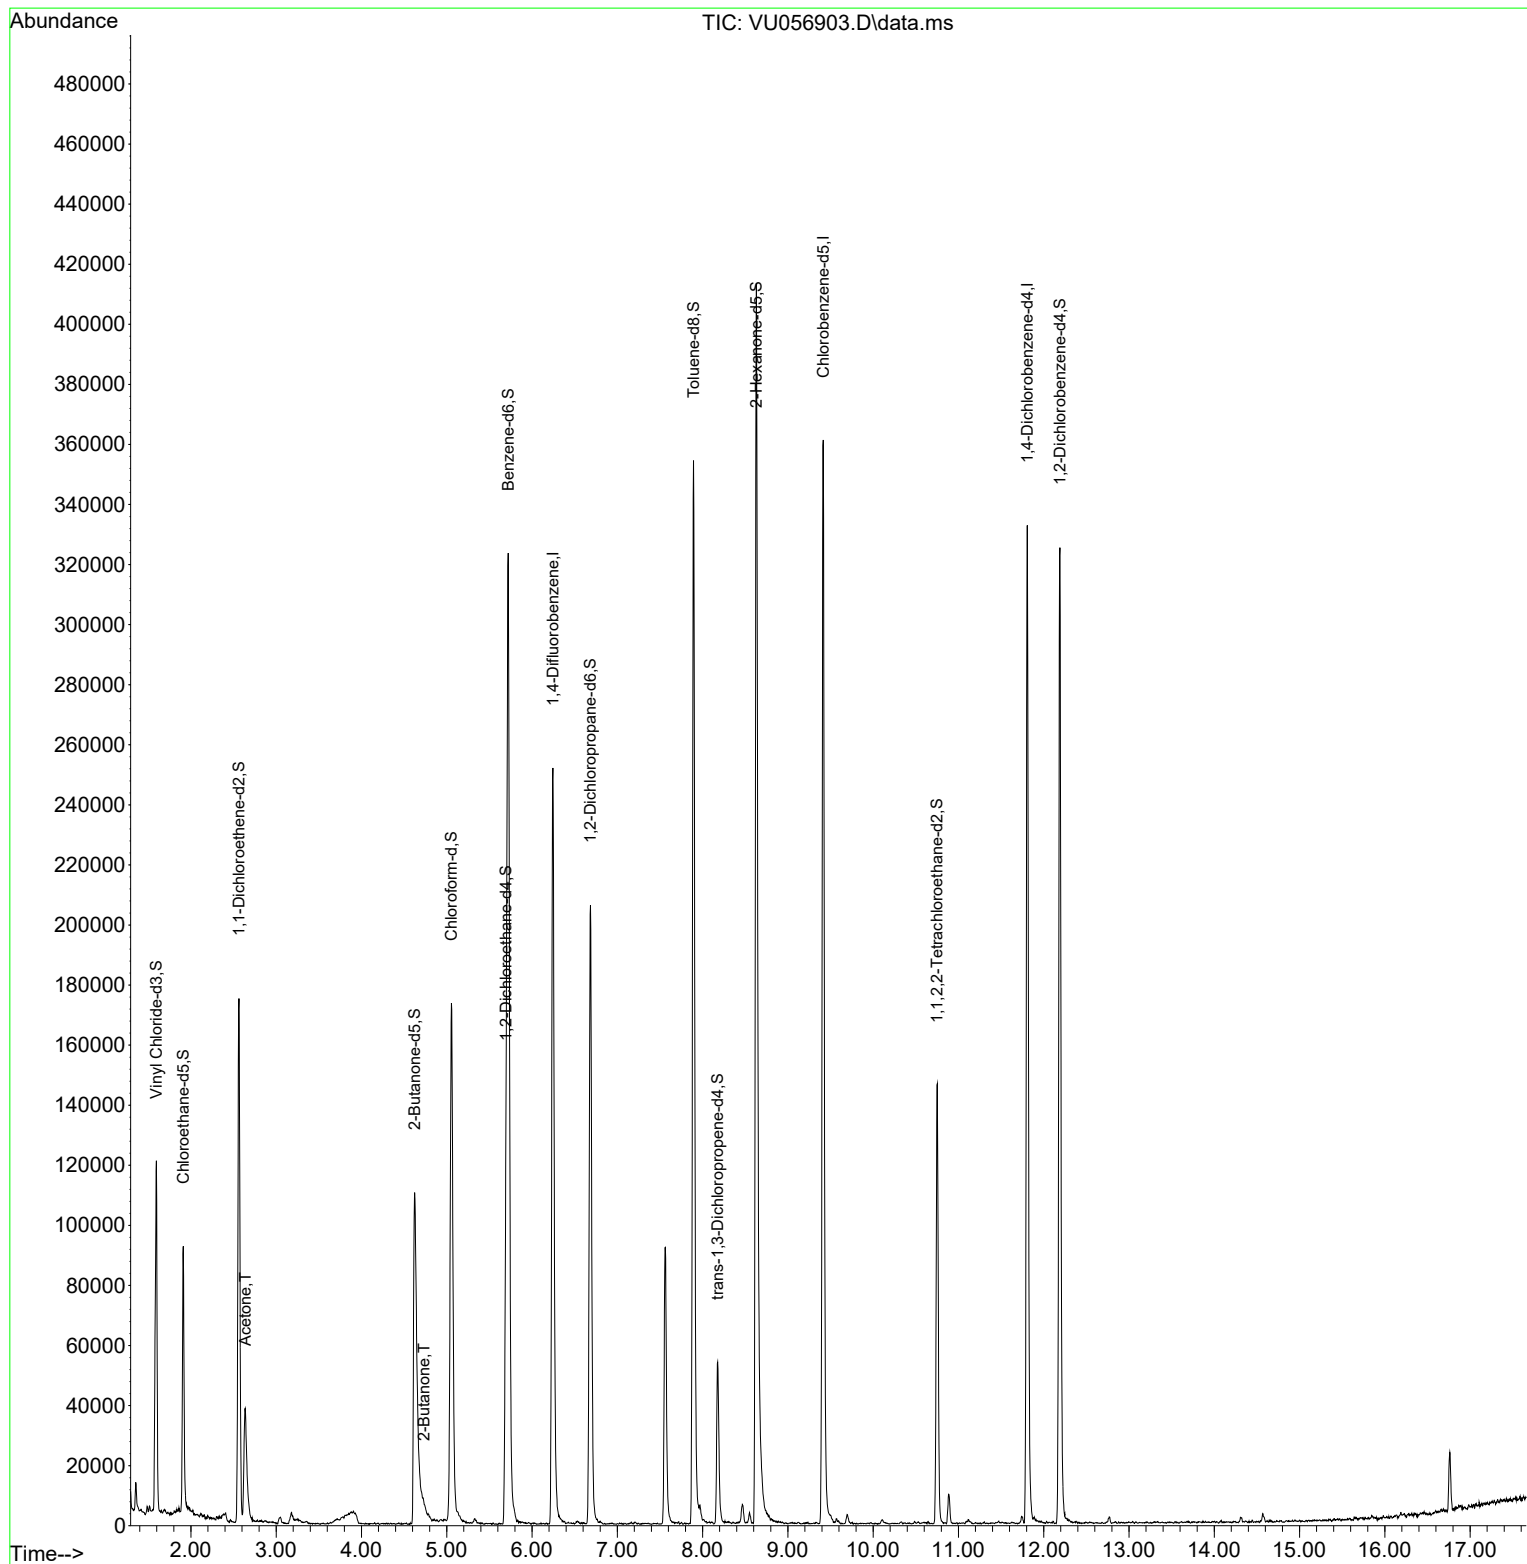

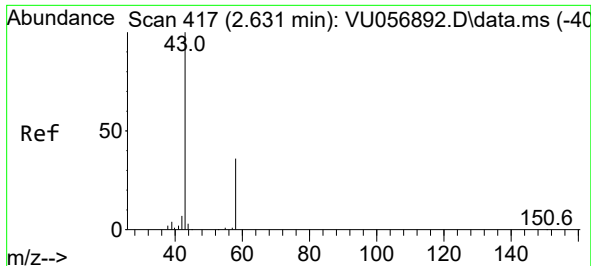

#13

Acetone

Concen: 28.193 ug/L

RT: 2.637 min Scan# 41

Delta R.T. 0.009 min

Lab File: VU056903.D

Acq: 16 Dec 2023 01:16

Instrument :

MSVOA_U

ClientSampleId :





F7C50

Tgt Ion: 43 Resp: 60407

Ion Ratio Lower Upper

43 100

58 33.7 0.0 72.6

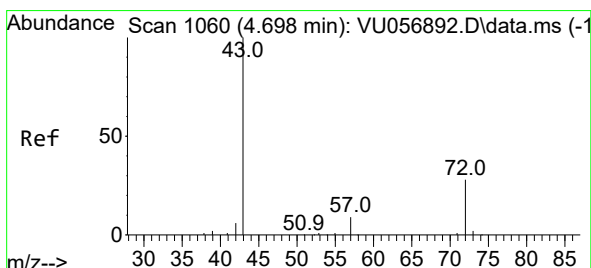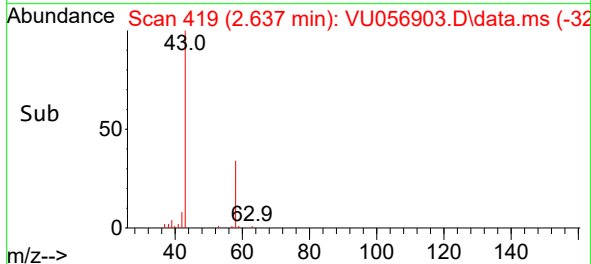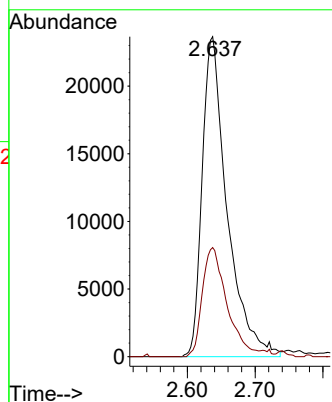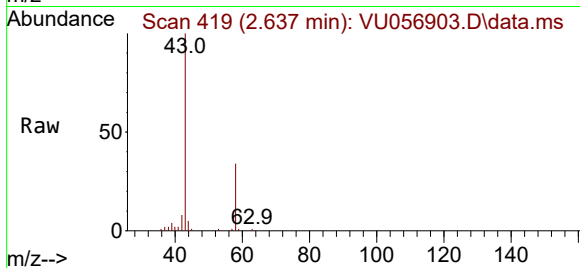

#21

2-Butanone

Concen: 1.571 ug/L

RT: 4.734 min Scan# 1071

Delta R.T. 0.035 min

Lab File: VU056903.D

Acq: 16 Dec 2023 01:16

Tgt Ion: 43 Resp: 5677

Ion Ratio Lower Upper

43 100

72 18.4 14.6 43.8

