

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121523\
 Data File : VU056906.D
 Acq On : 16 Dec 2023 02:29
 Operator : MD/SY
 Sample : 05809-13
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F7C55

Quant Time: Dec 16 05:13:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Dec 15 01:53:53 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	202824	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	214708	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	91059	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	76994	4.429	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.600%
7) Chloroethane-d5	1.911	69	62391	4.796	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.000%
11) 1,1-Dichloroethene-d2	2.563	65	33647	4.523	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	90.400%
20) 2-Butanone-d5	4.621	46	196397	57.203	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	114.400%
24) Chloroform-d	5.055	84	169039	5.135	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.600%
26) 1,2-Dichloroethane-d4	5.695	65	84296	5.411	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.200%
32) Benzene-d6	5.721	84	310604	4.664	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.200%
36) 1,2-Dichloropropane-d6	6.685	67	101654	4.877	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.600%
41) Toluene-d8	7.894	98	246728	4.145	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.000%
43) trans-1,3-Dichloroprop...	8.177	79	34786	4.303	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.000%
46) 2-Hexanone-d5	8.631	63	149818	49.140	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.280%
56) 1,1,2,2-Tetrachloroeth...	10.749	84	78647	5.215	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.200%
66) 1,2-Dichlorobenzene-d4	12.187	152	91471	5.110	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.200%
Target Compounds					Qvalue	
13) Acetone	2.634	43	56280	26.898	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121523\
Data File : VU056906.D
Acq On : 16 Dec 2023 02:29
Operator : MD/SY
Sample : 05809-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7C55

Quant Time: Dec 16 05:13:27 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Dec 15 01:53:53 2023
Response via : Initial Calibration

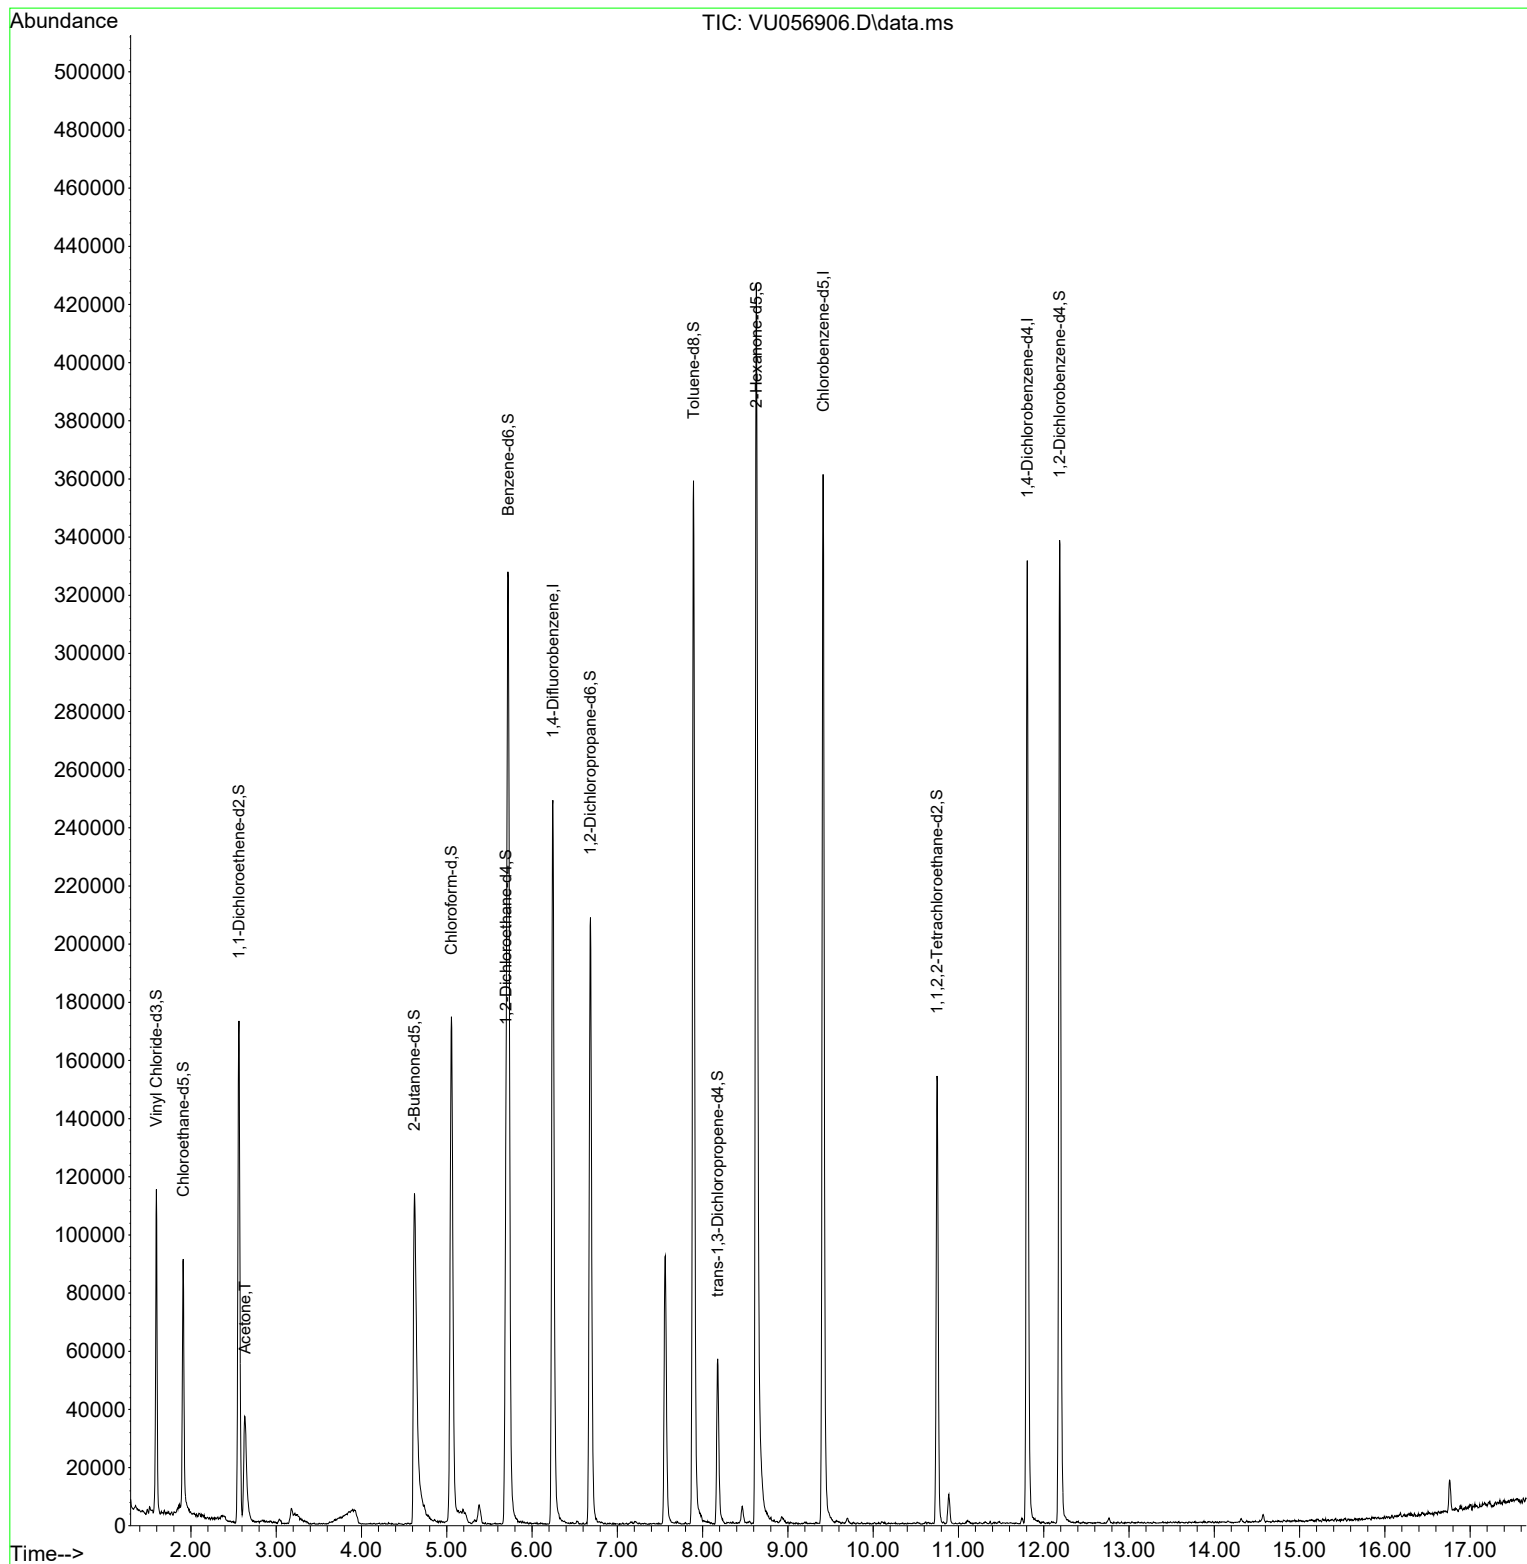

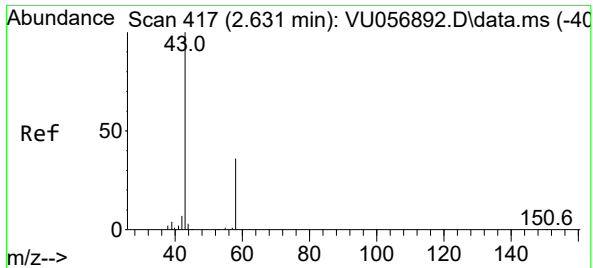

#13
 Acetone
 Concen: 26.898 ug/L
 RT: 2.634 min Scan# 41
 Delta R.T. 0.006 min
 Lab File: VU056906.D
 Acq: 16 Dec 2023 02:29

Instrument :
 MSVOA_U
 ClientSampleId :
 F7C55

Tgt Ion: 43 Resp: 56280
 Ion Ratio Lower Upper
 43 100
 58 34.5 0.0 72.6

