

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121523\
 Data File : VU056871.D
 Acq On : 15 Dec 2023 11:55
 Operator : MD/SY
 Sample : 05675-23
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU056871.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	86	95	109	rBV	135025	153044	16.19%	2.003%
2	1.911	185	193	212	rVB	98821	135281	14.31%	1.771%
3	2.564	383	396	418	rBV	214605	353914	37.43%	4.632%
4	3.043	534	545	560	rBV3	16014	31620	3.34%	0.414%
5	4.628	1027	1038	1075	rBV2	109654	328080	34.70%	4.294%
6	5.055	1154	1171	1200	rBV	190171	429252	45.40%	5.618%
7	5.721	1358	1378	1398	rBV2	368031	945521	100.00%	12.375%
8	6.245	1528	1541	1565	rBV	293706	582244	61.58%	7.621%
9	6.682	1663	1677	1700	rBV2	223600	448367	47.42%	5.868%
10	7.560	1937	1950	1977	rBV	105921	197247	20.86%	2.582%
11	7.895	2041	2054	2090	rBV	412234	755159	79.87%	9.884%
12	8.177	2128	2142	2163	rBV	61929	113004	11.95%	1.479%
13	8.470	2222	2233	2241	rBV3	5805	9466	1.00%	0.124%
14	8.631	2271	2283	2314	rBV2	422115	867718	91.77%	11.357%
15	9.415	2514	2527	2569	rBV	409718	746209	78.92%	9.767%
16	10.750	2930	2942	2963	rBV	154690	255812	27.06%	3.348%
17	10.888	2969	2985	2995	rVB2	6228	11394	1.21%	0.149%
18	11.808	3260	3271	3290	rBV	388485	647029	68.43%	8.469%
19	12.190	3377	3390	3408	rBV	368475	629950	66.62%	8.245%




Sum of corrected areas: 7640311

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121523\
Data File : VU056871.D
Acq On : 15 Dec 2023 11:55
Operator : MD/SY
Sample : 05675-23
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

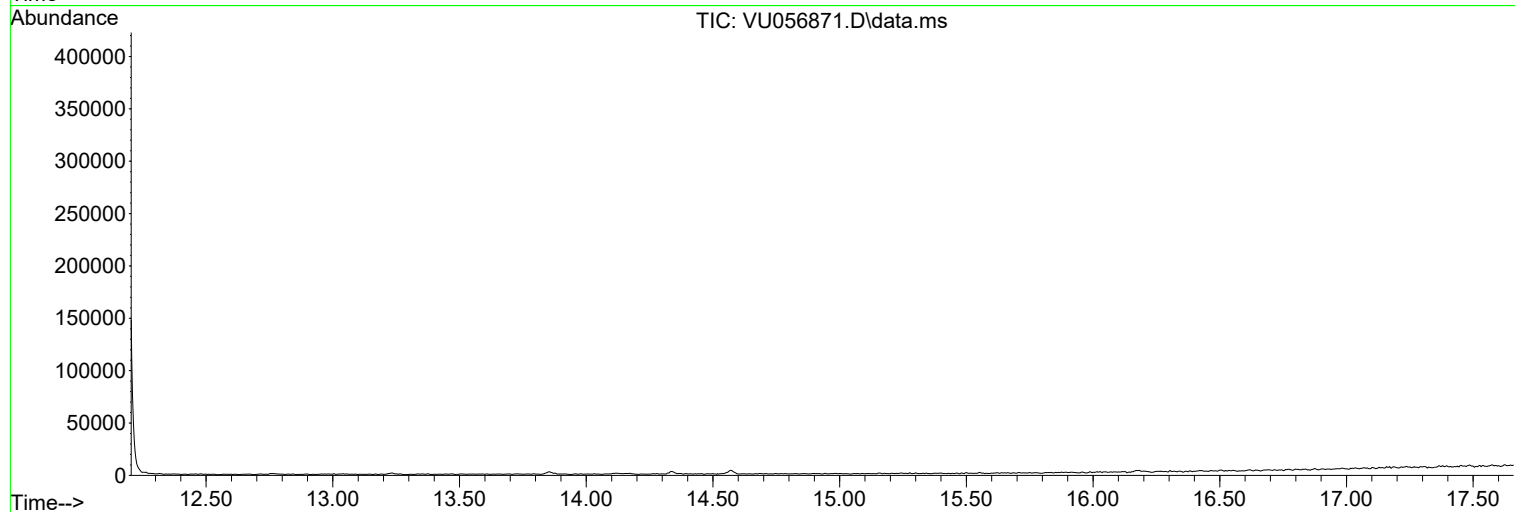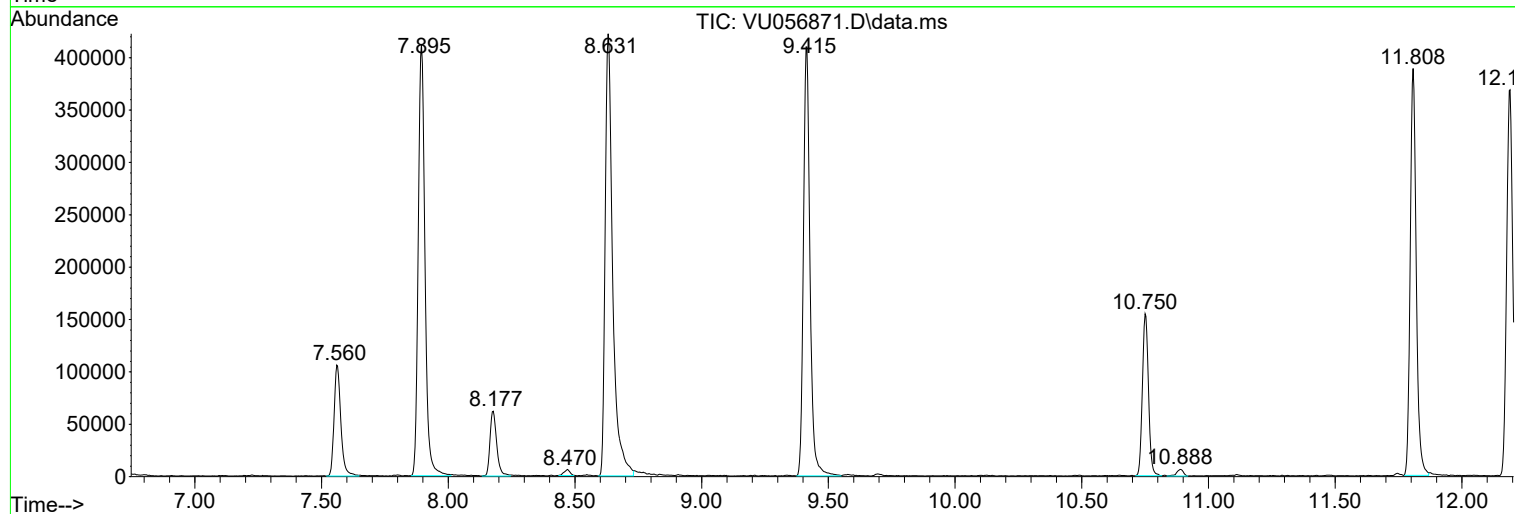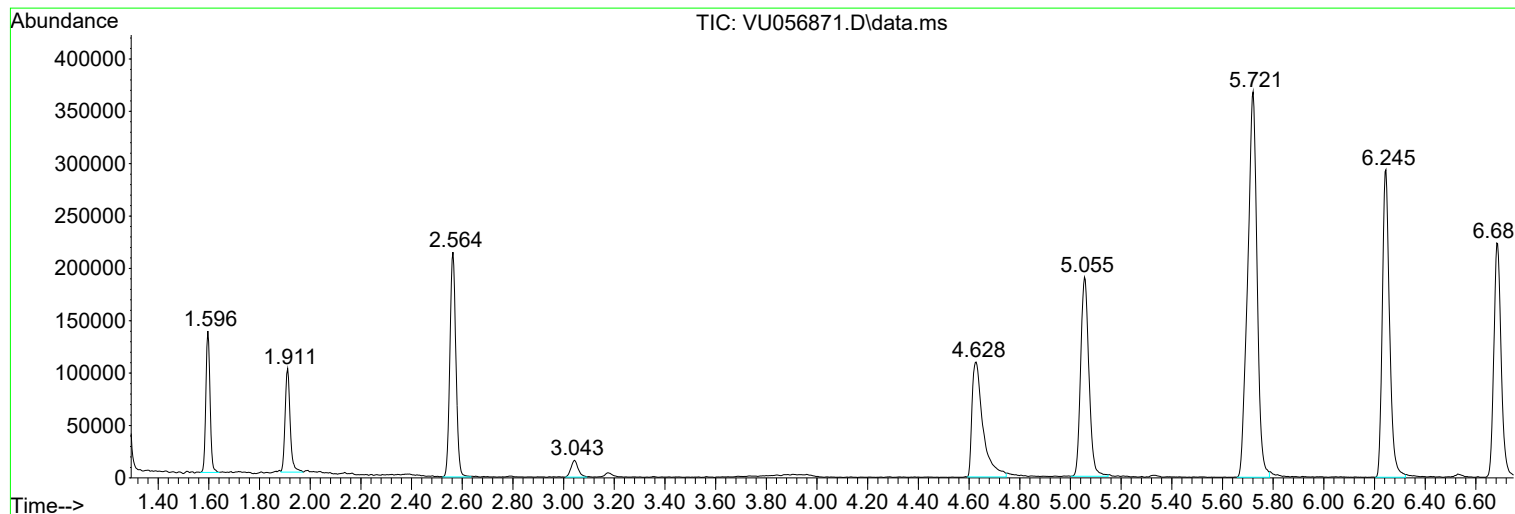

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121523\
Data File : VU056871.D
Acq On : 15 Dec 2023 11:55
Operator : MD/SY
Sample : 05675-23
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121523\
Data File : VU056871.D
Acq On : 15 Dec 2023 11:55
Operator : MD/SY
Sample : 05675-23
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc