

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121523\
 Data File : VU056877.D
 Acq On : 15 Dec 2023 14:21
 Operator : MD/SY
 Sample : 05677-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H0AC8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU056877.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	104	rBV	126721	143235	12.58%	1.489%
2	1.727	129	136	145	rVB	18351	22211	1.95%	0.231%
3	1.907	184	192	207	rVB	97150	134416	11.81%	1.397%
4	2.563	383	396	413	rBV2	215855	379184	33.30%	3.942%
5	3.184	576	589	604	rBV2	5364	12810	1.13%	0.133%
6	4.621	1024	1036	1083	rBV	118851	338248	29.71%	3.516%
7	5.055	1155	1171	1195	rBV2	187635	419593	36.85%	4.362%
8	5.721	1357	1378	1403	rBV2	364019	931201	81.79%	9.680%
9	6.245	1528	1541	1565	rBV	272872	539056	47.35%	5.603%
10	6.537	1617	1632	1660	rBV	563372	1084510	95.25%	11.273%
11	6.685	1665	1678	1698	rVV	219555	438641	38.53%	4.560%
12	7.560	1939	1950	1971	rBV	104338	189063	16.61%	1.965%
13	7.894	2041	2054	2073	rBV	400042	725257	63.70%	7.539%
14	8.177	2131	2142	2165	rBV2	61808	112232	9.86%	1.167%
15	8.547	2244	2257	2273	rBV	656018	1138569	100.00%	11.835%
16	8.631	2273	2283	2315	rVB2	430540	844450	74.17%	8.778%
17	9.415	2513	2527	2550	rBV	393483	693461	60.91%	7.208%
18	10.750	2929	2942	2965	rBV	152031	252366	22.17%	2.623%
19	11.807	3258	3271	3292	rBV	358077	601608	52.84%	6.254%
20	12.187	3377	3389	3410	rBV	355930	619956	54.45%	6.444%




Sum of corrected areas: 9620067

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121523\
Data File : VU056877.D
Acq On : 15 Dec 2023 14:21
Operator : MD/SY
Sample : 05677-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AC8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

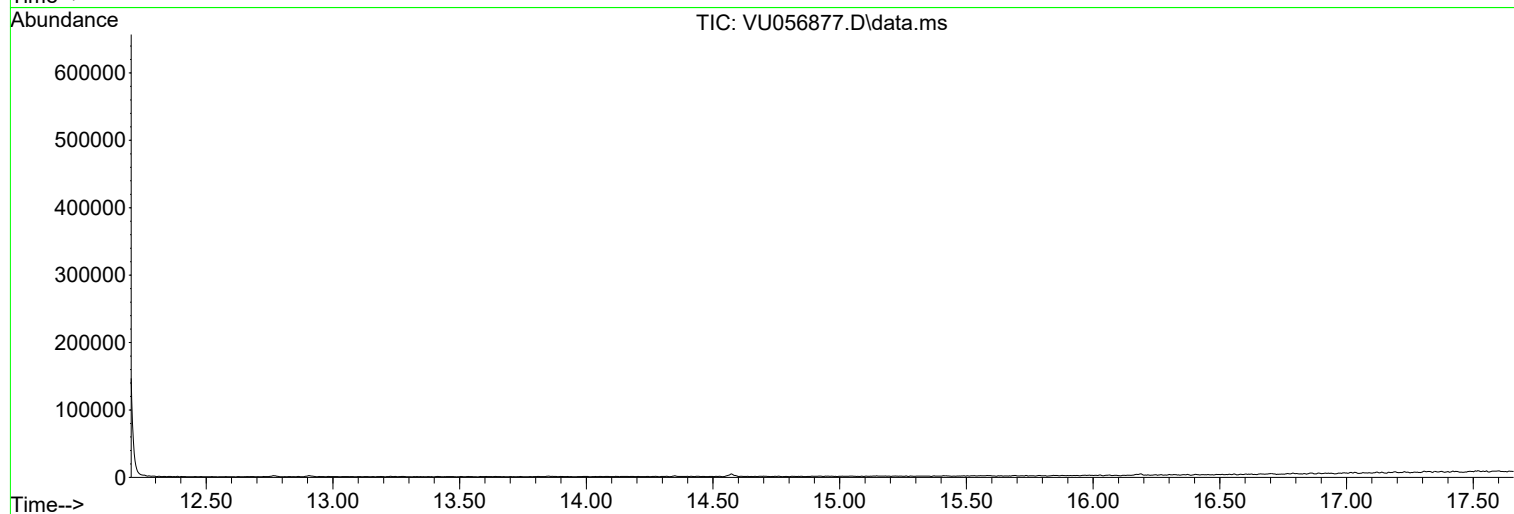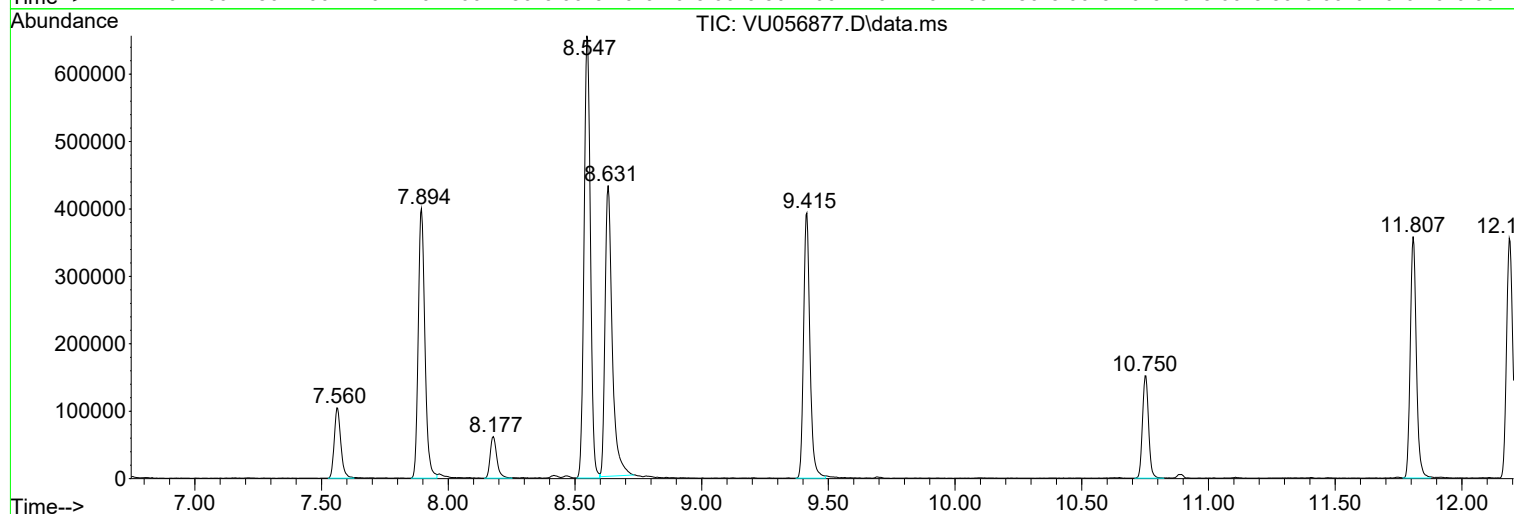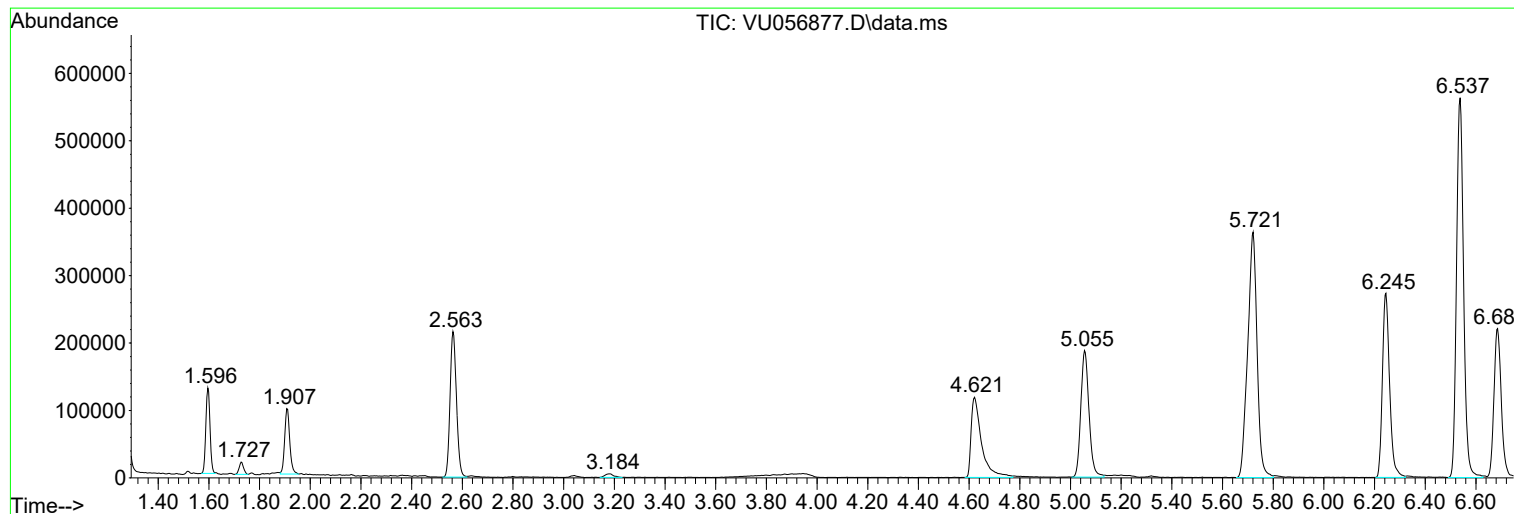

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121523\
Data File : VU056877.D
Acq On : 15 Dec 2023 14:21
Operator : MD/SY
Sample : 05677-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AC8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121523\
Data File : VU056877.D
Acq On : 15 Dec 2023 14:21
Operator : MD/SY
Sample : 05677-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AC8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc