

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121523\
 Data File : VU056878.D
 Acq On : 15 Dec 2023 14:46
 Operator : MD/SY
 Sample : 05677-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H0AD8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU056878.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	87	95	109	rVB	124417	141903	6.21%	1.337%
2	1.727	129	136	144	rVB	22046	28325	1.24%	0.267%
3	1.910	183	193	209	rBV	93494	127518	5.58%	1.201%
4	2.563	382	396	412	rBV3	223935	414874	18.15%	3.908%
5	4.624	1021	1037	1071	rBV2	117720	444566	19.45%	4.188%
6	5.055	1156	1171	1196	rBV	182193	421837	18.46%	3.974%
7	5.721	1357	1378	1404	rBV2	346421	908201	39.73%	8.555%
8	6.245	1527	1541	1568	rBV	283317	561367	24.56%	5.288%
9	6.537	1616	1632	1653	rBV	420645	806943	35.30%	7.601%
10	6.685	1665	1678	1703	rVB	215759	431262	18.87%	4.062%
11	7.563	1939	1951	1972	rBV	99686	182174	7.97%	1.716%
12	7.894	2041	2054	2073	rBV	393925	705519	30.87%	6.646%
13	8.177	2131	2142	2158	rBV2	61019	107762	4.71%	1.015%
14	8.547	2243	2257	2273	rBV	1332539	2285753	100.00%	21.531%
15	8.630	2273	2283	2310	rVB2	424157	825767	36.13%	7.779%
16	9.412	2513	2526	2556	rBV	407461	724313	31.69%	6.823%
17	10.749	2930	2942	2960	rBV	147532	244259	10.69%	2.301%
18	10.888	2975	2985	2996	rVB3	13810	23015	1.01%	0.217%
19	11.807	3260	3271	3294	rBV	374878	626368	27.40%	5.900%
20	12.187	3376	3389	3409	rBV	347702	604232	26.43%	5.692%




Sum of corrected areas: 10615958

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121523\
Data File : VU056878.D
Acq On : 15 Dec 2023 14:46
Operator : MD/SY
Sample : 05677-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AD8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

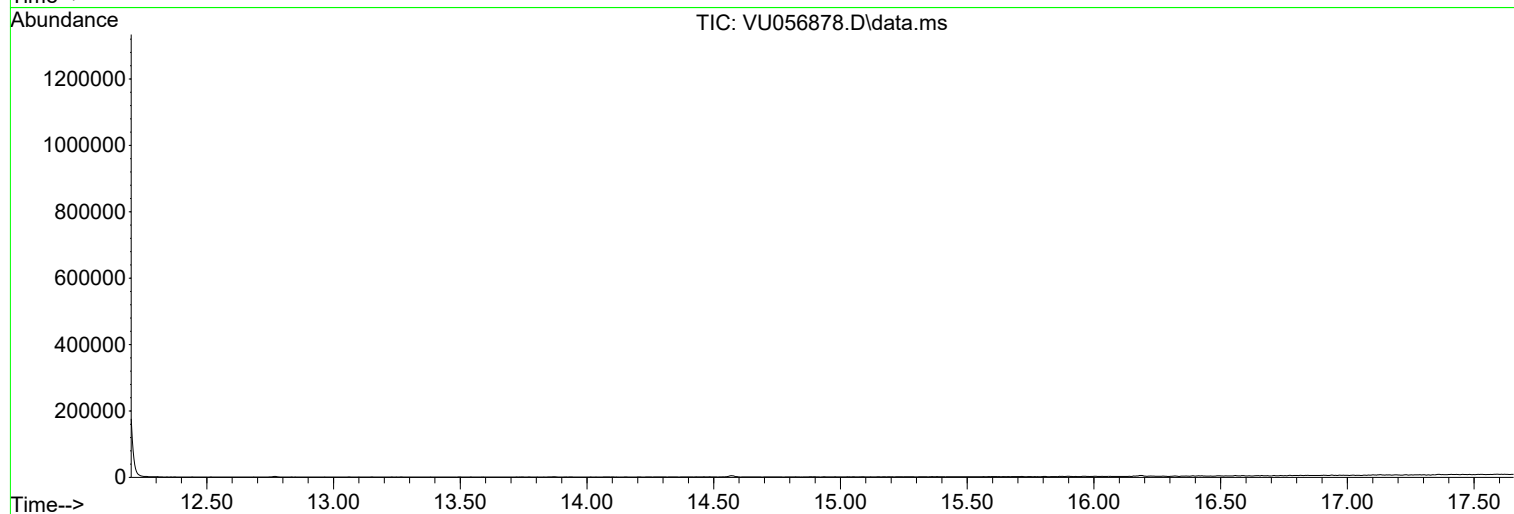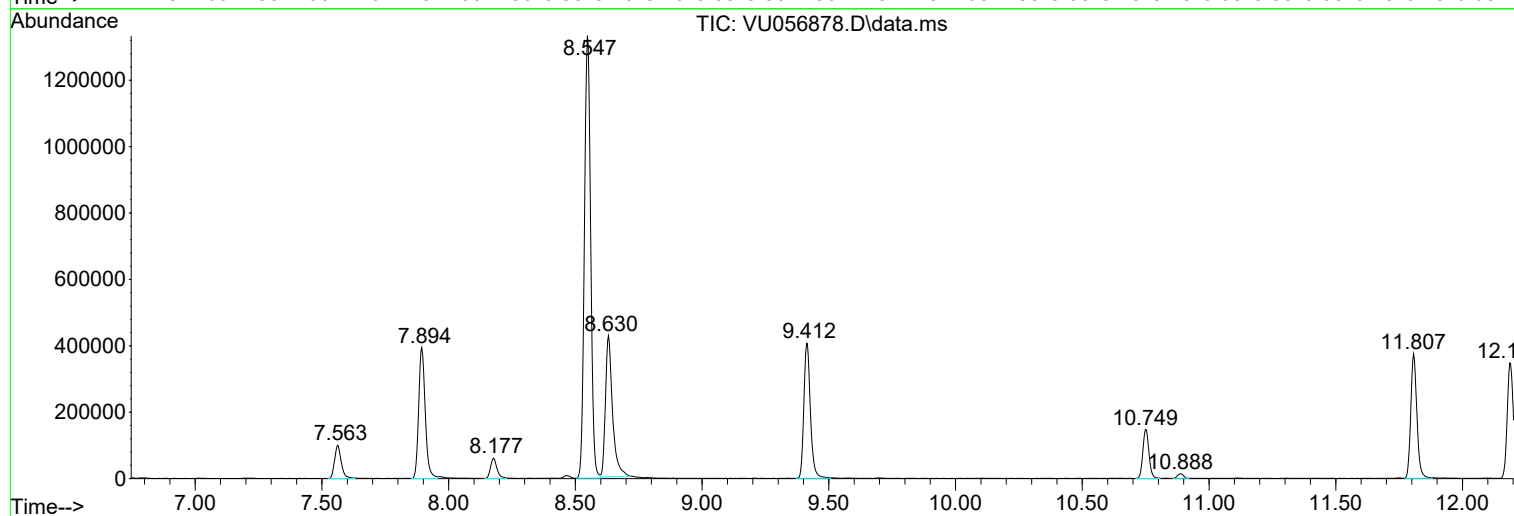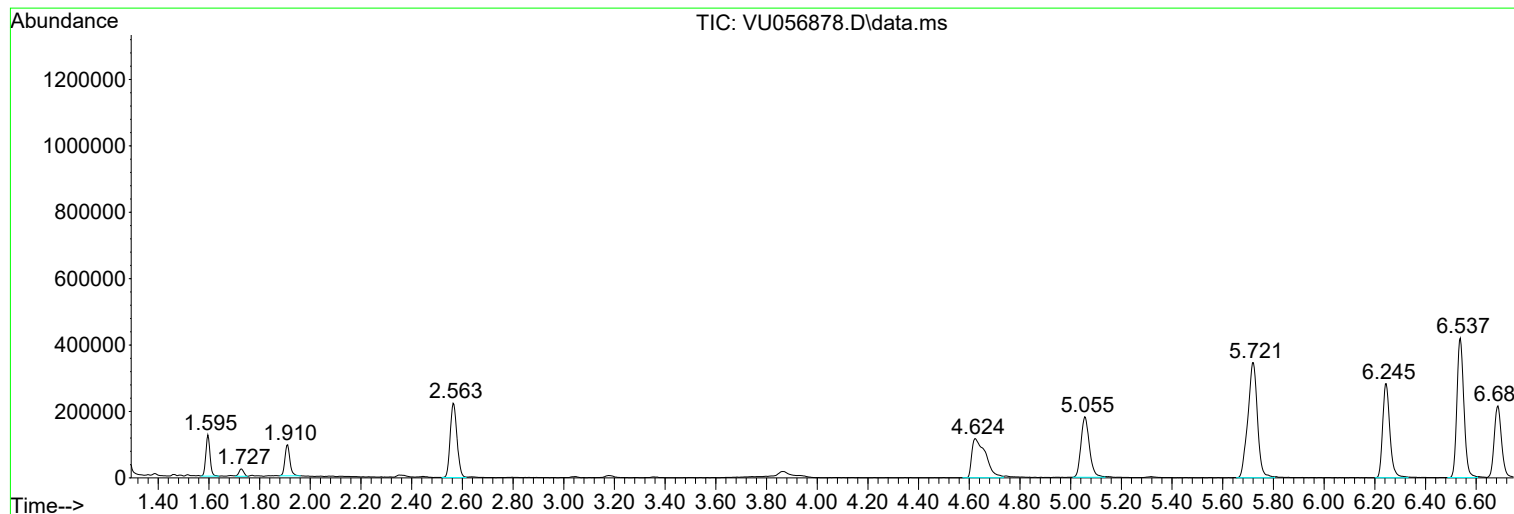

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121523\
Data File : VU056878.D
Acq On : 15 Dec 2023 14:46
Operator : MD/SY
Sample : 05677-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AD8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121523\
Data File : VU056878.D
Acq On : 15 Dec 2023 14:46
Operator : MD/SY
Sample : 05677-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AD8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc