

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121523\
 Data File : VU056882.D
 Acq On : 15 Dec 2023 16:23
 Operator : MD/SY
 Sample : 05799-20
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU056882.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	108	rVB	118705	135014	15.03%	1.863%
2	1.907	184	192	207	rVB	92098	127402	14.18%	1.758%
3	2.563	383	396	410	rBV	193032	315148	35.08%	4.348%
4	3.042	529	545	559	rBV3	14622	30082	3.35%	0.415%
5	3.174	572	586	598	rBV3	3909	9426	1.05%	0.130%
6	4.621	1023	1036	1068	rBV	114846	317400	35.33%	4.379%
7	5.055	1154	1171	1195	rBV	183530	412312	45.90%	5.689%
8	5.718	1357	1377	1403	rBV3	338379	898318	100.00%	12.394%
9	6.245	1527	1541	1566	rBV	264668	521871	58.09%	7.200%
10	6.685	1661	1678	1700	rBV	213313	427632	47.60%	5.900%
11	7.563	1938	1951	1969	rBV	98632	182286	20.29%	2.515%
12	7.894	2041	2054	2077	rBV	383282	691276	76.95%	9.537%
13	8.177	2131	2142	2160	rBV	59805	106423	11.85%	1.468%
14	8.631	2270	2283	2325	rBV2	415267	844685	94.03%	11.654%
15	9.412	2514	2526	2555	rBV	373515	670441	74.63%	9.250%
16	10.753	2931	2943	2960	rBV	148934	247159	27.51%	3.410%
17	11.746	3243	3252	3260	rBV3	11552	18070	2.01%	0.249%
18	11.807	3260	3271	3298	rVB	352652	628197	69.93%	8.667%
19	12.190	3377	3390	3413	rBV	356012	645199	71.82%	8.902%
20	16.762	4802	4812	4824	rBV9	12509	19765	2.20%	0.273%




Sum of corrected areas: 7248106

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121523\
Data File : VU056882.D
Acq On : 15 Dec 2023 16:23
Operator : MD/SY
Sample : 05799-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

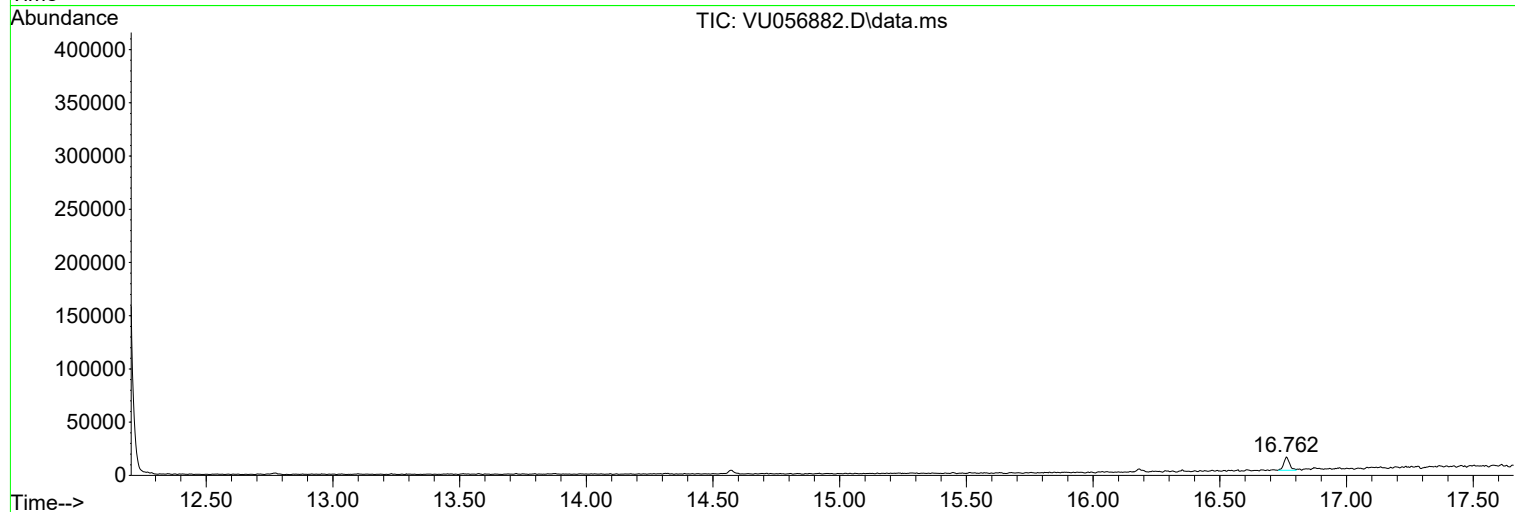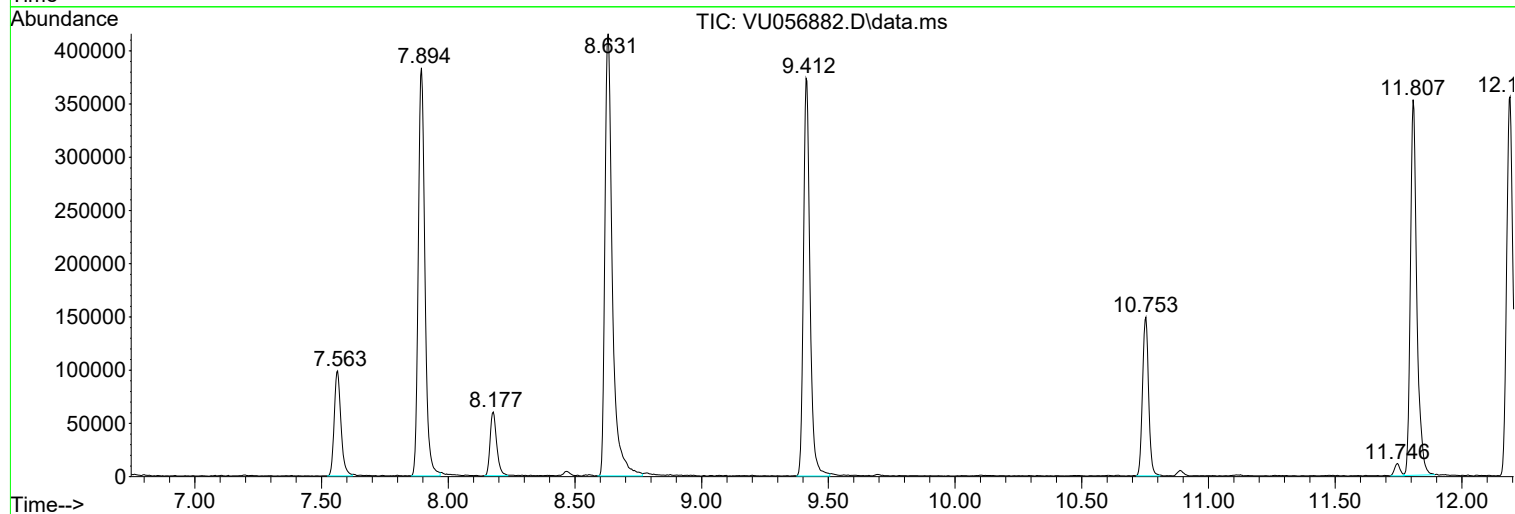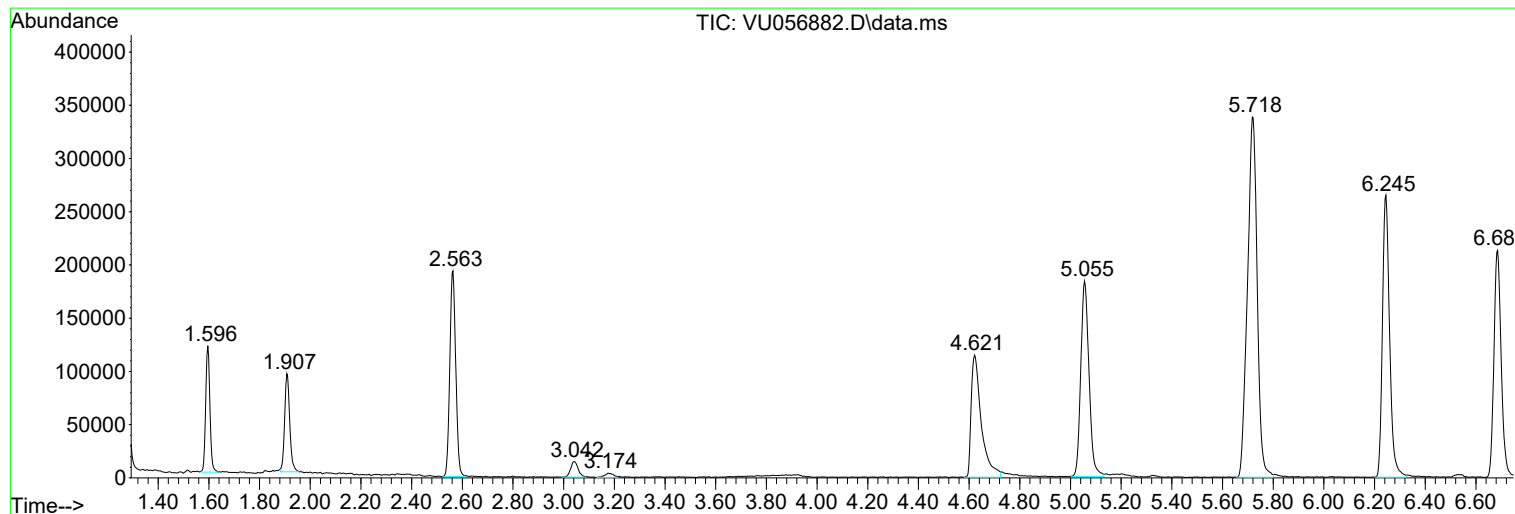

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121523\
Data File : VU056882.D
Acq On : 15 Dec 2023 16:23
Operator : MD/SY
Sample : 05799-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121523\
Data File : VU056882.D
Acq On : 15 Dec 2023 16:23
Operator : MD/SY
Sample : 05799-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc