

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121523\
 Data File : VU056887.D
 Acq On : 15 Dec 2023 18:25
 Operator : MD/SY
 Sample : 05770-23
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU056887.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	84	95	109	rVB	120014	150858	16.72%	2.109%
2	1.907	184	192	205	rVB	93317	125429	13.90%	1.754%
3	2.563	383	396	411	rBV	187582	312478	34.64%	4.369%
4	4.621	1022	1036	1066	rBV	116752	323667	35.88%	4.525%
5	4.824	1089	1099	1117	rVB3	3673	10095	1.12%	0.141%
6	5.055	1155	1171	1193	rBV	182925	410800	45.54%	5.744%
7	5.721	1357	1378	1415	rBV2	339306	902076	100.00%	12.613%
8	6.245	1527	1541	1569	rBV	260999	510706	56.61%	7.141%
9	6.685	1664	1678	1699	rBV2	215244	427925	47.44%	5.983%
10	7.560	1938	1950	1972	rBV2	97810	183279	20.32%	2.563%
11	7.791	2013	2022	2037	rBV4	4592	9927	1.10%	0.139%
12	7.894	2041	2054	2073	rBV	373739	682694	75.68%	9.545%
13	8.174	2131	2141	2162	rBV	60258	108989	12.08%	1.524%
14	8.466	2223	2232	2244	rVB3	12960	21960	2.43%	0.307%
15	8.630	2271	2283	2315	rBV	424204	851525	94.40%	11.906%
16	9.415	2514	2527	2552	rBV	369356	656137	72.74%	9.174%
17	10.749	2931	2942	2961	rVB	150329	250692	27.79%	3.505%
18	10.888	2974	2985	2998	rVB2	20983	33321	3.69%	0.466%
19	11.807	3259	3271	3295	rBV	338927	567700	62.93%	7.937%
20	12.187	3377	3389	3407	rBV	359583	611869	67.83%	8.555%




Sum of corrected areas: 7152127

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121523\
Data File : VU056887.D
Acq On : 15 Dec 2023 18:25
Operator : MD/SY
Sample : 05770-23
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

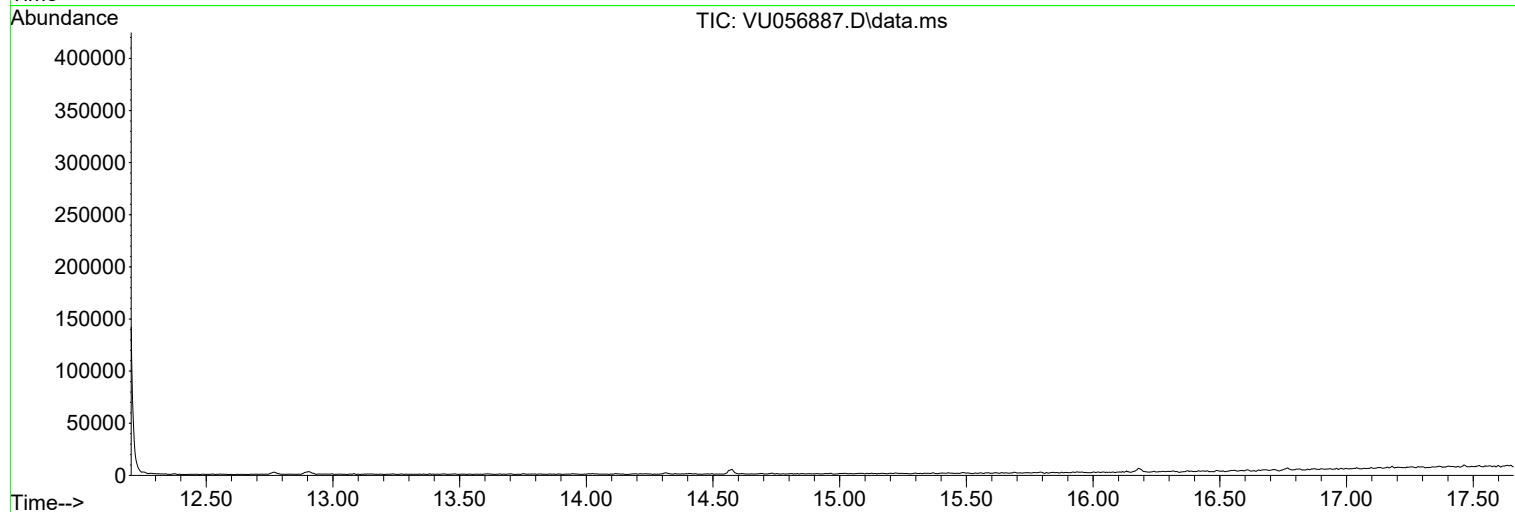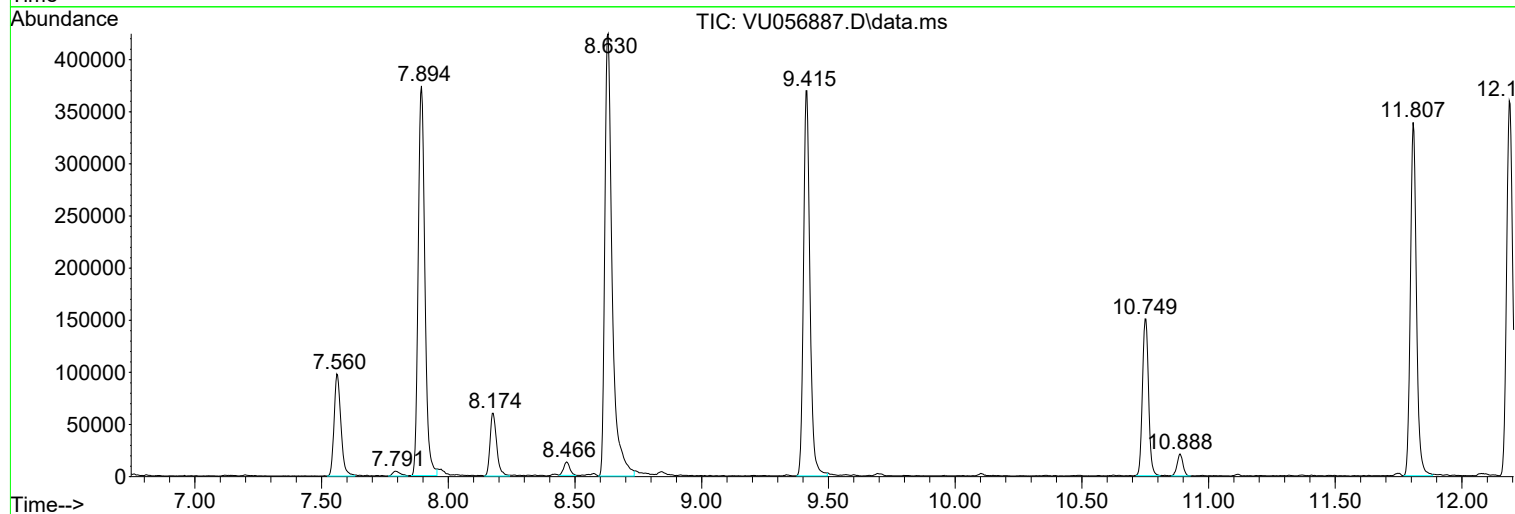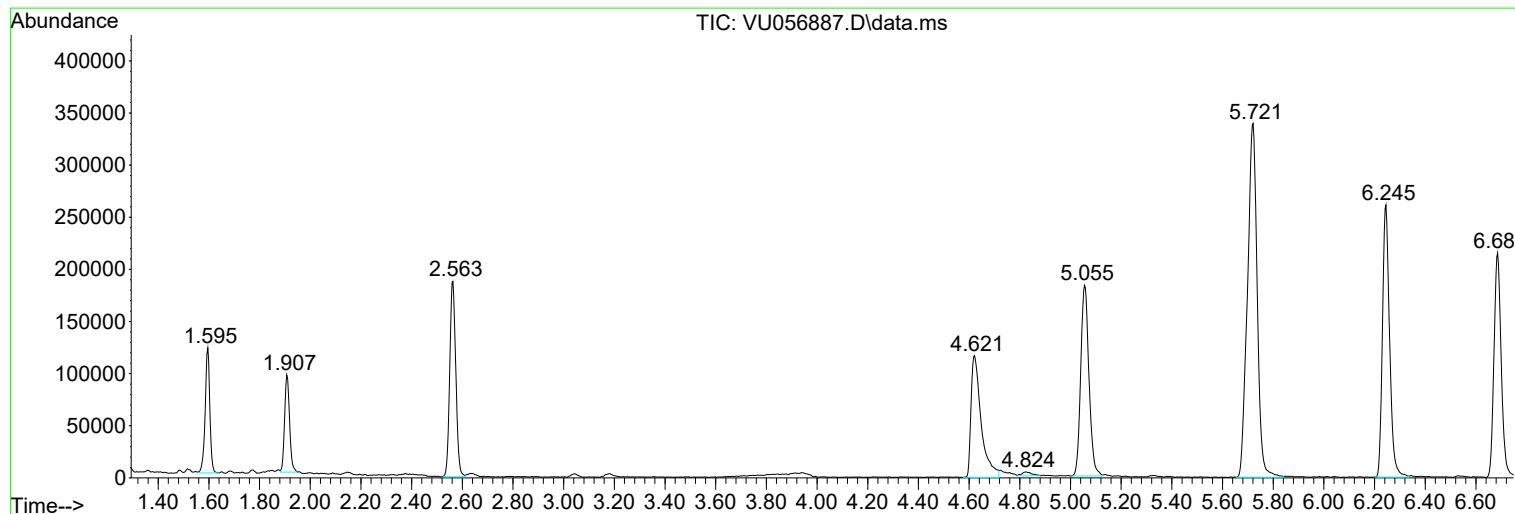

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121523\
Data File : VU056887.D
Acq On : 15 Dec 2023 18:25
Operator : MD/SY
Sample : 05770-23
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121523\
Data File : VU056887.D
Acq On : 15 Dec 2023 18:25
Operator : MD/SY
Sample : 05770-23
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc