

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121523\
 Data File : VU056901.D
 Acq On : 16 Dec 2023 00:28
 Operator : MD/SY
 Sample : 05809-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F7C30

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU056901.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	107	rVB	112314	127992	14.39%	1.822%
2	1.907	184	192	206	rBV	83897	111147	12.49%	1.583%
3	2.560	383	395	411	rBV	183572	302055	33.95%	4.301%
4	3.181	574	588	595	rBV	7220	14853	1.67%	0.211%
5	4.624	1021	1037	1070	rBV	115870	331161	37.22%	4.715%
6	5.055	1153	1171	1194	rBV2	182693	404721	45.49%	5.763%
7	5.721	1358	1378	1413	rBV2	339179	889640	100.00%	12.667%
8	6.245	1526	1541	1565	rBV	249717	495426	55.69%	7.054%
9	6.685	1664	1678	1698	rBV	214692	427498	48.05%	6.087%
10	7.560	1936	1950	1973	rBV2	96337	177553	19.96%	2.528%
11	7.894	2040	2054	2075	rBV	368043	669704	75.28%	9.536%
12	8.177	2130	2142	2161	rBV	59322	106286	11.95%	1.513%
13	8.467	2217	2232	2241	rBV2	9165	16998	1.91%	0.242%
14	8.631	2272	2283	2318	rBV2	434227	877538	98.64%	12.495%
15	9.412	2514	2526	2560	rBV	353982	638490	71.77%	9.091%
16	10.750	2931	2942	2957	rBV	152565	255958	28.77%	3.645%
17	10.888	2974	2985	2994	rBV3	15809	25288	2.84%	0.360%
18	11.807	3259	3271	3296	rBV	337231	553949	62.27%	7.888%
19	12.190	3377	3390	3410	rBV	348905	596803	67.08%	8.498%




Sum of corrected areas: 7023060

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121523\
Data File : VU056901.D
Acq On : 16 Dec 2023 00:28
Operator : MD/SY
Sample : 05809-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7C30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

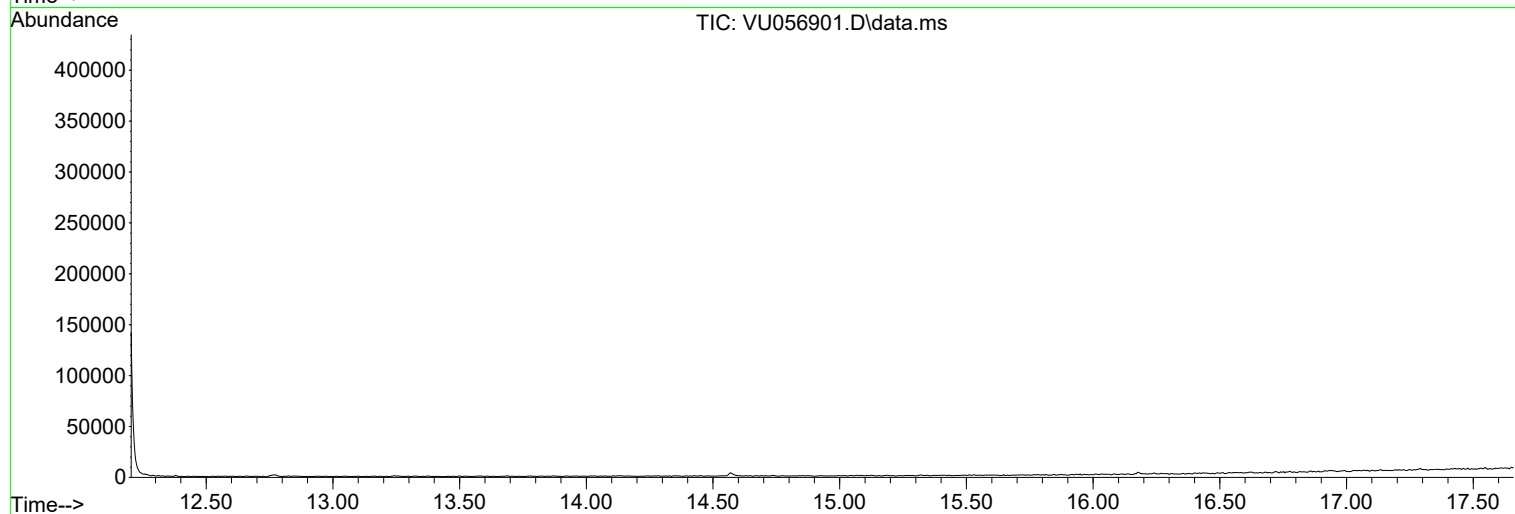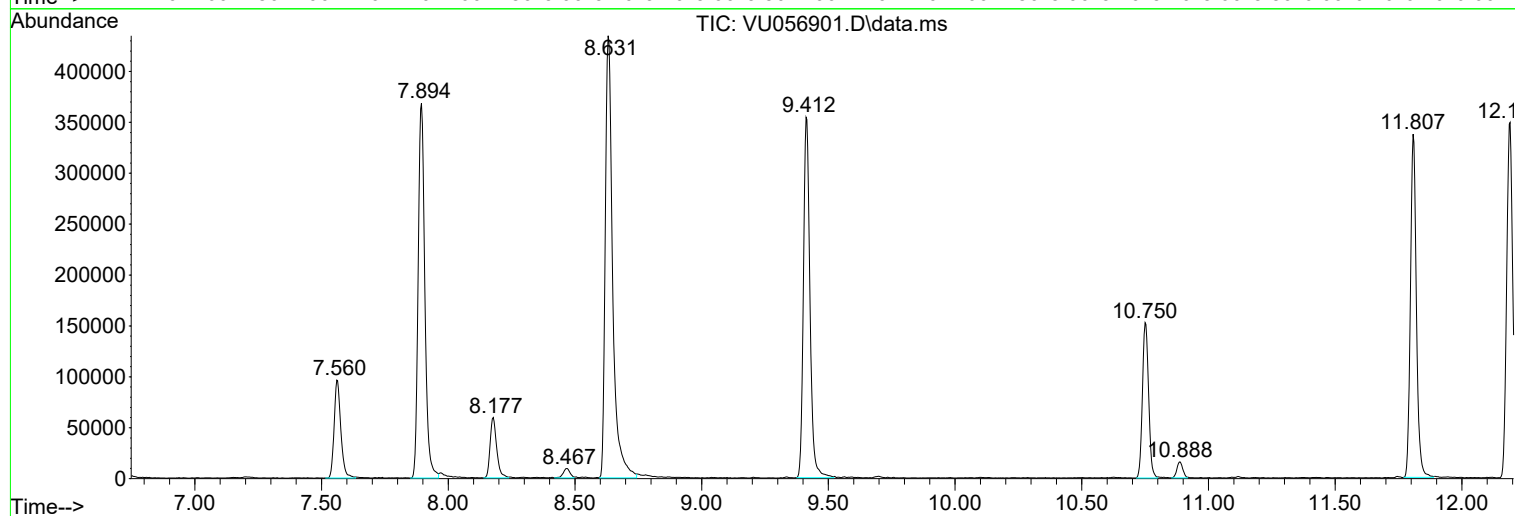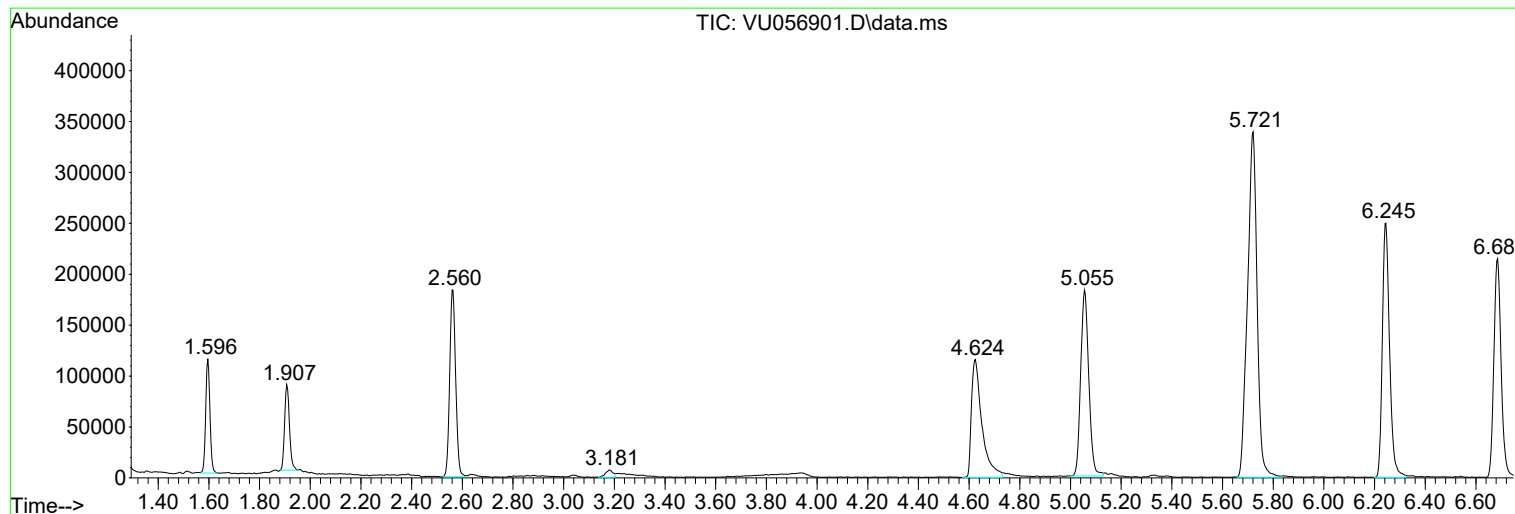

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121523\
Data File : VU056901.D
Acq On : 16 Dec 2023 00:28
Operator : MD/SY
Sample : 05809-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7C30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121523\
Data File : VU056901.D
Acq On : 16 Dec 2023 00:28
Operator : MD/SY
Sample : 05809-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7C30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc