

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121523\
 Data File : VU056904.D
 Acq On : 16 Dec 2023 01:41
 Operator : MD/SY
 Sample : 05809-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F7C51

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU056904.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	84	95	107	rVB	111195	130725	15.45%	1.883%
2	1.911	183	193	204	rBV	85566	117645	13.90%	1.695%
3	2.563	384	396	408	rBV	180226	293387	34.68%	4.226%
4	2.634	408	418	441	rVB	51003	119403	14.11%	1.720%
5	4.624	1024	1037	1071	rBV	108096	326613	38.60%	4.705%
6	5.055	1153	1171	1194	rBV	170301	392636	46.41%	5.656%
7	5.721	1358	1378	1401	rBV2	321695	844112	99.77%	12.160%
8	6.245	1525	1541	1561	rBV	249265	492041	58.15%	7.088%
9	6.685	1664	1678	1702	rBV	204721	413692	48.89%	5.960%
10	7.560	1938	1950	1971	rBV2	90698	170263	20.12%	2.453%
11	7.894	2040	2054	2085	rBV	352200	648342	76.63%	9.340%
12	8.177	2131	2142	2167	rBV2	56032	101089	11.95%	1.456%
13	8.630	2268	2283	2329	rBV2	409057	846098	100.00%	12.189%
14	9.412	2513	2526	2546	rBV	361085	633469	74.87%	9.126%
15	10.749	2930	2942	2964	rBV	149371	246753	29.16%	3.555%
16	10.888	2972	2985	2997	rVB4	8497	15080	1.78%	0.217%
17	11.807	3259	3271	3295	rBV	330784	557417	65.88%	8.030%
18	12.190	3373	3390	3411	rBV	336917	573666	67.80%	8.264%
19	16.762	4804	4812	4821	rVB7	12539	19253	2.28%	0.277%




Sum of corrected areas: 6941684

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121523\
Data File : VU056904.D
Acq On : 16 Dec 2023 01:41
Operator : MD/SY
Sample : 05809-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7C51

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

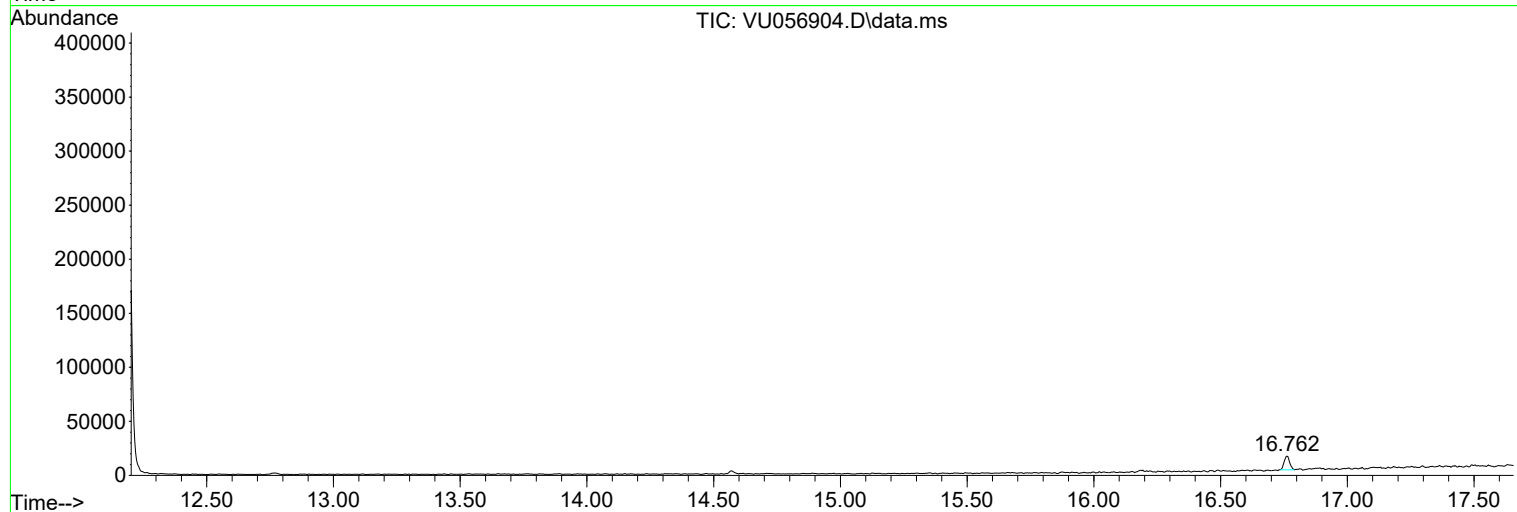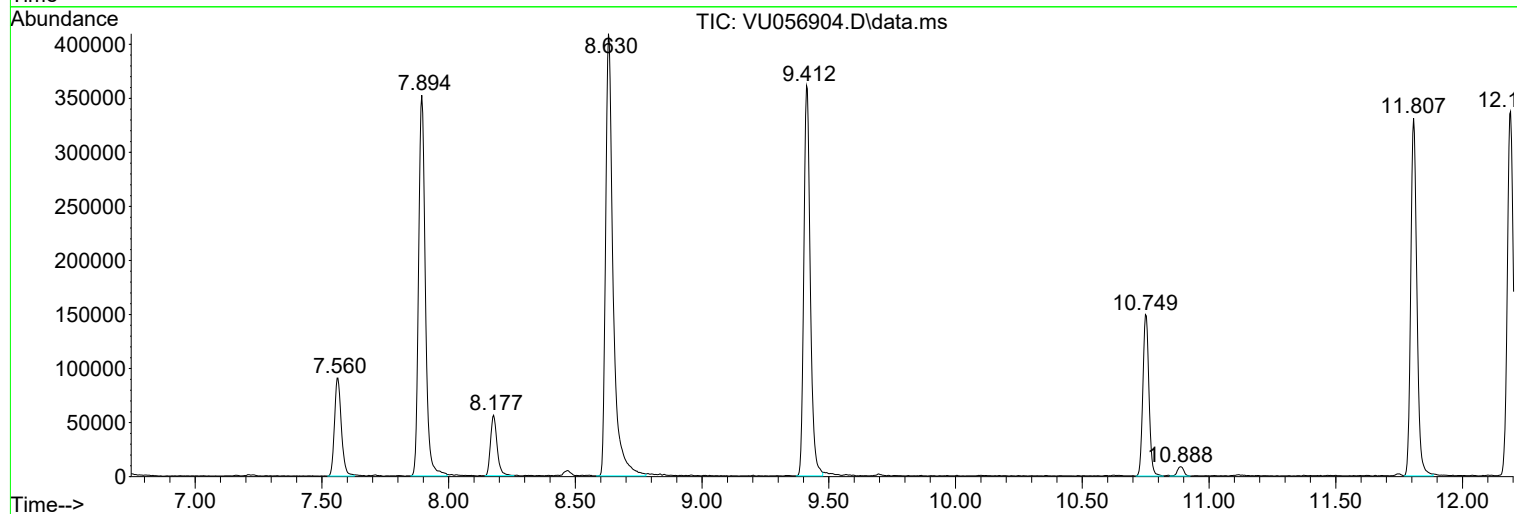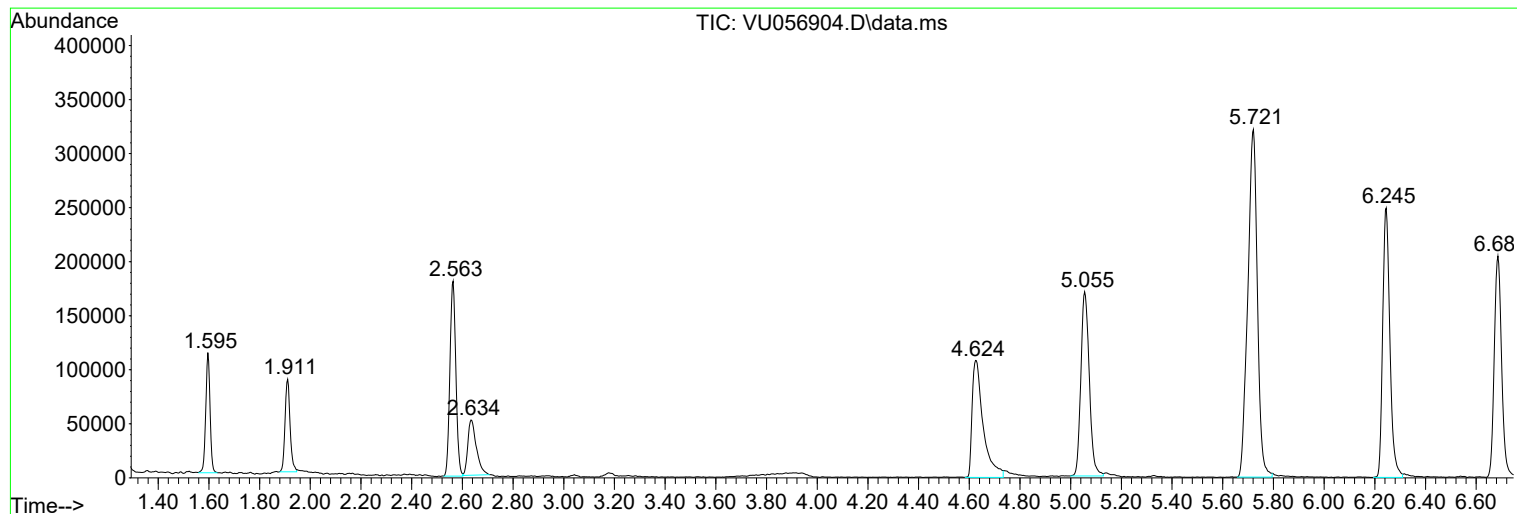

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121523\
Data File : VU056904.D
Acq On : 16 Dec 2023 01:41
Operator : MD/SY
Sample : 05809-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7C51

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121523\
Data File : VU056904.D
Acq On : 16 Dec 2023 01:41
Operator : MD/SY
Sample : 05809-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7C51

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc