


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121523\
Data File : VU056867.D
Acq On : 15 Dec 2023 09:03
Operator : MD/SY
Sample : BFB093
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB093

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Mon Dec 18 01:16:15 2023

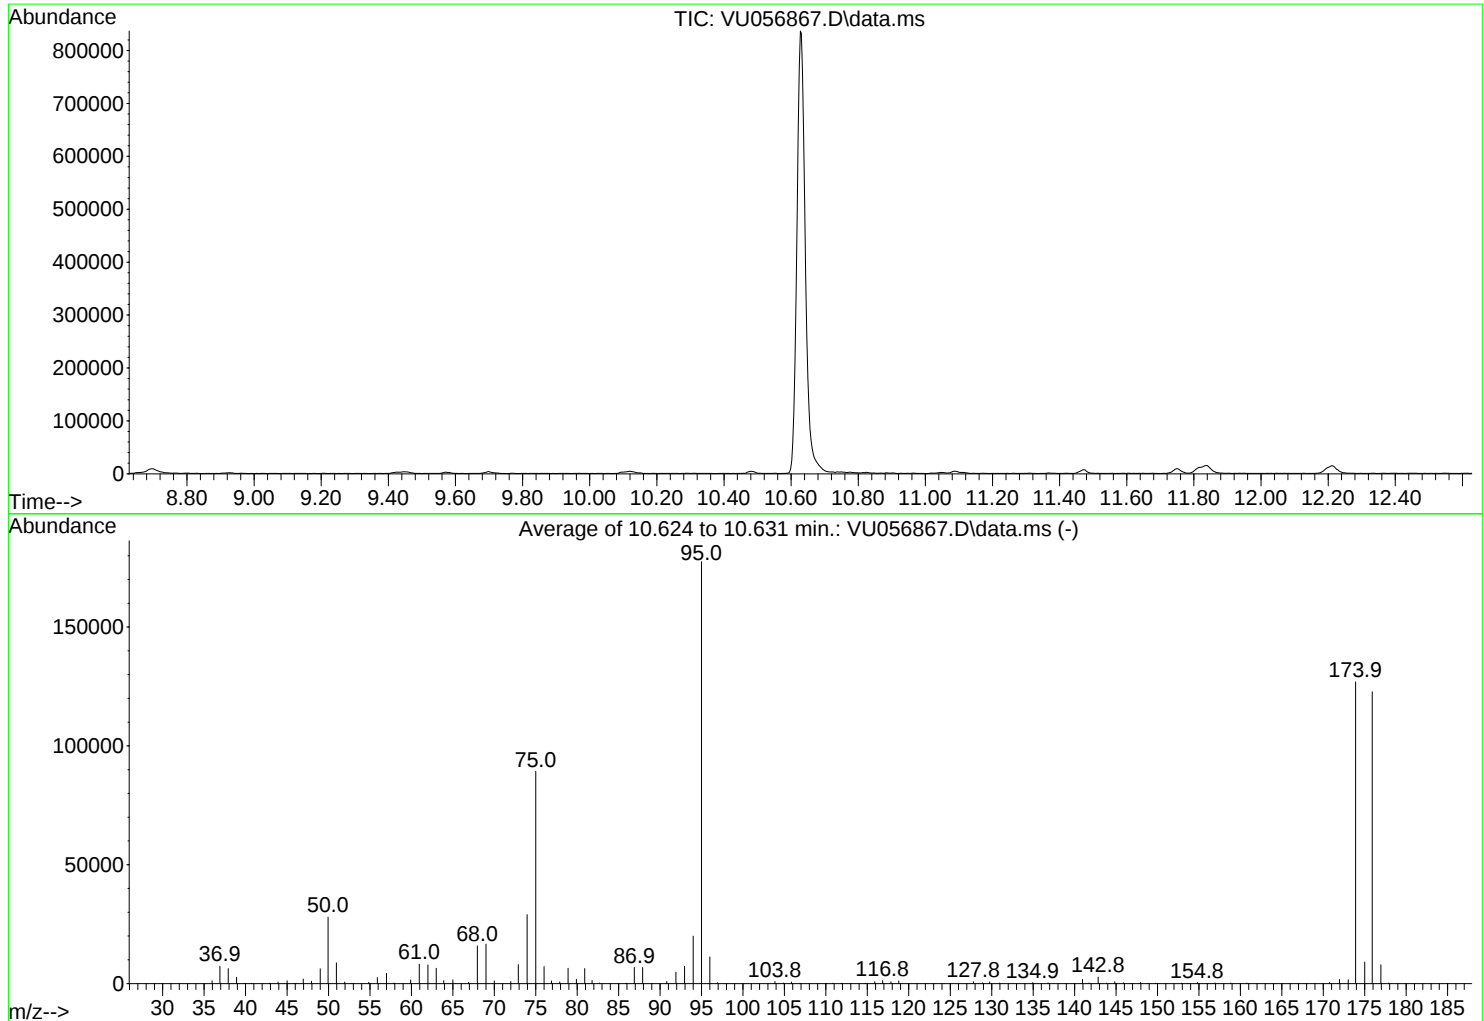

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	27896	PASS
75	95	30	80	50.3	89331	PASS
95	95	100	100	100.0	177472	PASS
96	95	5	9	6.3	11236	PASS
173	174	0.00	2	1.2	1579	PASS
174	95	50	120	71.5	126965	PASS
175	174	5	9	7.1	9029	PASS
176	174	95	101	96.7	122739	PASS
177	176	5	9	6.5	7951	PASS

m/z	Abundance
39.80	360.0
43.90	535.0

Instrument :
MSVOA_U
ClientSampleId :
BFB093

m/z	Abundance
35.90	1106.0
36.90	6849.0
37.90	6001.0
38.90	2579.0
39.80	390.0
40.70	127.0
43.00	236.0
43.90	1179.0
45.00	1104.0
45.80	175.0
46.10	190.0
46.90	1921.0
48.00	1000.0
49.00	5820.0
49.90	27288.0
51.00	8099.0
51.90	645.0
52.80	112.0
54.80	446.0
55.90	2470.0
57.00	4250.0
57.80	267.0
59.90	1371.0
60.90	8099.0
62.00	7634.0
63.00	6522.0
63.90	1313.0
65.00	1291.0
66.90	486.0
67.90	15288.0
69.00	16146.0
70.00	998.0
72.00	835.0
72.90	8086.0
74.00	28080.0
75.00	83760.0
76.00	7374.0
76.90	1021.0
77.90	600.0
78.90	6002.0
79.90	1671.0
80.90	5999.0
81.80	1355.0
82.70	165.0
85.90	267.0
86.90	6279.0
87.90	6821.0
90.80	927.0
91.90	4533.0
92.90	6986.0
94.00	18960.0
95.00	169472.0
96.00	10709.0
96.90	337.0
103.80	799.0
104.80	269.0
105.90	607.0
106.90	155.0
110.90	185.0
111.80	152.0
113.00	127.0
114.80	181.0
115.90	717.0
116.90	1279.0
117.90	725.0
118.80	1096.0
127.80	850.0
128.90	306.0
129.80	582.0
131.00	247.0
135.00	348.0
136.80	259.0
140.90	1696.0
141.70	261.0
142.80	2859.0
143.90	200.0
144.90	774.0
145.90	379.0
146.80	134.0
148.00	398.0
148.80	138.0
149.80	167.0
152.80	147.0
153.60	143.0
154.80	374.0
156.90	204.0
158.80	233.0
160.80	197.0
170.70	323.0
171.90	1437.0
173.00	1443.0
173.90	117272.0

Instrument :
MSVOA_U
ClientSampleId :
BFB093

175.00	8508.0
175.90	112160.0
176.90	7539.0
177.90	226.0

Instrument :
MSVOA_U
ClientSampleId :
BFB093

m/z	Abundance
36.00	1234.0
36.90	7545.0
37.90	6643.0
38.90	2702.0
39.80	449.0
40.70	116.0
42.90	174.0
44.00	1215.0
45.00	1265.0
46.10	190.0
46.90	1967.0
48.00	982.0
49.00	6483.0
50.00	28688.0
51.00	8872.0
52.00	701.0
53.00	163.0
54.90	521.0
55.90	2647.0
57.00	4385.0
57.90	233.0
59.90	1528.0
60.90	8300.0
62.00	8034.0
63.00	6586.0
63.90	1327.0
65.00	1613.0
66.90	510.0
68.00	16196.0
69.00	17088.0
70.00	1143.0
72.00	903.0
72.90	8319.0
74.00	29864.0
75.00	91760.0
76.00	7296.0
76.90	1198.0
77.90	739.0
78.90	6662.0
79.90	1840.0
80.90	6460.0
81.80	1382.0
82.70	294.0
85.90	206.0
86.90	6900.0
87.90	7073.0
89.10	100.0
90.80	964.0
91.90	4906.0
92.90	7281.0
94.00	20640.0
95.00	183168.0
96.00	11508.0
97.00	374.0
103.90	923.0
104.80	265.0
105.80	700.0
106.90	147.0
110.00	135.0
110.80	201.0
111.90	178.0
113.00	105.0
114.70	198.0
115.90	866.0
116.90	1327.0
117.90	727.0
118.80	1173.0
127.80	812.0
128.90	307.0
129.70	778.0
131.00	262.0
135.00	379.0
136.80	323.0
140.90	1781.0
141.80	255.0
142.80	2810.0
143.90	254.0
144.90	855.0
145.90	351.0
146.80	100.0
148.00	460.0
148.90	135.0
149.80	189.0
152.90	192.0
153.70	119.0
154.80	484.0
156.10	135.0
157.00	232.0
158.90	265.0
160.80	237.0
170.80	413.0
172.00	1778.0

Instrument :
MSVOA_U
ClientSampleId :
BFB093

173.00	1664.0
173.90	130696.0
175.00	9269.0
175.90	126680.0
177.00	8178.0
177.90	223.0

Instrument :
MSVOA_U
ClientSampleId :
BFB093

m/z	Abundance
36.00	1219.0
36.90	7561.0
37.90	6351.0
38.90	2681.0
39.90	488.0
42.80	164.0
44.00	1133.0
45.00	1269.0
45.90	164.0
47.00	1845.0
47.90	907.0
49.00	6467.0
50.00	27712.0
50.90	9116.0
52.00	579.0
53.00	211.0
54.90	523.0
55.90	2530.0
57.00	4221.0
58.00	278.0
59.90	1619.0
61.00	8095.0
62.00	7806.0
63.00	6243.0
63.90	1166.0
65.00	1768.0
66.90	429.0
68.00	16108.0
69.00	16512.0
70.00	1234.0
72.00	872.0
72.90	7602.0
73.90	29064.0
75.00	92472.0
76.00	6851.0
76.90	1166.0
77.90	807.0
78.90	6577.0
79.90	1795.0
80.90	6407.0
81.80	1276.0
82.70	341.0
86.90	7207.0
87.90	6359.0
90.80	845.0
91.90	5106.0
93.00	7547.0
94.00	20328.0
95.00	179776.0
96.00	11491.0
96.90	374.0
103.90	889.0
104.90	254.0
105.80	715.0
106.90	102.0
110.00	142.0
110.80	186.0
111.80	159.0
114.80	195.0
115.90	848.0
116.80	1249.0
117.80	763.0
118.80	1059.0
127.80	727.0
128.90	266.0
129.70	809.0
130.90	210.0
134.90	366.0
136.80	328.0
141.00	1771.0
141.80	241.0
142.90	2475.0
143.80	263.0
144.80	802.0
145.90	282.0
146.80	106.0
147.80	389.0
148.90	111.0
149.80	179.0
152.90	199.0
154.80	502.0
156.10	130.0
157.00	272.0
158.90	255.0
160.80	217.0
170.80	468.0
172.00	1937.0
173.00	1630.0
173.90	132928.0
175.00	9310.0
175.90	129376.0
177.00	8136.0

Instrument :
MSVOA_U
ClientSampleId :
BFB093

177.90

222.0

Instrument :

MSVOA_U

ClientSampleId :

BFB093