

Data File : VU036238.D
Acq On : 16 Dec 2019 16:55
Operator : JC/MD
Sample : K6240-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFQX8

Quant Time: Dec 17 01:24:57 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 17 01:19:57 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	225302	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.45	117	256999	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.84	152	92445	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	85139	4.29	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.80%
7) Chloroethane-d5	1.93	69	82634	4.65	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.00%
11) 1,1-Dichloroethene-d2	2.59	63	89074	3.11	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.20%
20) 2-Butanone-d5	4.69	46	206994	55.69	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	111.38%
24) Chloroform-d	5.11	84	153517	4.81	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.20%
26) 1,2-Dichloroethane-d4	5.75	65	85790	5.12	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.40%
32) Benzene-d6	5.77	84	280767	4.35	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.00%
36) 1,2-Dichloropropane-d6	6.73	67	94455	4.64	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.80%
41) Toluene-d8	7.93	98	229040	3.77	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	75.40%
43) trans-1,3-Dichloropropene-	8.21	79	36604	4.37	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.40%
46) 2-Hexanone-d5	8.67	63	158465	49.48	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.96%
57) 1,1,2,2-Tetrachloroethane-	10.78	84	94891	5.10	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.00%
64) 1,2-Dichlorobenzene-d4	12.22	152	92665	5.24	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.80%


Target Compounds


					Qvalue
12) 1,1-Dichloroethene	2.60	96	1122	0.067 ug/L #	1
13) Acetone	2.66	43	112670	34.781 ug/L	99
15) Methyl Acetate	3.00	43	2405	0.367 ug/L	97
16) Methylene chloride	3.08	84	6020	0.245 ug/L	85
21) 2-Butanone	4.77	43	29396	6.791 ug/L	98
35) Methylcyclohexane	6.73	83	22698	0.784 ug/L #	18
37) 1,2-Dichloropropane	6.73	63	10172	0.505 ug/L #	86
40) 4-Methyl-2-pentanone	7.84	43	24118	2.288 ug/L #	86
42) Toluene	8.01	91	10664	0.126 ug/L	97
48) 2-Hexanone	8.72	43	10925	1.389 ug/L #	52
59) 1,2,3-Trichloropropane	11.83	75	11437	0.854 ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :
MSVOA_U
ClientSampleId :
BFQX8

Quant Time: Dec 17 01:24:57 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121319WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 17 01:19:57 2019
Response via : Initial Calibration

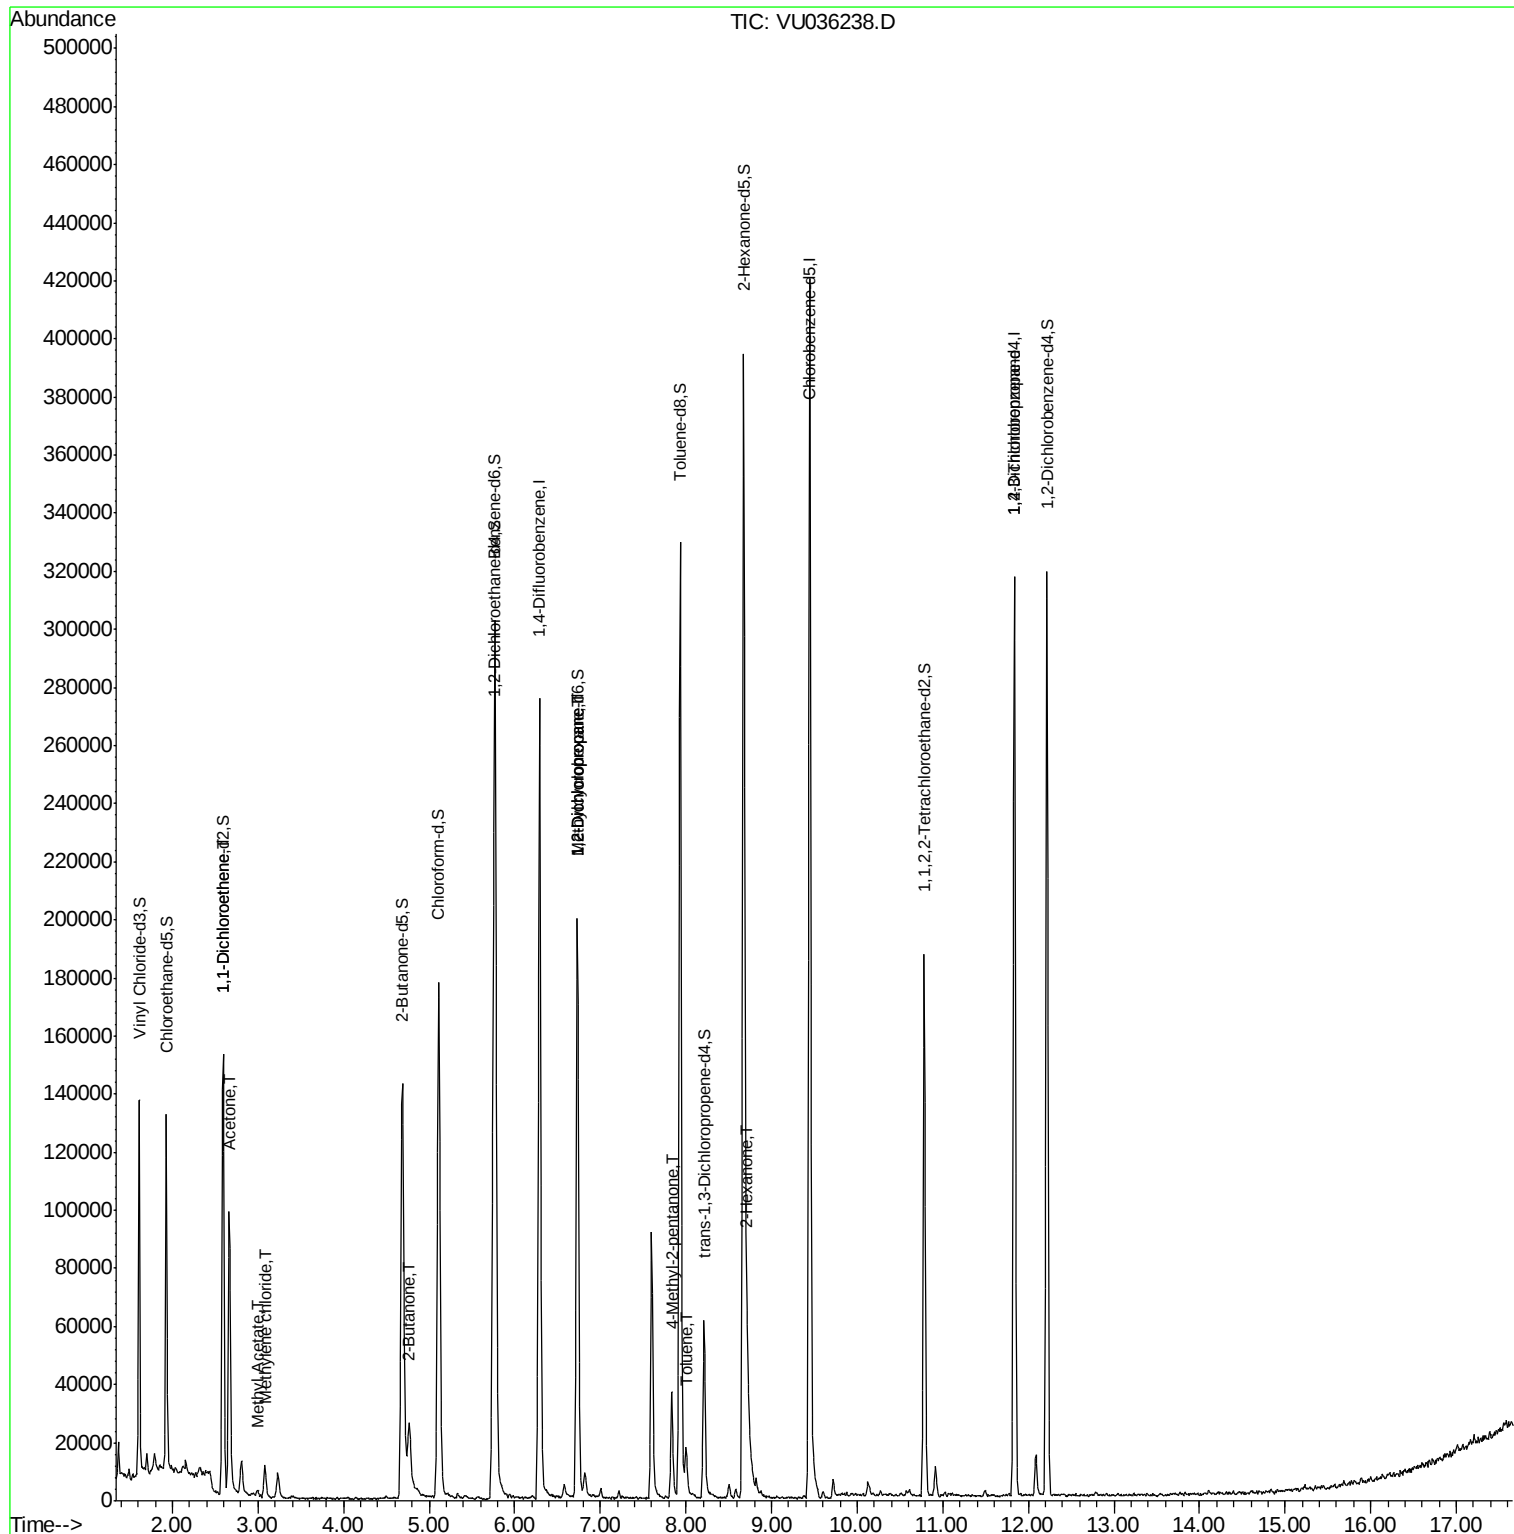

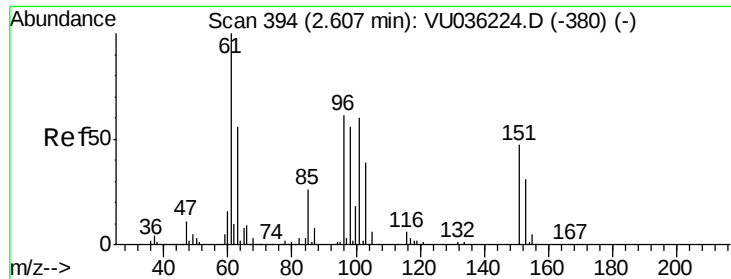

#12

1,1-Dichloroethene

Concen: 0.067 ug/L

RT: 2.60 min Scan# 392

Delta R.T. -0.01 min

Lab File: VU036238.D

Acq: 16 Dec 2019 16:55

Instrument :

MSVOA_U

ClientSampleId :

BFQX8


Tgt Ion: 96 Resp: 1122

Ion Ratio Lower Upper

96 100

61 1135.4 114.0 211.8#




63 7750.1 63.6 118.0#

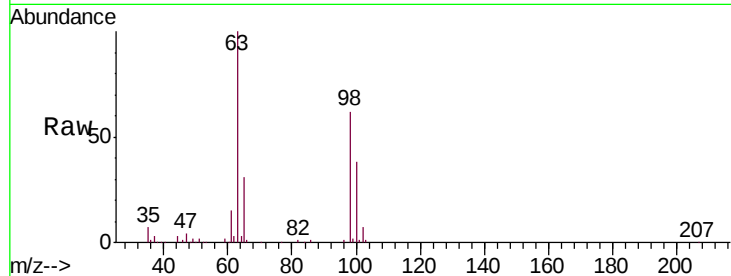

Abundance Ion 96.00 (95.70 to 96.70): VU036224.D (-380) (-)

Ion 61.05 (60.75 to 61.75): VU036224.D (-380) (-)

Ion 63.00 (62.70 to 63.70): VU036224.D (-380) (-)

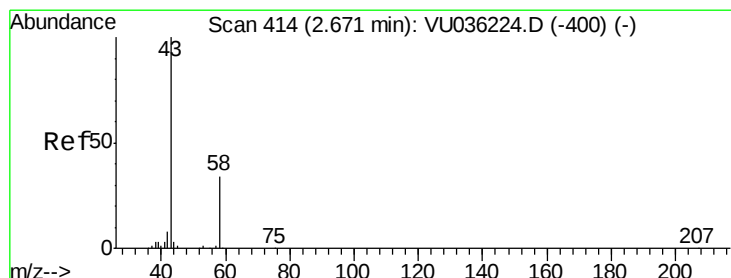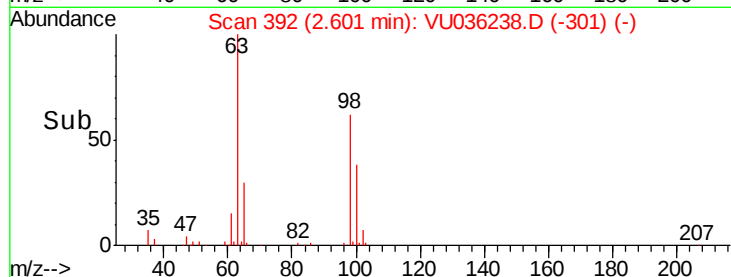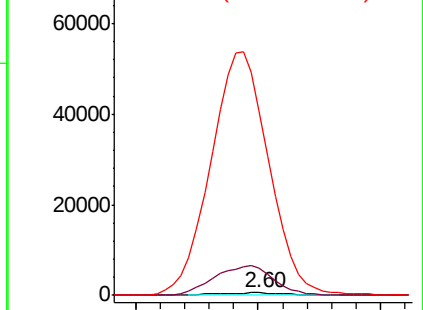

#13

Acetone

Concen: 34.781 ug/L

RT: 2.66 min Scan# 412

Delta R.T. -0.01 min

Lab File: VU036238.D


Acq: 16 Dec 2019 16:55

Tgt Ion: 43 Resp: 112670

Ion Ratio Lower Upper



43 100


58 34.1 0.0 67.6

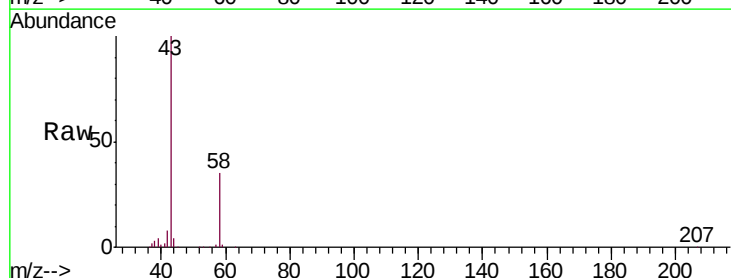

Abundance Ion 43.05 (42.75 to 43.75): VU036224.D (-400) (-)

Ion 58.05 (57.75 to 58.75): VU036224.D (-400) (-)



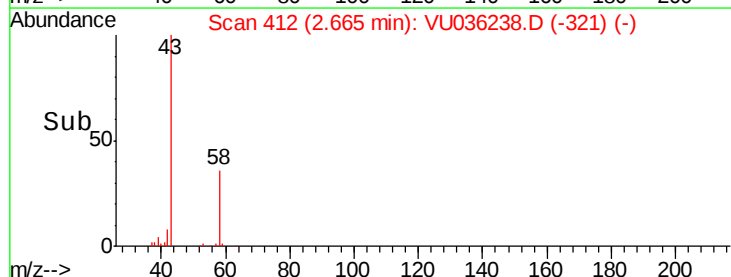
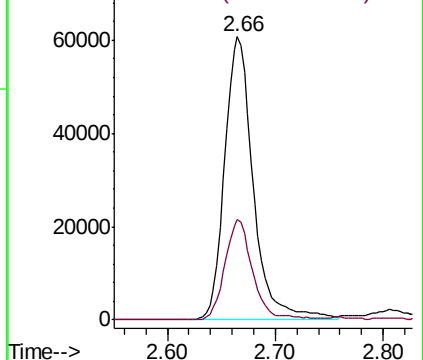


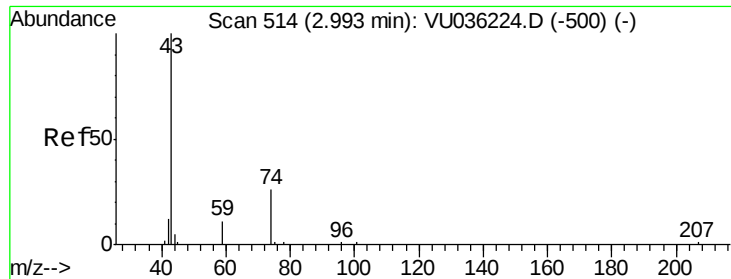

#15
Methyl Acetate
Concen: 0.367 ug/L
RT: 3.00 min Scan# 516
Delta R.T. 0.01 min
Lab File: VU036238.D
Acq: 16 Dec 2019 16:55




Instrument :
MSVOA_U
ClientSampleId :
BFQX8


Tgt Ion: 43 Resp: 2405
Ion Ratio Lower Upper
43 100
74 27.4 20.8 31.2

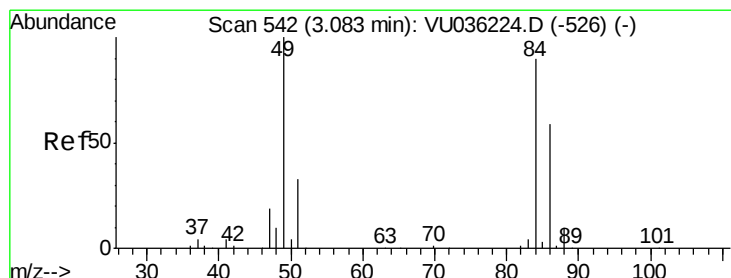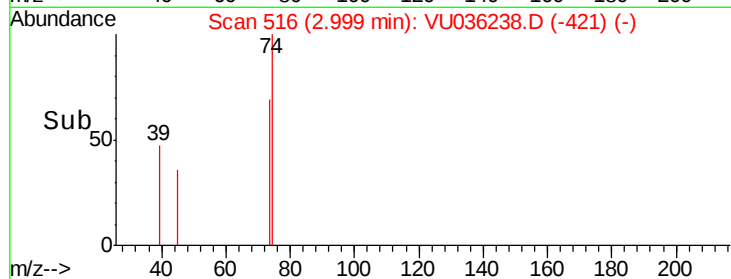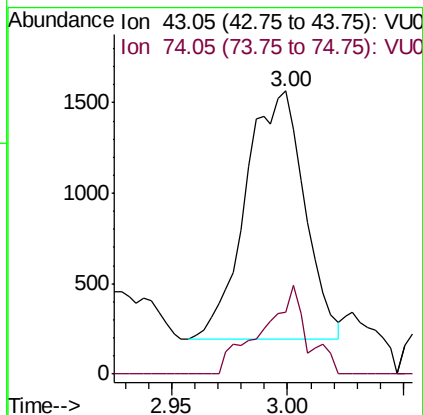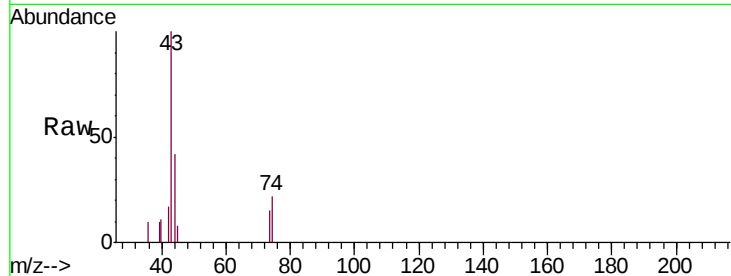

#16
Methylene chloride
Concen: 0.245 ug/L
RT: 3.08 min Scan# 542
Delta R.T. 0.00 min
Lab File: VU036238.D
Acq: 16 Dec 2019 16:55

Tgt Ion: 84 Resp: 6020
Ion Ratio Lower Upper
84 100
86 50.0 43.0 79.8
49 94.2 77.3 143.5

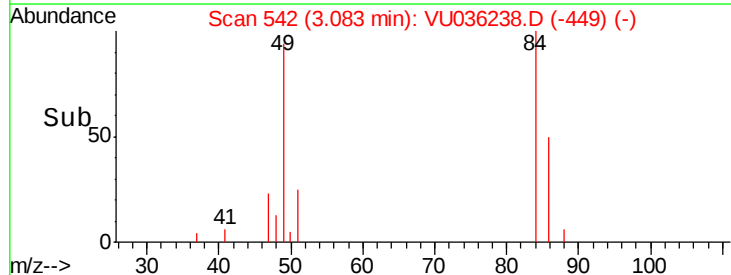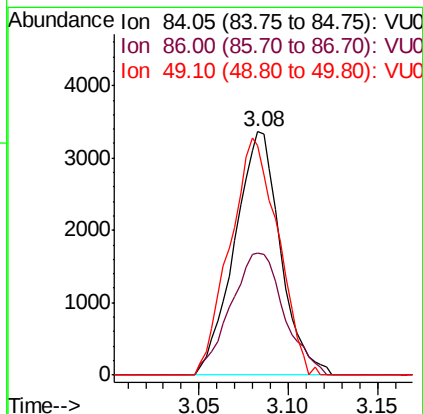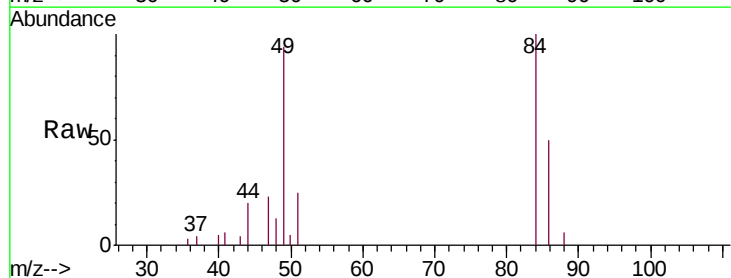

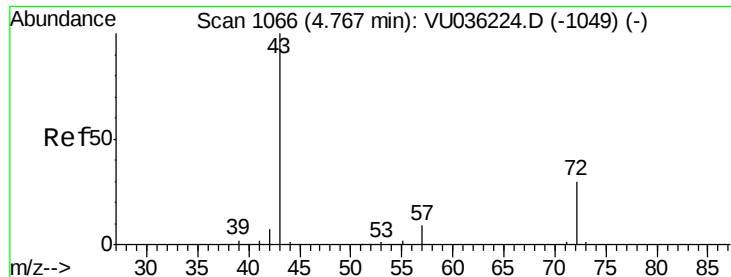

#21

2-Butanone

Concen: 6.791 ug/L

RT: 4.77 min Scan# 1067

Delta R.T. 0.00 min

Lab File: VU036238.D

Acq: 16 Dec 2019 16:55

Instrument :

MSVOA_U

ClientSampled :





BFQX8

Tgt Ion: 43 Resp: 29396

Ion Ratio Lower Upper

43 100

72 29.8 14.4 43.4

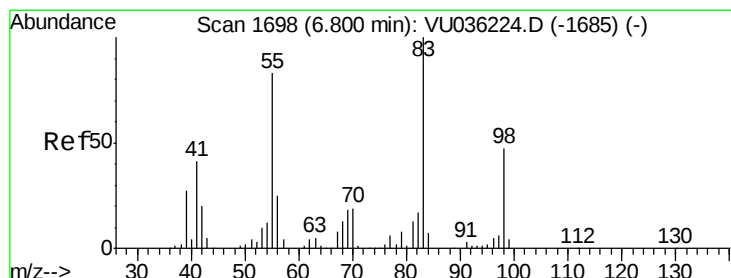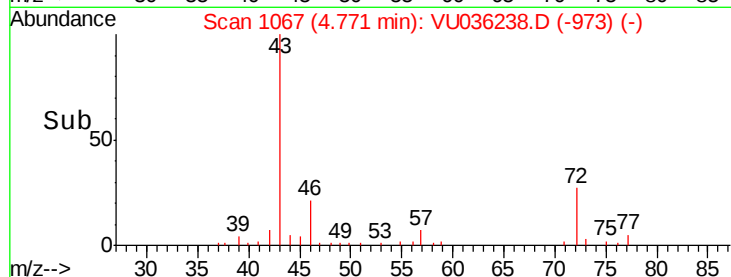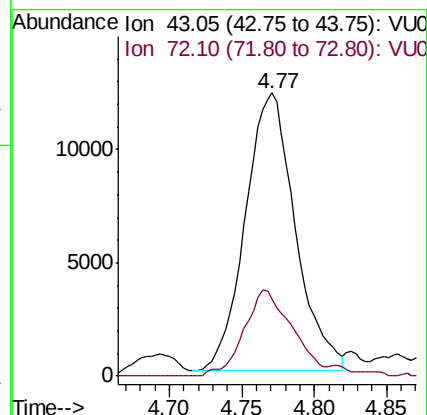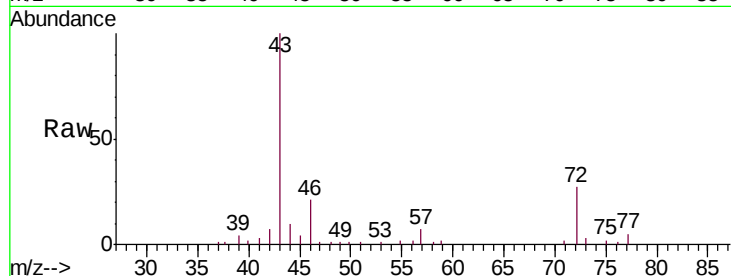

#35

Methylcyclohexane

Concen: 0.784 ug/L

RT: 6.73 min Scan# 1677

Delta R.T. -0.07 min

Lab File: VU036238.D

Acq: 16 Dec 2019 16:55




Tgt Ion: 83 Resp: 22698


Ion Ratio Lower Upper

83 100

55 0.3 62.6 94.0#

98 0.7 36.2 54.2#


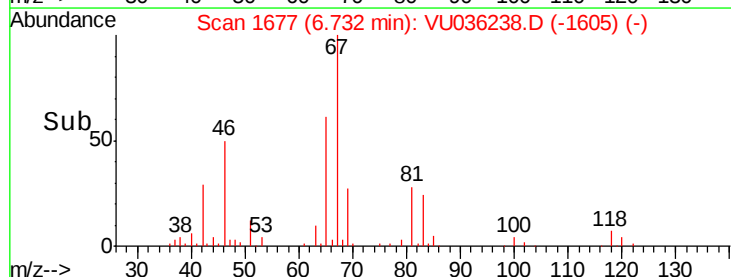
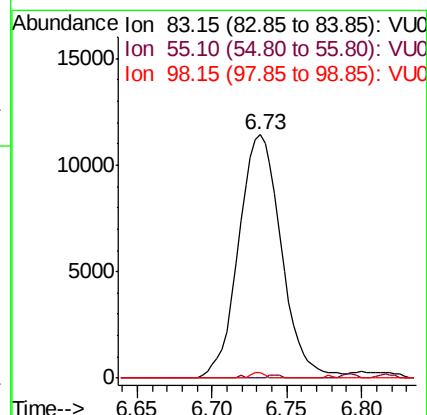
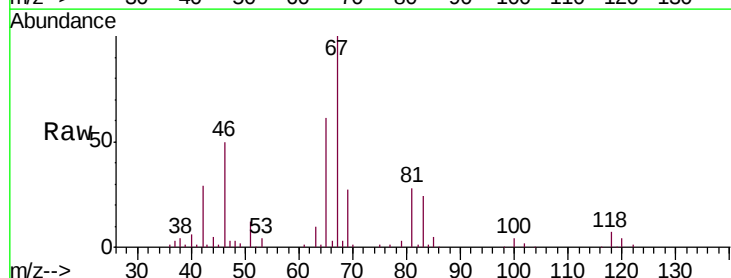


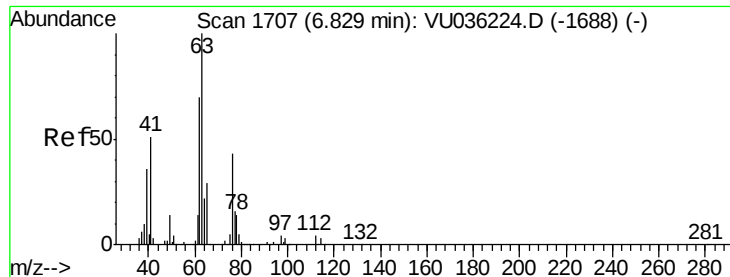

#37
 1,2-Dichloropropane
 Concen: 0.505 ug/L
 RT: 6.73 min Scan# 1676
 Delta R.T. -0.10 min
 Lab File: VU036238.D
 Acq: 16 Dec 2019 16:55




Instrument :
 MSVOA_U
 ClientSampled :
 BFQX8


Tgt Ion: 63 Resp: 10172
 Ion Ratio Lower Upper
 63 100
 112 0.2 3.8 5.8#

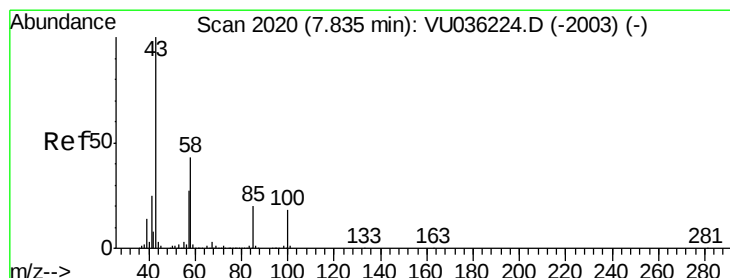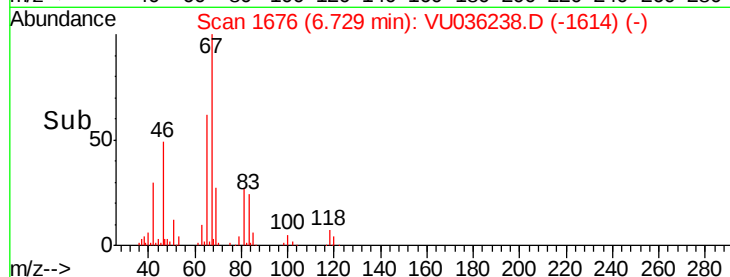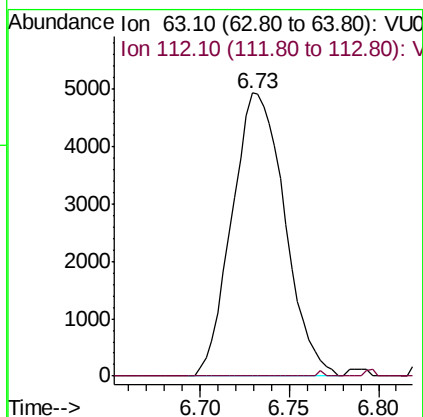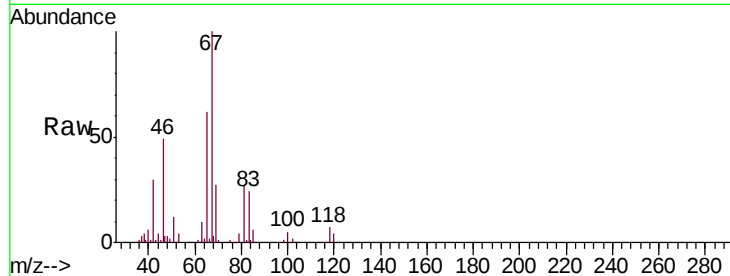

#40
 4-Methyl-2-pentanone
 Concen: 2.288 ug/L
 RT: 7.84 min Scan# 2020
 Delta R.T. 0.00 min
 Lab File: VU036238.D
 Acq: 16 Dec 2019 16:55

Tgt Ion: 43 Resp: 24118
 Ion Ratio Lower Upper
 43 100
 58 39.7 33.3 49.9
 100 0.0 13.7 20.5#

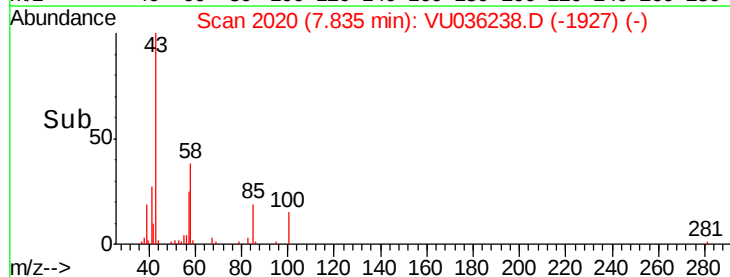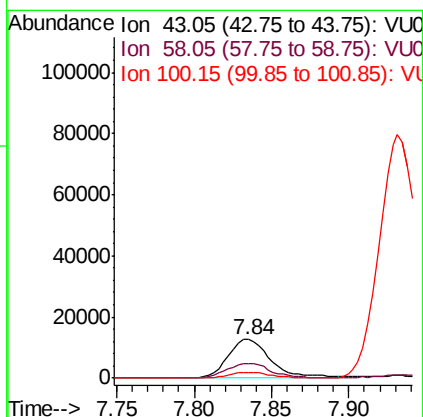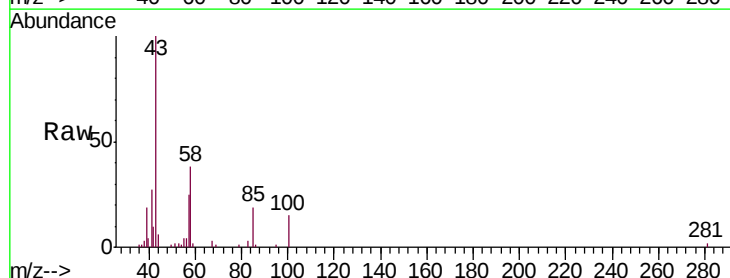

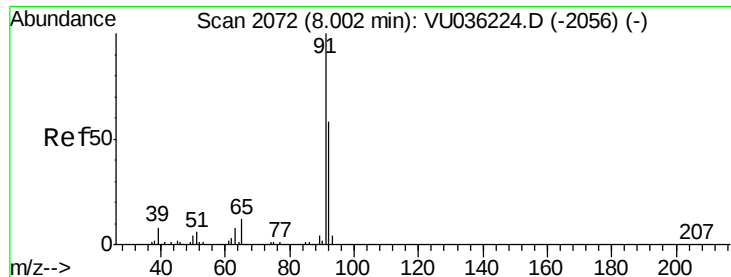

#42

Toluene

Concen: 0.126 ug/L

RT: 8.01 min Scan# 2073

Delta R.T. 0.00 min

Lab File: VU036238.D

Acq: 16 Dec 2019 16:55

Instrument :

MSVOA_U

ClientSampleId :


BFQX8

Tgt Ion: 91 Resp: 10664

Ion Ratio Lower Upper

91 100

92 56.6 41.2 76.6

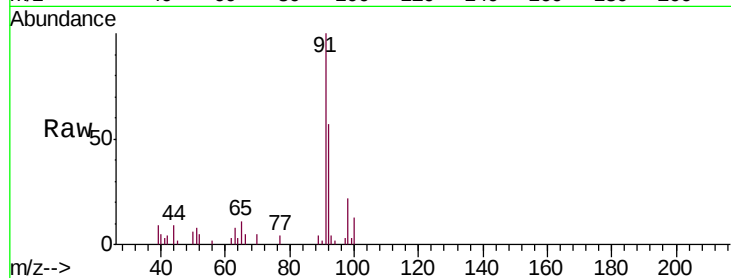

Abundance Ion 91.15 (90.85 to 91.85): VU036224.D (-2056) (-)

Ion 92.15 (91.85 to 92.85): VU036224.D (-2056) (-)

8.01

6000



4000

2000

0

7.95 8.00 8.05

Time-->

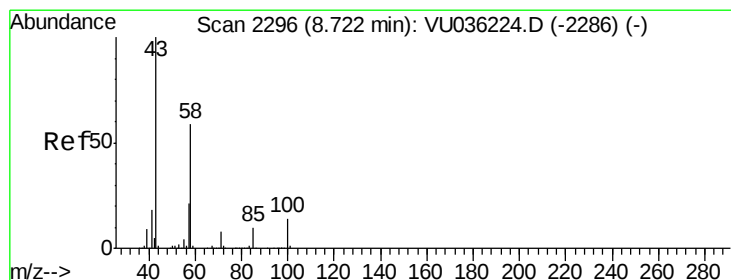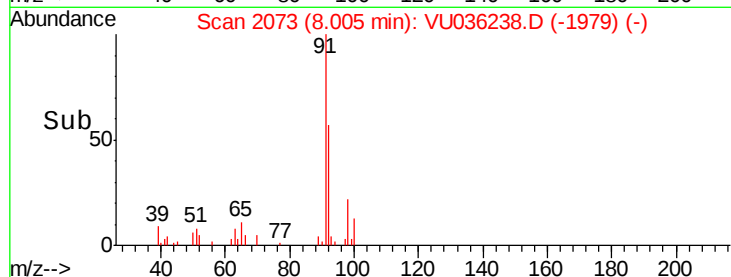

#48

2-Hexanone

Concen: 1.389 ug/L

RT: 8.72 min Scan# 2295

Delta R.T. -0.00 min

Lab File: VU036238.D

Acq: 16 Dec 2019 16:55

Tgt Ion: 43 Resp: 10925


Ion Ratio Lower Upper

43 100

58 6.1 46.2 69.2#

57 26.1 16.2 24.4#

100 9.5 10.2 15.4#

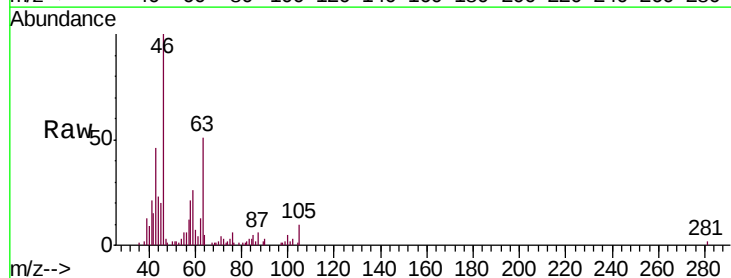

Abundance Ion 43.05 (42.75 to 43.75): VU036224.D (-2286) (-)

Ion 58.05 (57.75 to 58.75): VU036224.D (-2286) (-)

Ion 57.20 (56.90 to 57.90): VU036224.D (-2286) (-)

Ion 100.15 (99.85 to 100.85): VU036224.D (-2286) (-)

15000


10000


5000

0

8.70 8.75 8.80

Time-->

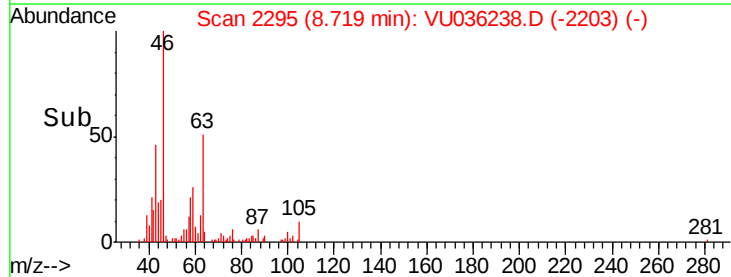

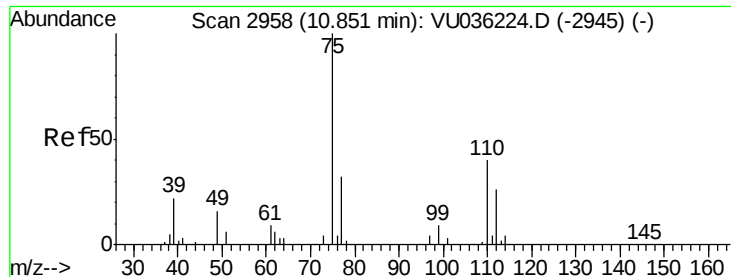

#59

1,2,3-Trichloropropane

Concen: 0.854 ug/L

RT: 11.83 min Scan# 3264

Delta R.T. 0.98 min

Lab File: VU036238.D

Acq: 16 Dec 2019 16:55

Instrument :

MSVOA_U

ClientSampleId :


BFQX8

Tgt Ion: 75 Resp: 11437

Ion Ratio Lower Upper

75 100

77 35.4 27.2 40.8

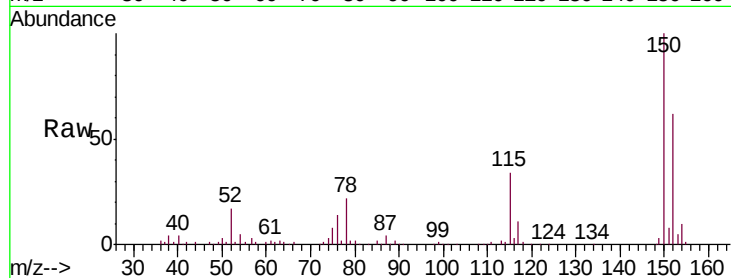

Abundance Ion 75.00 (74.70 to 75.70): VU0

Ion 77.00 (76.70 to 77.70): VU0

