


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU121619\
Data File : VU036223.D
Acq On : 16 Dec 2019 09:19
Operator : JC/MD
Sample : BFB19
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB19

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121319WMA.M
Title : TRACE VOA SOM01.0
Last Update : Wed Dec 18 00:44:43 2019

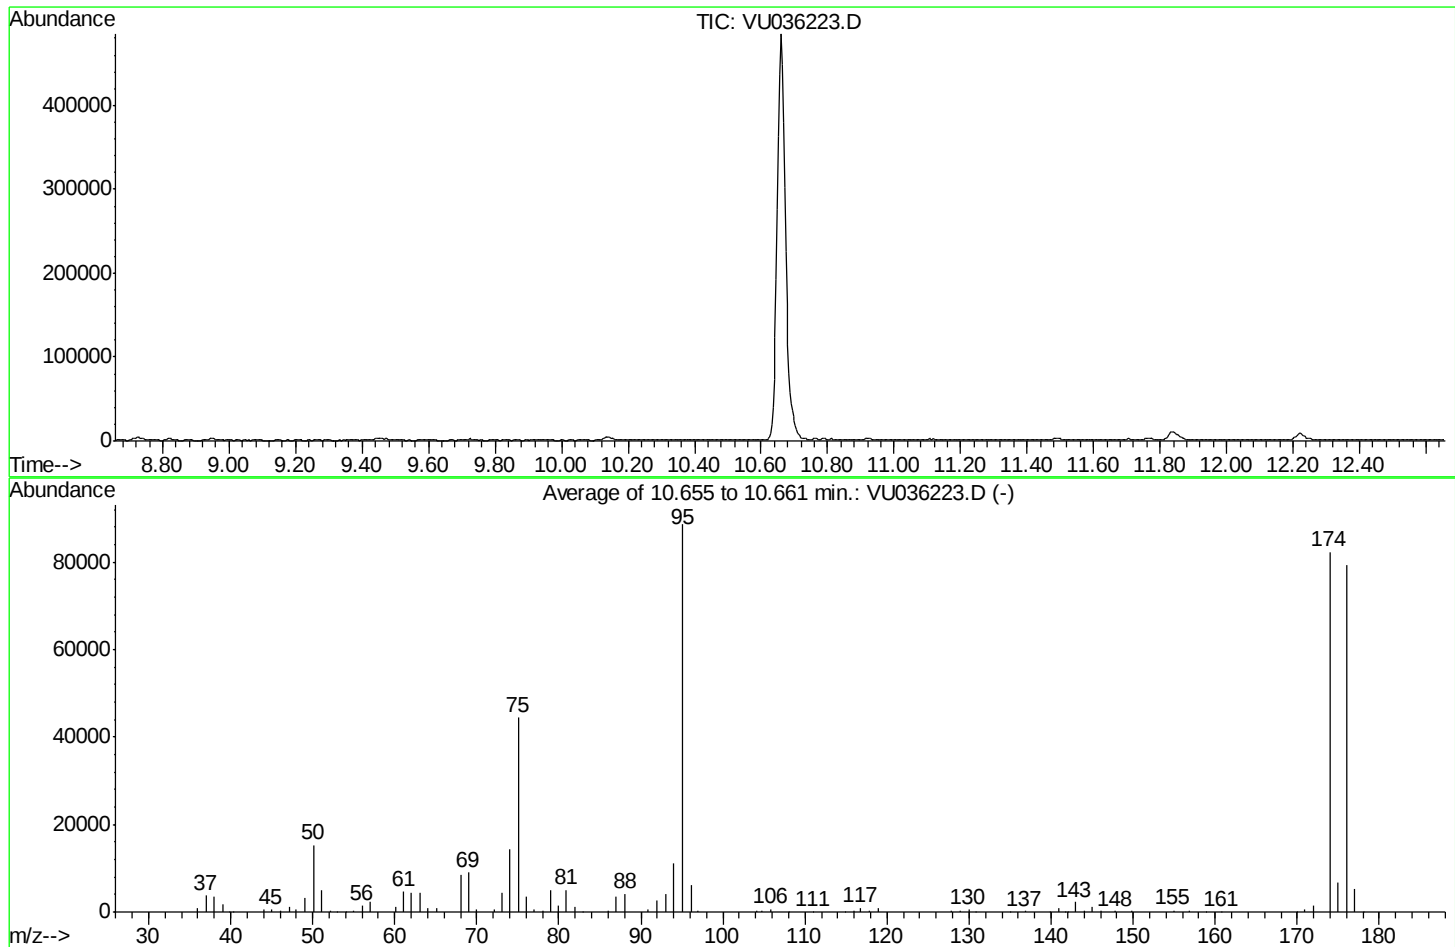

AutoFind: Scans 2897, 2898, 2899; Background Corrected with Scan 2883

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	15359	PASS
75	95	30	80	50.1	44442	PASS
95	95	100	100	100.0	88621	PASS
96	95	5	9	7.0	6167	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	92.8	82248	PASS
175	174	5	9	8.1	6643	PASS
176	174	95	101	96.3	79226	PASS
177	176	5	9	6.8	5389	PASS

m/z	Abundance
35.90	468.0
38.10	123.0
39.90	202.0
44.00	695.0

Instrument :
MSVOA_U
ClientSampleId :
BFB19

m/z	Abundance
36.00	1299.0
37.00	3444.0
38.00	3425.0
39.00	1731.0
39.80	290.0
40.30	194.0
44.00	1283.0
45.10	447.0
46.10	175.0
47.10	1008.0
47.90	476.0
49.00	3423.0
50.00	14622.0
51.00	4595.0
52.10	190.0
53.00	133.0
55.00	238.0
56.00	1280.0
57.00	1914.0
60.10	1069.0
61.10	4277.0
62.10	4350.0
63.10	4006.0
64.00	997.0
65.00	921.0
68.00	7943.0
69.00	8540.0
69.90	594.0
72.10	731.0
73.10	3836.0
74.00	13493.0
75.00	42048.0
76.00	3521.0
77.00	638.0
78.00	457.0
78.90	4432.0
80.00	1379.0
80.90	4681.0
81.90	1118.0
82.90	117.0
86.10	179.0
87.00	3384.0
88.10	3779.0
90.90	447.0
92.00	2525.0
93.00	3577.0
94.00	10520.0
95.10	84536.0
96.10	6146.0
97.00	362.0
104.00	360.0
104.70	151.0
105.90	587.0
111.00	122.0
115.90	227.0
116.80	967.0
117.90	453.0
118.90	728.0
127.80	430.0
128.90	198.0
129.90	502.0
136.80	287.0
140.90	859.0
142.00	148.0
142.90	2174.0
144.20	130.0
145.00	1101.0
146.00	180.0
147.90	296.0
149.70	124.0
154.90	338.0
156.90	209.0
158.90	145.0
160.80	143.0
170.00	118.0
170.90	477.0
171.90	1267.0
174.00	75704.0
175.00	5862.0
176.00	71880.0
176.90	4996.0
178.00	116.0

Instrument :
MSVOA_U
ClientSampleId :
BFB19

m/z	Abundance
36.00	1285.0
37.00	3939.0
38.00	3785.0
39.00	1649.0
39.80	274.0
40.30	136.0
44.00	1246.0
44.90	591.0
46.00	250.0
47.10	1197.0
47.90	538.0
49.00	3470.0
50.10	15721.0
51.00	5220.0
52.10	248.0
52.90	157.0
54.10	122.0
55.00	208.0
56.00	1457.0
57.00	2321.0
60.10	1114.0
61.10	4835.0
62.10	4501.0
63.10	4560.0
64.00	989.0
65.10	875.0
68.00	8606.0
69.00	9471.0
69.90	649.0
72.10	669.0
73.00	4534.0
74.00	14724.0
75.10	45712.0
76.00	3818.0
76.90	575.0
78.00	447.0
78.90	5039.0
80.00	1538.0
80.90	5158.0
81.90	1253.0
82.90	151.0
86.10	219.0
87.00	3680.0
88.10	4372.0
90.90	553.0
92.00	2554.0
93.00	4278.0
94.00	11443.0
95.10	90800.0
96.10	6359.0
97.00	347.0
104.10	401.0
104.70	232.0
105.90	636.0
107.90	107.0
116.00	278.0
116.80	1055.0
117.90	379.0
119.00	738.0
127.80	456.0
128.90	197.0
129.90	573.0
130.80	122.0
136.80	284.0
139.80	130.0
140.90	843.0
142.00	141.0
142.90	2426.0
144.10	178.0
145.00	1259.0
146.00	173.0
147.80	303.0
149.80	173.0
154.90	335.0
156.80	248.0
158.90	106.0
160.80	140.0
170.90	541.0
172.00	1512.0
174.00	84832.0
175.00	6766.0
176.00	81288.0
177.00	5566.0
178.10	102.0

Instrument :
MSVOA_U
ClientSampleId :
BFB19

m/z	Abundance
36.00	1220.0
37.00	3942.0
38.00	3843.0
39.10	1631.0
39.80	217.0
40.30	118.0
44.00	1125.0
44.90	724.0
46.00	313.0
47.10	1207.0
48.00	687.0
49.00	3216.0
50.10	15736.0
51.00	5470.0
52.10	351.0
52.90	171.0
54.00	182.0
55.00	204.0
56.00	1590.0
57.00	2504.0
60.10	964.0
61.10	4830.0
62.00	4755.0
63.10	4734.0
64.10	1007.0
65.20	886.0
68.00	8572.0
69.00	9056.0
69.90	679.0
72.00	655.0
73.00	4689.0
74.10	15080.0
75.10	45568.0
76.00	3652.0
76.90	488.0
78.00	446.0
79.00	5189.0
80.00	1468.0
80.90	5269.0
81.90	1249.0
82.90	125.0
86.00	198.0
87.00	3597.0
88.00	4492.0
90.90	571.0
92.00	2435.0
93.00	4437.0
94.00	11132.0
95.10	90528.0
96.10	5996.0
96.90	213.0
104.00	387.0
104.70	259.0
105.90	568.0
108.00	164.0
114.80	144.0
116.00	330.0
116.80	993.0
117.90	332.0
119.00	818.0
127.80	340.0
128.90	155.0
130.00	552.0
130.70	108.0
135.00	130.0
136.80	217.0
139.80	137.0
140.90	825.0
141.70	211.0
142.90	2428.0
144.00	164.0
145.00	1337.0
146.00	202.0
147.80	229.0
149.80	203.0
154.90	336.0
156.80	284.0
160.80	130.0
171.00	574.0
172.00	1587.0
174.00	86208.0
175.00	7303.0
176.00	84512.0
177.00	5607.0

Instrument :
MSVOA_U
ClientSampleId :
BFB19