




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046413.D
 Acq On : 16 Dec 2021 12:15
 Operator : SY/MD
 Sample : M4997-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5R2

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/17/2021
 Supervised By :Mahesh Dadoda 12/17/2021

Quant Time: Dec 17 01:51:03 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 17 01:49:40 2021
 Response via : Initial Calibration

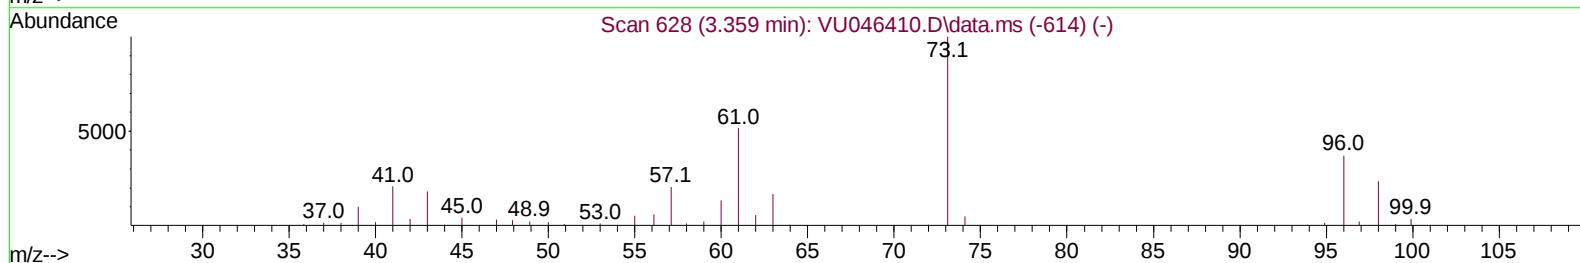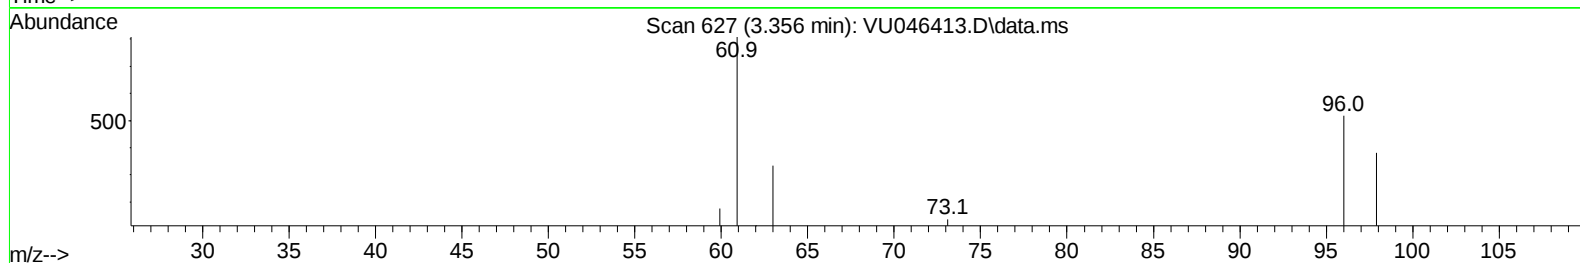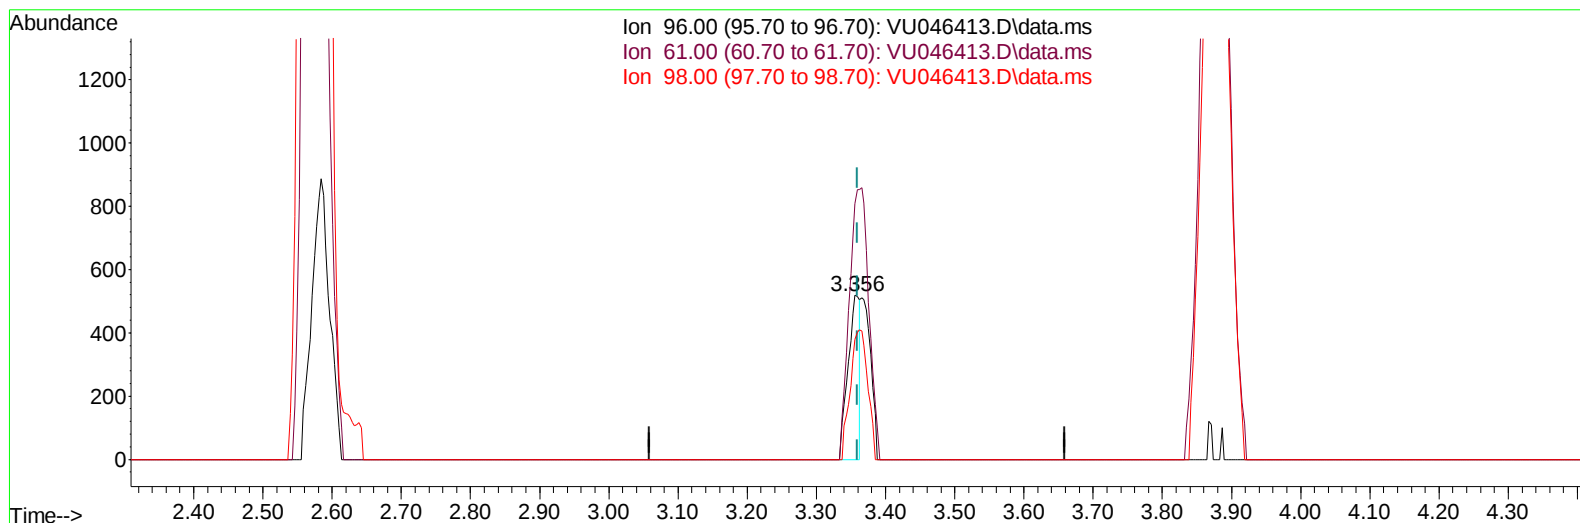

TIC: VU046413.D\data.ms

(17) trans-1,2-Dichloroethene (T)

3.356min (-0.003) 0.61 ug/L

response 619

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	135.10	155.98
98.00	62.90	73.36
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046413.D
Acq On : 16 Dec 2021 12:15
Operator : SY/MD
Sample : M4997-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5R2

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/17/2021
Supervised By :Mahesh Dadoda 12/17/2021

Quant Time: Dec 17 01:51:03 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 17 01:49:40 2021
Response via : Initial Calibration

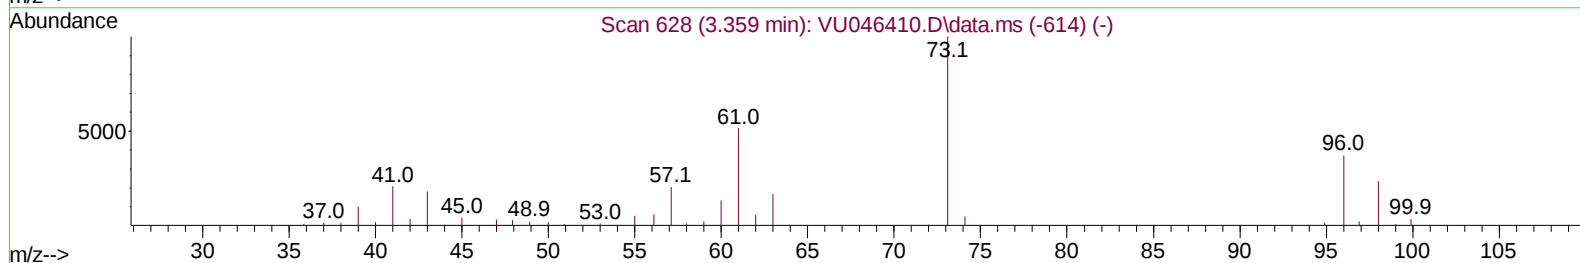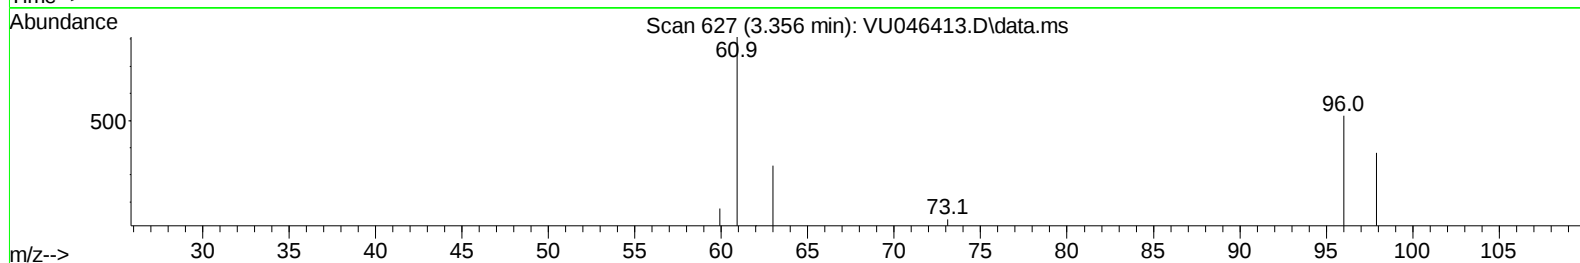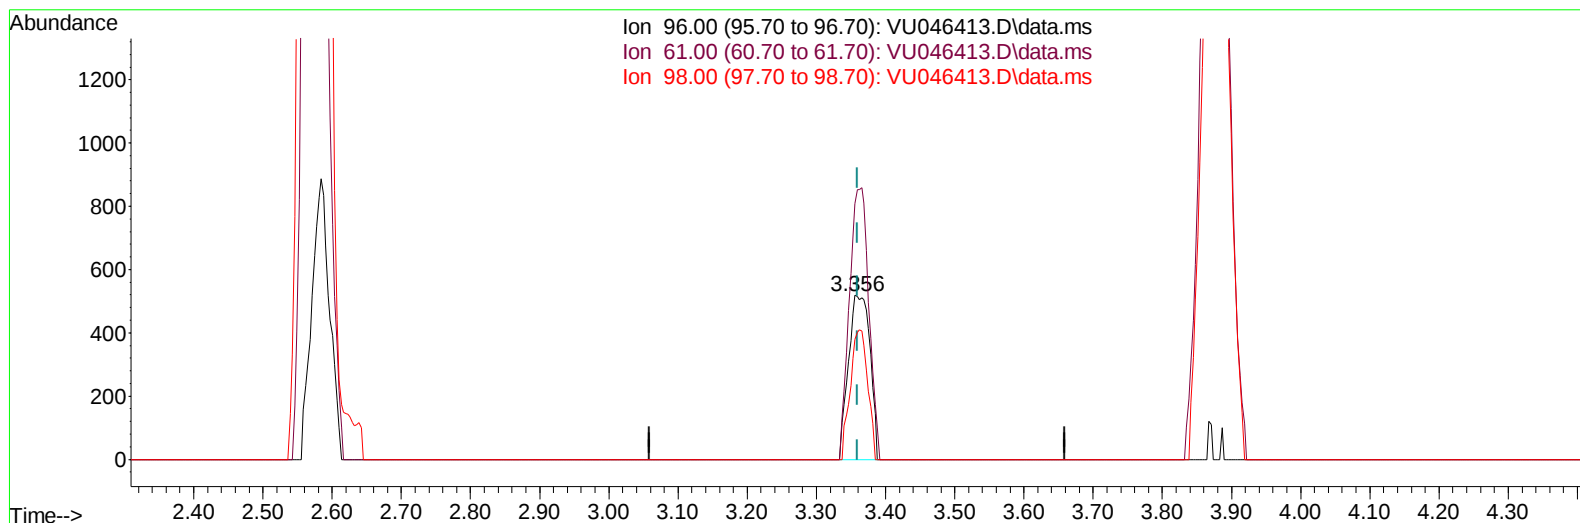

TIC: VU046413.D\data.ms

(17) trans-1,2-Dichloroethene (T)

3.356min (-0.003) 1.11 ug/L m

response 1121

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	135.10	155.98
98.00	62.90	73.36
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046413.D
 Acq On : 16 Dec 2021 12:15
 Operator : SY/MD
 Sample : M4997-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5R2

Manual IntegrationsAPPROVED

Quant Time: Dec 17 01:51:03 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 17 01:49:40 2021
 Response via : Initial Calibration

Reviewed By : John Carlone 12/17/2021
 Supervised By : Mahesh Dadoda 12/17/2021

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	138020	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	143255	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	66530	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	60405	53.130	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	106.260%	
7) Chloroethane-d5	1.919	69	43382	49.697	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	99.400%	
11) 1,1-Dichloroethene-d2	2.571	63	77260	37.854	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	75.700%	
21) 2-Butanone-d5	4.636	46	77024	85.221	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	85.220%	
24) Chloroform-d	5.070	84	102157	53.806	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	107.620%	
26) 1,2-Dichloroethane-d4	5.706	65	67013	52.593	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	105.180%	
32) Benzene-d6	5.732	84	199325	48.546	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	97.100%	
36) 1,2-Dichloropropane-d6	6.693	67	61936	48.673	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	97.340%	
41) Toluene-d8	7.899	98	170706	45.662	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	91.320%	
43) trans-1,3-Dichloroprop...	8.182	79	28491	46.381	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	92.760%	
47) 2-Hexanone-d5	8.636	63	58587	97.104	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	97.100%	
56) 1,1,2,2-Tetrachloroeth...	10.758	84	88443	45.830	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	91.660%	
66) 1,2-Dichlorobenzene-d4	12.195	152	63104	49.252	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	98.500%	
Target Compounds						
12) 1,1-Dichloroethene	2.584	96	1569	1.644	ug/L #	1
17) trans-1,2-Dichloroethene	3.356	96	1121m	1.110	ug/L	
19) 1,1-Dichloroethane	3.877	63	89565	48.775	ug/L	99
20) cis-1,2-Dichloroethene	4.674	96	11122	10.149	ug/L	95
30) 1,1,1-Trichloroethane	5.321	97	124687	70.907	ug/L	100
46) Tetrachloroethene	8.555	164	4714	5.616	ug/L	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046413.D
Acq On : 16 Dec 2021 12:15
Operator : SY/MD
Sample : M4997-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5R2

Manual IntegrationsAPPROVED

Quant Time: Dec 17 01:51:03 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 17 01:49:40 2021
Response via : Initial Calibration

Reviewed By :John Carlone 12/17/2021
Supervised By :Mahesh Dadoda 12/17/2021

