

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046439.D
 Acq On : 16 Dec 2021 22:54
 Operator : SY/MD
 Sample : M5101-11ME
 Misc : 7.06g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL35ME

Manual Integrations
 APPROVED

Reviewed By : John Carlone 12/17/2021
 Supervised By : Mahesh Dadoda 12/17/2021

Quant Time: Dec 17 04:05:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 17 03:50:47 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	155558	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	165770	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	81486	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	49503	38.632	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	77.260%		
7) Chloroethane-d5	1.912	69	33369	33.917	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	67.840%#		
11) 1,1-Dichloroethene-d2	2.546	63	64082	27.857	ug/L	-0.03
Spiked Amount 50.000	Range 60 - 125		Recovery =	55.720%#		
21) 2-Butanone-d5	4.649	46	69528	68.255	ug/L	0.02
Spiked Amount 100.000	Range 40 - 130		Recovery =	68.250%		
24) Chloroform-d	5.063	84	88748	41.473	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	82.940%		
26) 1,2-Dichloroethane-d4	5.703	65	61090	42.539	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.080%		
32) Benzene-d6	5.722	84	180492	37.988	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	75.980%		
36) 1,2-Dichloropropane-d6	6.690	67	55749	37.860	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	75.720%		
41) Toluene-d8	7.899	98	158622	36.667	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	73.340%#		
43) trans-1,3-Dichloroprop...	8.185	79	26022	36.608	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	73.220%		
47) 2-Hexanone-d5	8.677	63	54586	78.185	ug/L	0.04
Spiked Amount 100.000	Range 45 - 130		Recovery =	78.180%		
56) 1,1,2,2-Tetrachloroeth...	10.770	84	84042	37.635	ug/L	0.01
Spiked Amount 50.000	Range 65 - 120		Recovery =	75.260%		
66) 1,2-Dichlorobenzene-d4	12.201	152	61264	39.040	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	78.080%#		
Target Compounds						Qvalue
19) 1,1-Dichloroethane	3.864	63	1369	0.661	ug/L #	81
22) 2-Butanone	4.739	43	10413m	7.514	ug/L	
30) 1,1,1-Trichloroethane	5.311	97	11087	5.449	ug/L	99
46) Tetrachloroethene	8.552	164	11159	11.488	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046439.D
Acq On : 16 Dec 2021 22:54
Operator : SY/MD
Sample : M5101-11ME
Misc : 7.06g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 32 Sample Multiplier: 1


Instrument :
MSVOA_U
ClientSampleId :
BGL35ME

Quant Time: Dec 17 04:05:32 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 17 03:50:47 2021
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By : John Carlone 12/17/2021
Supervised By : Mahesh Dadoda 12/17/2021

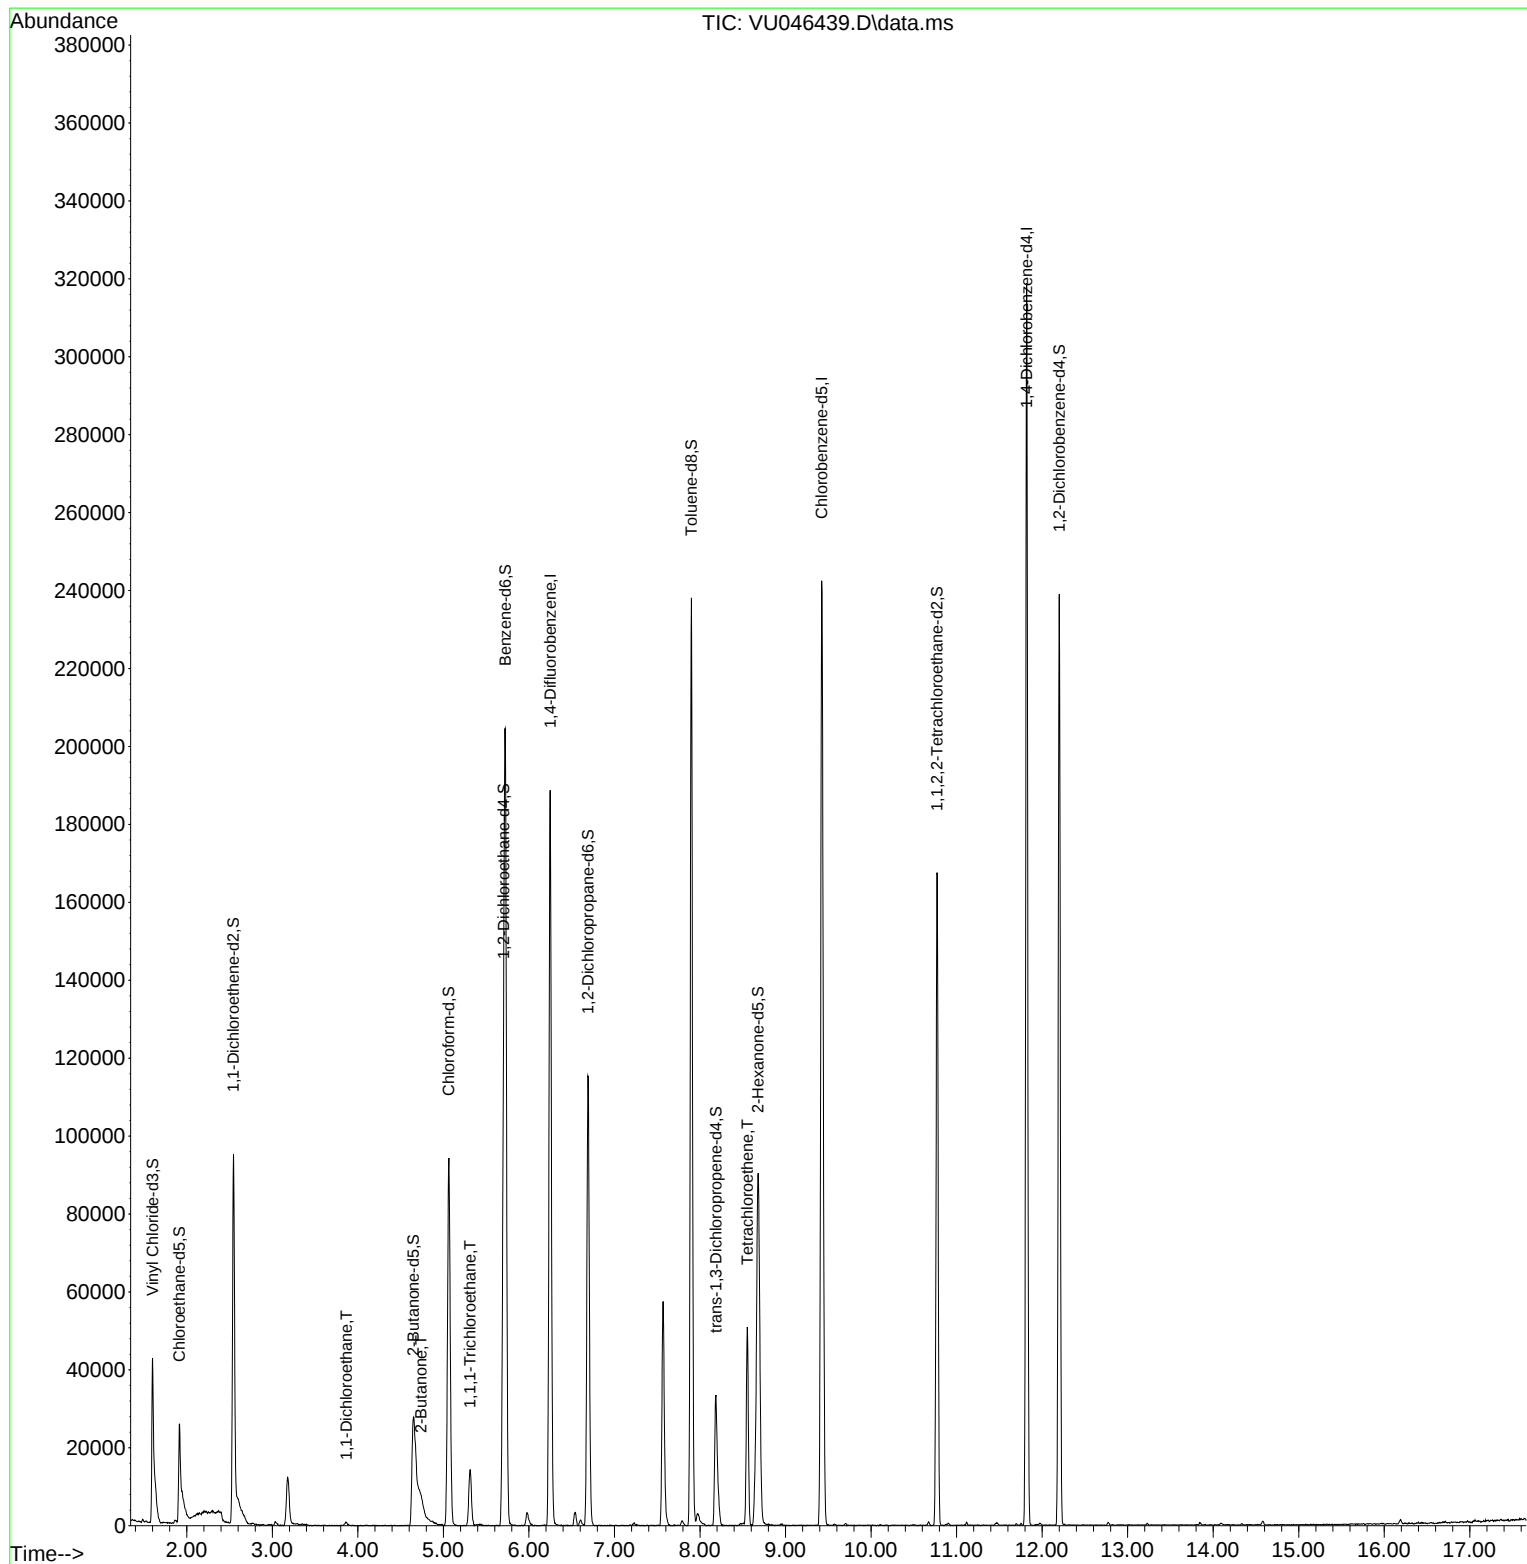

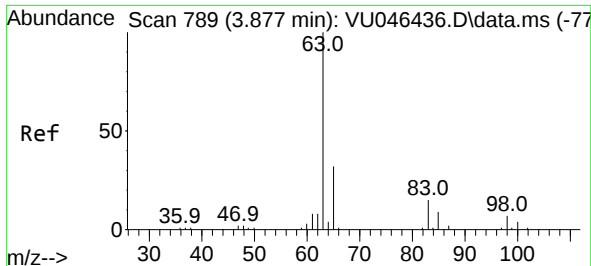

#19

1,1-Dichloroethane

Concen: 0.661 ug/L

RT: 3.864 min Scan# 71

Delta R.T. -0.013 min

Lab File: VU046439.D

Acq: 16 Dec 2021 22:54

Instrument :

MSVOA_U

ClientSampleId :

BGL35ME





Tgt Ion: 63	Resp: 136
Ion Ratio	Lower Upper
63 100	
65 25.2	22.8 42.4
83 0.0	9.6 17.8

Manual Integrations

APPROVED

Reviewed By :John Carlone 12/17/2021

Supervised By :Mahesh Dadoda 12/17/2021

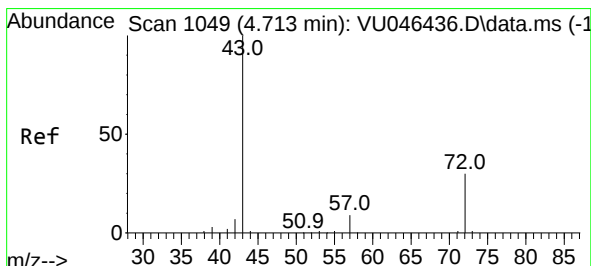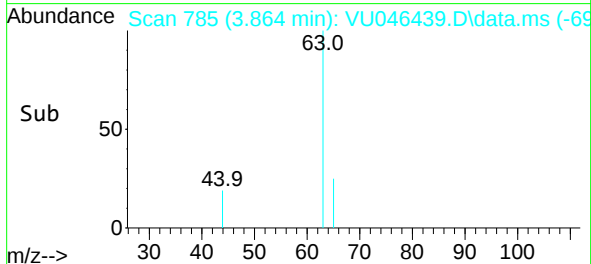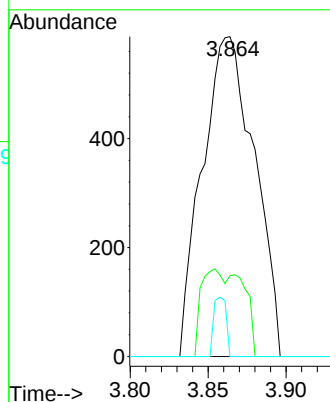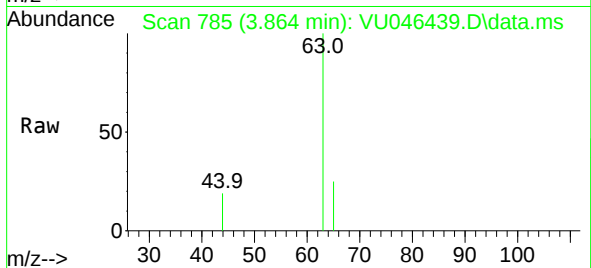

#22

2-Butanone

Concen: 7.514 ug/L m




RT: 4.739 min Scan# 1057


Delta R.T. 0.026 min

Lab File: VU046439.D

Acq: 16 Dec 2021 22:54

Tgt Ion: 43	Resp: 10413
Ion Ratio	Lower Upper
43 100	
72 20.7	14.5 43.6

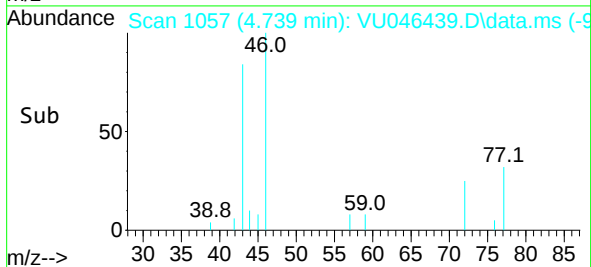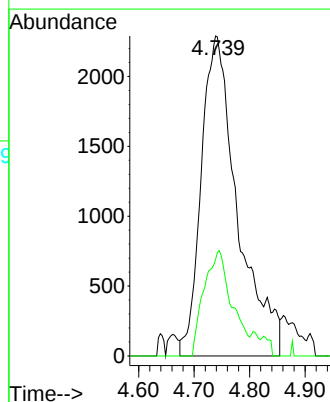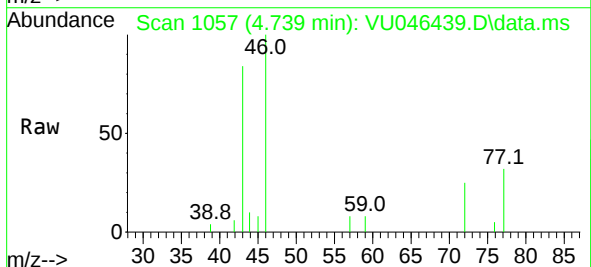

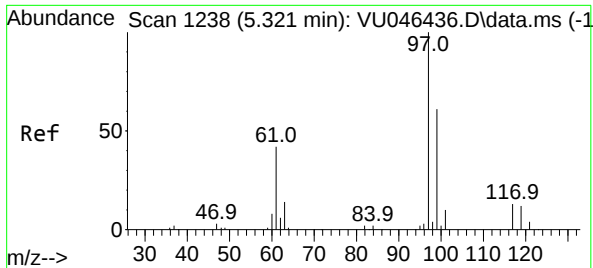

#30

1,1,1-Trichloroethane

Concen: 5.449 ug/L

RT: 5.311 min Scan# 1108

Delta R.T. -0.010 min

Lab File: VU046439.D

Acq: 16 Dec 2021 22:54

Instrument :

MSVOA_U

ClientSampleId :

BGL35ME





Tgt Ion:	97	Resp:	1108
Ion	Ratio	Lower	Upper
97	100		
99	66.3	51.8	77.6
61	43.2	34.4	51.6

Manual Integrations

APPROVED

Reviewed By :John Carlone 12/17/2021

Supervised By :Mahesh Dadoda 12/17/2021

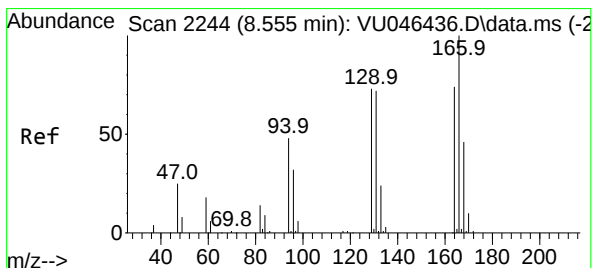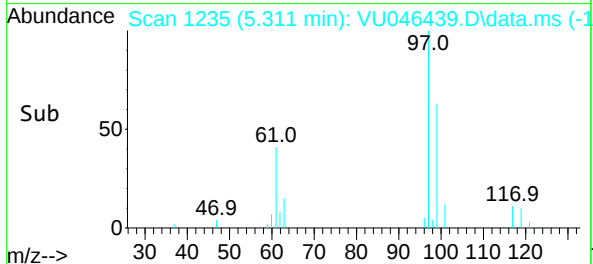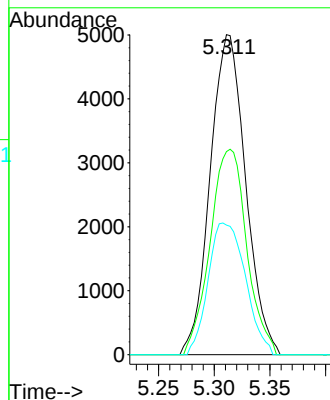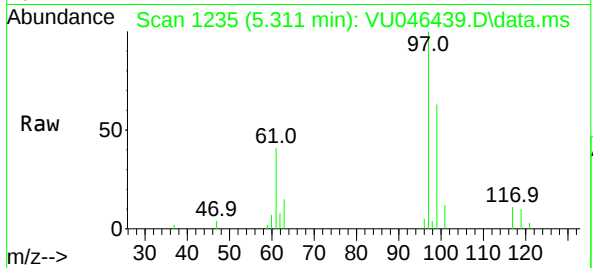

#46

Tetrachloroethene

Concen: 11.488 ug/L

RT: 8.552 min Scan# 2243

Delta R.T. -0.003 min

Lab File: VU046439.D

Acq: 16 Dec 2021 22:54

Tgt Ion:	164	Resp:	11159
Ion	Ratio	Lower	Upper
164	100		
129	100.6	71.1	132.1
131	95.8	67.8	126.0
166	126.8	90.6	168.2

