

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046411.D
 Acq On : 16 Dec 2021 11:09
 Operator : SY/MD
 Sample : VU1216MBL01
 Misc : 5.00g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK066

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046411.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	105	rBV	77108	94460	16.85%	2.142%
2	1.919	171	180	208	rBV	52197	76308	13.61%	1.731%
3	2.424	334	337	340	rBV	177	139	0.02%	0.003%
4	2.575	372	384	421	rVB	125426	211794	37.77%	4.803%
5	2.765	440	443	448	rBV	154	203	0.04%	0.005%
6	2.803	448	455	462	rVV2	268	463	0.08%	0.011%
7	2.867	470	475	480	rBV	159	222	0.04%	0.005%
8	3.054	529	533	534	rBV	227	173	0.03%	0.004%
9	3.195	571	577	582	rVB2	523	719	0.13%	0.016%
10	3.253	591	595	598	rBV	144	175	0.03%	0.004%
11	3.504	671	673	677	rBV	136	137	0.02%	0.003%
12	4.642	1012	1027	1063	rBV2	43887	131351	23.43%	2.979%
13	4.790	1070	1073	1076	rVB	212	150	0.03%	0.003%
14	4.819	1078	1082	1086	rVV2	171	155	0.03%	0.004%
15	5.070	1144	1160	1179	rBV	102372	224020	39.96%	5.081%
16	5.182	1191	1195	1198	rBB2	240	191	0.03%	0.004%
17	5.218	1203	1206	1209	rBB	143	118	0.02%	0.003%
18	5.237	1209	1212	1215	rBB	274	152	0.03%	0.003%
19	5.253	1215	1217	1221	rBB	246	165	0.03%	0.004%
20	5.289	1226	1228	1230	rVB	233	110	0.02%	0.002%
21	5.729	1344	1365	1394	rBV2	210084	560680	100.00%	12.716%
22	5.883	1410	1413	1416	rBB	132	116	0.02%	0.003%
23	6.034	1457	1460	1463	rBB	144	124	0.02%	0.003%
24	6.253	1514	1528	1550	rBV	186913	351256	62.65%	7.966%
25	6.530	1612	1614	1617	rBB	335	171	0.03%	0.004%
26	6.694	1652	1665	1685	rBV	128159	248657	44.35%	5.639%
27	6.777	1689	1691	1695	rVB2	235	162	0.03%	0.004%
28	7.211	1824	1826	1829	rBV	126	111	0.02%	0.003%
29	7.263	1840	1842	1845	rBV	132	113	0.02%	0.003%
30	7.385	1877	1880	1883	rBV	158	159	0.03%	0.004%
31	7.568	1926	1937	1958	rBB2	69798	119337	21.28%	2.706%
32	7.661	1963	1966	1968	rBV	132	112	0.02%	0.003%
33	7.816	2011	2014	2017	rBB	131	114	0.02%	0.003%
34	7.903	2027	2041	2056	rVV	255699	436267	77.81%	9.894%
35	7.973	2058	2063	2073	rVV	3439	5430	0.97%	0.123%
36	8.022	2075	2078	2080	rVB2	241	155	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046411.D
 Acq On : 16 Dec 2021 11:09
 Operator : SY/MD
 Sample : VU1216MBL01
 Misc : 5.00g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK066

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	8.182	2117	2128	2142	rBV	48485	81120	14.47%	1.840%
38	8.247	2146	2148	2154	rVB3	174	188	0.03%	0.004%
39	8.304	2164	2166	2171	rBV	244	228	0.04%	0.005%
40	8.436	2205	2207	2211	rBB	171	109	0.02%	0.002%
41	8.462	2212	2215	2216	rBV	252	130	0.02%	0.003%
42	8.491	2216	2224	2225	rBV	260	271	0.05%	0.006%
43	8.510	2227	2230	2234	rBV	335	304	0.05%	0.007%
44	8.636	2258	2269	2302	rVB	160579	273536	48.79%	6.204%
45	8.841	2329	2333	2336	rBV	133	164	0.03%	0.004%
46	8.986	2375	2378	2380	rBV	137	124	0.02%	0.003%
47	9.031	2390	2392	2396	rBB	118	107	0.02%	0.002%
48	9.060	2397	2401	2403	rBV	143	154	0.03%	0.003%
49	9.208	2444	2447	2449	rBV	136	116	0.02%	0.003%
50	9.221	2449	2451	2455	rVB	155	135	0.02%	0.003%
51	9.247	2456	2459	2463	rBB	120	110	0.02%	0.002%
52	9.340	2484	2488	2492	rBB	199	206	0.04%	0.005%
53	9.420	2500	2513	2532	rBV	275833	449732	80.21%	10.200%
54	9.568	2555	2559	2560	rBV2	210	165	0.03%	0.004%
55	9.600	2566	2569	2573	rVB	174	168	0.03%	0.004%
56	9.645	2580	2583	2590	rBV	172	251	0.04%	0.006%
57	9.697	2593	2599	2605	rVB3	557	834	0.15%	0.019%
58	9.777	2620	2624	2626	rBV	133	139	0.02%	0.003%
59	9.912	2664	2666	2670	rBB	128	114	0.02%	0.003%
60	9.947	2673	2677	2681	rBV	193	242	0.04%	0.005%
61	10.102	2722	2725	2727	rVV2	250	183	0.03%	0.004%
62	10.128	2731	2733	2737	rVB2	270	182	0.03%	0.004%
63	10.153	2738	2741	2745	rBB	150	151	0.03%	0.003%
64	10.279	2775	2780	2783	rBV	220	266	0.05%	0.006%
65	10.430	2820	2827	2829	rBV	173	252	0.04%	0.006%
66	10.481	2840	2843	2846	rBV2	216	176	0.03%	0.004%
67	10.671	2897	2902	2910	rBV2	1123	1212	0.22%	0.027%
68	10.758	2917	2929	2947	rBV	179499	286775	51.15%	6.504%
69	10.822	2947	2949	2953	rVB2	188	130	0.02%	0.003%
70	10.893	2968	2971	2981	rBV3	450	594	0.11%	0.013%
71	10.983	2995	2999	3000	rBV	164	143	0.03%	0.003%
72	11.095	3030	3034	3038	rBV2	211	188	0.03%	0.004%
73	11.462	3141	3148	3149	rBV2	753	737	0.13%	0.017%
74	11.507	3159	3162	3163	rBV	155	111	0.02%	0.003%
75	11.693	3217	3220	3223	rBV	175	156	0.03%	0.004%
76	11.751	3230	3238	3242	rBV2	676	896	0.16%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046411.D
 Acq On : 16 Dec 2021 11:09
 Operator : SY/MD
 Sample : VU1216MBL01
 Misc : 5.00g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK066

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.816	3245	3258	3276	rVV	283577	443350	79.07%	10.055%
78	11.941	3294	3297	3300	rBV2	194	187	0.03%	0.004%
79	11.976	3303	3308	3313	rVB	972	994	0.18%	0.023%
80	12.095	3341	3345	3348	rBV	220	234	0.04%	0.005%
81	12.195	3364	3376	3393	rBV	244501	387285	69.07%	8.783%
82	12.639	3510	3514	3516	rBV	200	141	0.03%	0.003%
83	12.774	3549	3556	3557	rBV	361	349	0.06%	0.008%
84	13.230	3690	3698	3703	rVB4	1008	1340	0.24%	0.030%
85	13.848	3883	3890	3896	rVB4	1989	2373	0.42%	0.054%
86	14.092	3959	3966	3978	rVB	2419	3424	0.61%	0.078%
87	14.336	4033	4042	4048	rBV3	1725	2251	0.40%	0.051%
88	14.574	4109	4116	4117	rBV2	296	319	0.06%	0.007%
89	14.857	4200	4204	4208	rBV	151	140	0.02%	0.003%
90	15.381	4365	4367	4372	rVB	254	132	0.02%	0.003%
91	15.420	4376	4379	4385	rVV2	223	182	0.03%	0.004%
92	15.507	4403	4406	4409	rBV2	217	153	0.03%	0.003%
93	15.587	4429	4431	4436	rVB2	229	162	0.03%	0.004%
94	15.748	4479	4481	4485	rVB	239	172	0.03%	0.004%
95	15.774	4485	4489	4490	rBV	204	146	0.03%	0.003%
96	15.889	4522	4525	4527	rBV	169	120	0.02%	0.003%
97	16.024	4562	4567	4570	rBV	177	226	0.04%	0.005%
98	16.327	4657	4661	4664	rBV2	279	224	0.04%	0.005%
99	16.645	4757	4760	4765	rBV3	270	308	0.05%	0.007%
100	16.854	4823	4825	4829	rBV	267	119	0.02%	0.003%




Sum of corrected areas: 4409299

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046411.D
Acq On : 16 Dec 2021 11:09
Operator : SY/MD
Sample : VU1216MBL01
Misc : 5.00g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK066

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

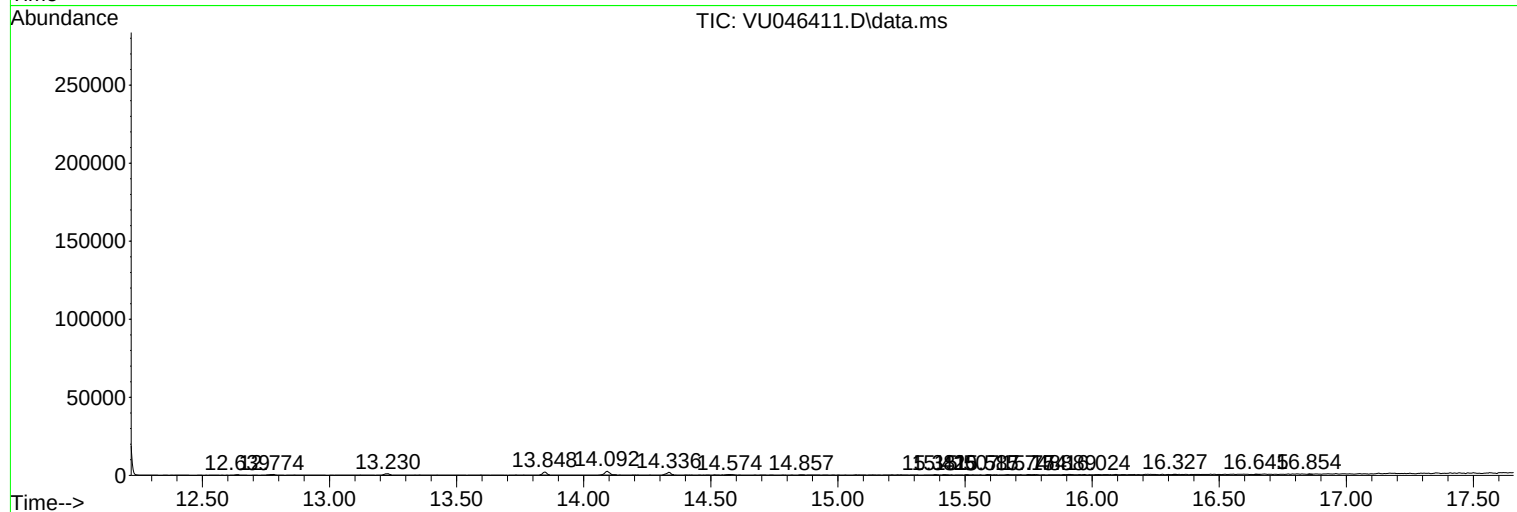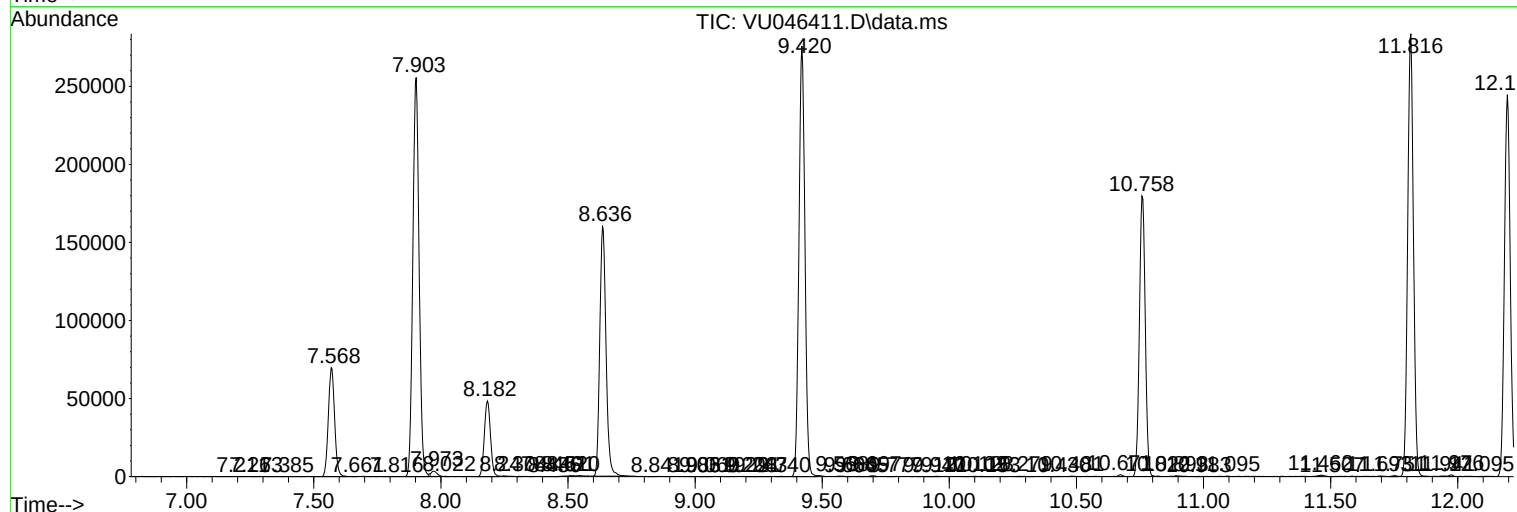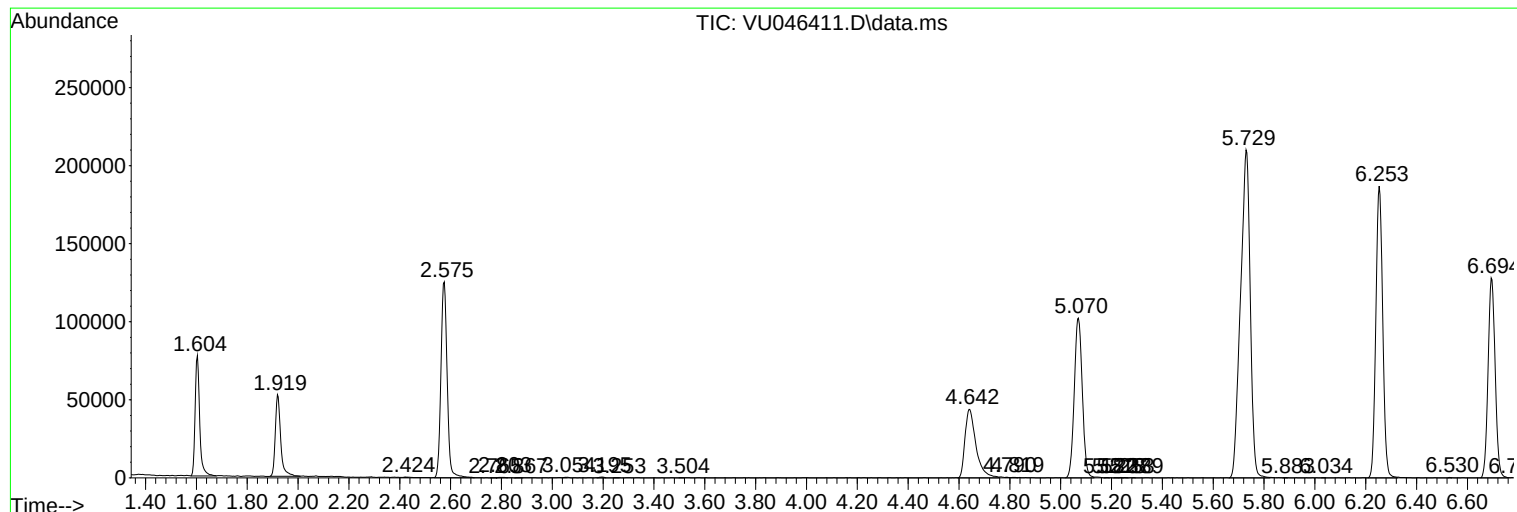

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046411.D
Acq On : 16 Dec 2021 11:09
Operator : SY/MD
Sample : VU1216MBL01
Misc : 5.00g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK066

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046411.D
Acq On : 16 Dec 2021 11:09
Operator : SY/MD
Sample : VU1216MBL01
Misc : 5.00g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK066

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc