

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046413.D
 Acq On : 16 Dec 2021 12:15
 Operator : SY/MD
 Sample : M4997-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5R2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046413.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	101	rBV	78314	95857	16.43%	1.891%
2	1.919	172	180	195	rBV	51961	74141	12.71%	1.463%
3	2.575	372	384	402	rBV	129041	216392	37.09%	4.269%
4	2.687	417	419	425	rVB	312	154	0.03%	0.003%
5	2.980	507	510	513	rBV	166	162	0.03%	0.003%
6	3.124	552	555	560	rBV	162	200	0.03%	0.004%
7	3.192	567	576	583	rVB2	715	1237	0.21%	0.024%
8	3.362	620	629	640	rVB3	2694	4855	0.83%	0.096%
9	3.877	771	789	807	rVV2	77811	183917	31.53%	3.628%
10	4.639	1012	1026	1063	rBV3	48270	174684	29.94%	3.446%
11	4.848	1088	1091	1093	rBV	130	116	0.02%	0.002%
12	4.954	1122	1124	1129	rBB	140	143	0.02%	0.003%
13	4.986	1130	1134	1140	rBB	131	207	0.04%	0.004%
14	5.070	1143	1160	1181	rBV	106544	232355	39.83%	4.583%
15	5.321	1221	1238	1258	rBV	165073	376029	64.46%	7.418%
16	5.423	1269	1270	1276	rVB2	271	233	0.04%	0.005%
17	5.729	1344	1365	1394	rBV2	216809	583375	100.00%	11.508%
18	5.973	1438	1441	1443	rBV	130	117	0.02%	0.002%
19	6.070	1468	1471	1474	rBB	121	109	0.02%	0.002%
20	6.253	1512	1528	1545	rBV	173835	323283	55.42%	6.377%
21	6.427	1578	1582	1585	rBV	164	187	0.03%	0.004%
22	6.488	1597	1601	1606	rBB	150	205	0.04%	0.004%
23	6.546	1610	1619	1630	rBB5	4152	7371	1.26%	0.145%
24	6.603	1634	1637	1640	rBV	139	142	0.02%	0.003%
25	6.693	1651	1665	1689	rBB	133922	256756	44.01%	5.065%
26	6.812	1697	1702	1704	rBV	242	241	0.04%	0.005%
27	6.874	1717	1721	1724	rBV	189	185	0.03%	0.004%
28	6.906	1728	1731	1734	rBB	165	144	0.02%	0.003%
29	6.928	1735	1738	1740	rBV	134	112	0.02%	0.002%
30	7.044	1767	1774	1777	rVV2	213	258	0.04%	0.005%
31	7.124	1797	1799	1802	rBV	133	113	0.02%	0.002%
32	7.189	1815	1819	1823	rVB2	348	317	0.05%	0.006%
33	7.269	1842	1844	1848	rBB	138	115	0.02%	0.002%
34	7.324	1857	1861	1863	rBV	129	112	0.02%	0.002%
35	7.520	1920	1922	1925	rBV	132	115	0.02%	0.002%
36	7.568	1925	1937	1958	rVB	71874	124224	21.29%	2.450%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046413.D
 Acq On : 16 Dec 2021 12:15
 Operator : SY/MD
 Sample : M4997-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5R2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	7.693	1973	1976	1977	rBV	332	201	0.03%	0.004%
38	7.825	2008	2017	2021	rBV	170	346	0.06%	0.007%
39	7.899	2027	2040	2057	rBV	263709	450742	77.26%	8.891%
40	7.970	2057	2062	2072	rVV2	3440	5625	0.96%	0.111%
41	8.009	2072	2074	2075	rVV	335	136	0.02%	0.003%
42	8.182	2117	2128	2148	rVV	49700	84193	14.43%	1.661%
43	8.256	2148	2151	2155	rBV2	255	186	0.03%	0.004%
44	8.279	2155	2158	2161	rBV2	193	160	0.03%	0.003%
45	8.320	2169	2171	2172	rBV	231	111	0.02%	0.002%
46	8.475	2208	2219	2230	rBV3	7211	13359	2.29%	0.264%
47	8.555	2234	2244	2255	rVV2	21004	34562	5.92%	0.682%
48	8.636	2257	2269	2292	rBV	163217	275508	47.23%	5.435%
49	8.970	2370	2373	2381	rBB	175	269	0.05%	0.005%
50	9.018	2384	2388	2389	rBV	137	119	0.02%	0.002%
51	9.131	2420	2423	2425	rBV	132	113	0.02%	0.002%
52	9.198	2441	2444	2447	rBV	157	155	0.03%	0.003%
53	9.330	2482	2485	2487	rBV	177	137	0.02%	0.003%
54	9.420	2500	2513	2531	rBV	261711	423144	72.53%	8.347%
55	9.693	2590	2598	2607	rVB2	348	388	0.07%	0.008%
56	9.957	2677	2680	2682	rBV	133	116	0.02%	0.002%
57	10.131	2730	2734	2743	rVB	116	153	0.03%	0.003%
58	10.201	2752	2756	2758	rBV	164	139	0.02%	0.003%
59	10.256	2767	2773	2780	rBV	204	401	0.07%	0.008%
60	10.365	2804	2807	2808	rBV	160	113	0.02%	0.002%
61	10.414	2820	2822	2825	rBV	163	134	0.02%	0.003%
62	10.497	2843	2848	2851	rBV	142	195	0.03%	0.004%
63	10.671	2896	2902	2908	rBV3	1037	1164	0.20%	0.023%
64	10.758	2917	2929	2944	rBV	188830	293573	50.32%	5.791%
65	10.896	2961	2972	2985	rVB	6990	11789	2.02%	0.233%
66	11.018	3007	3010	3012	rBV	155	134	0.02%	0.003%
67	11.140	3044	3048	3049	rBV	160	135	0.02%	0.003%
68	11.459	3141	3147	3156	rVB3	663	1047	0.18%	0.021%
69	11.581	3180	3185	3188	rBV2	224	222	0.04%	0.004%
70	11.696	3218	3221	3226	rVB2	286	253	0.04%	0.005%
71	11.812	3245	3257	3278	rBV	258029	402602	69.01%	7.942%
72	11.941	3290	3297	3302	rBV2	267	429	0.07%	0.008%
73	11.976	3304	3308	3313	rVB	832	686	0.12%	0.014%
74	12.066	3333	3336	3339	rBV	274	192	0.03%	0.004%
75	12.195	3363	3376	3392	rBV	248645	399658	68.51%	7.884%
76	12.574	3491	3494	3501	rVB	144	141	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046413.D
 Acq On : 16 Dec 2021 12:15
 Operator : SY/MD
 Sample : M4997-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5R2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	12.639	3511	3514	3519	rVB	195	155	0.03%	0.003%
78	12.777	3546	3557	3564	rBV3	2244	3392	0.58%	0.067%
79	13.221	3692	3695	3697	rBV	217	126	0.02%	0.002%
80	13.362	3736	3739	3745	rBV	142	187	0.03%	0.004%
81	13.513	3783	3786	3791	rBV	110	129	0.02%	0.003%
82	13.848	3885	3890	3895	rBV2	346	255	0.04%	0.005%
83	13.873	3895	3898	3902	rBV	144	136	0.02%	0.003%
84	14.089	3962	3965	3966	rBV	177	113	0.02%	0.002%
85	14.230	4005	4009	4013	rBV	117	137	0.02%	0.003%
86	14.577	4114	4117	4127	rVB2	664	788	0.14%	0.016%
87	15.259	4327	4329	4333	rVB	192	119	0.02%	0.002%
88	15.407	4372	4375	4378	rBV2	166	122	0.02%	0.002%
89	15.494	4400	4402	4409	rVB	274	170	0.03%	0.003%
90	15.529	4409	4413	4415	rBV	206	168	0.03%	0.003%
91	15.645	4446	4449	4453	rVB	231	140	0.02%	0.003%
92	15.671	4454	4457	4460	rBV2	155	124	0.02%	0.002%
93	15.796	4492	4496	4499	rBV2	186	200	0.03%	0.004%
94	15.896	4524	4527	4532	rVB	286	245	0.04%	0.005%
95	15.921	4532	4535	4538	rBV	268	218	0.04%	0.004%
96	15.963	4546	4548	4552	rBV2	199	213	0.04%	0.004%
97	16.056	4574	4577	4580	rBV	238	202	0.03%	0.004%
98	16.658	4762	4764	4766	rBV2	272	110	0.02%	0.002%
99	17.253	4946	4949	4951	rBV2	608	454	0.08%	0.009%
100	17.452	5009	5011	5017	rBV5	640	622	0.11%	0.012%




Sum of corrected areas: 5069418

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046413.D
Acq On : 16 Dec 2021 12:15
Operator : SY/MD
Sample : M4997-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5R2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

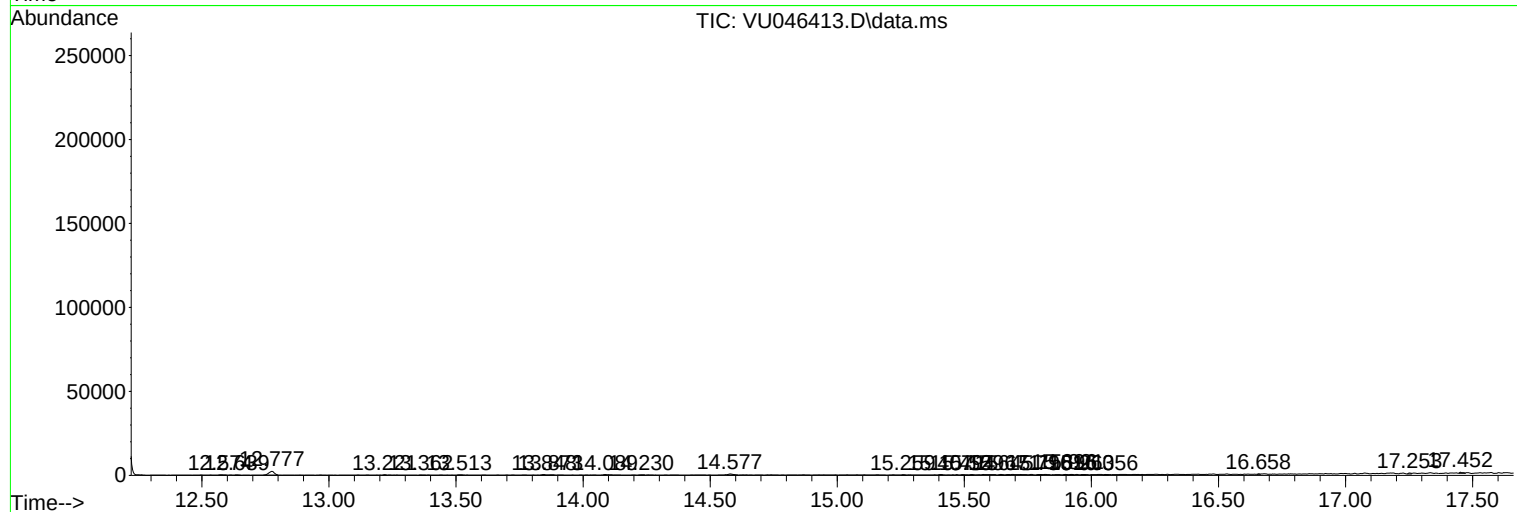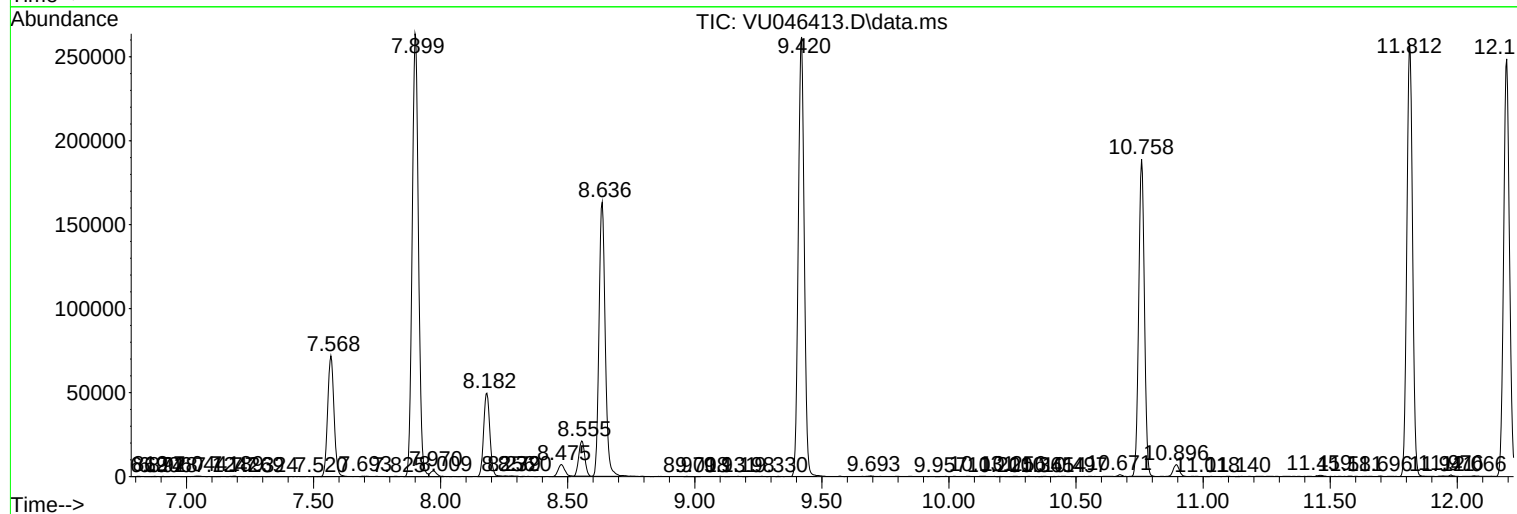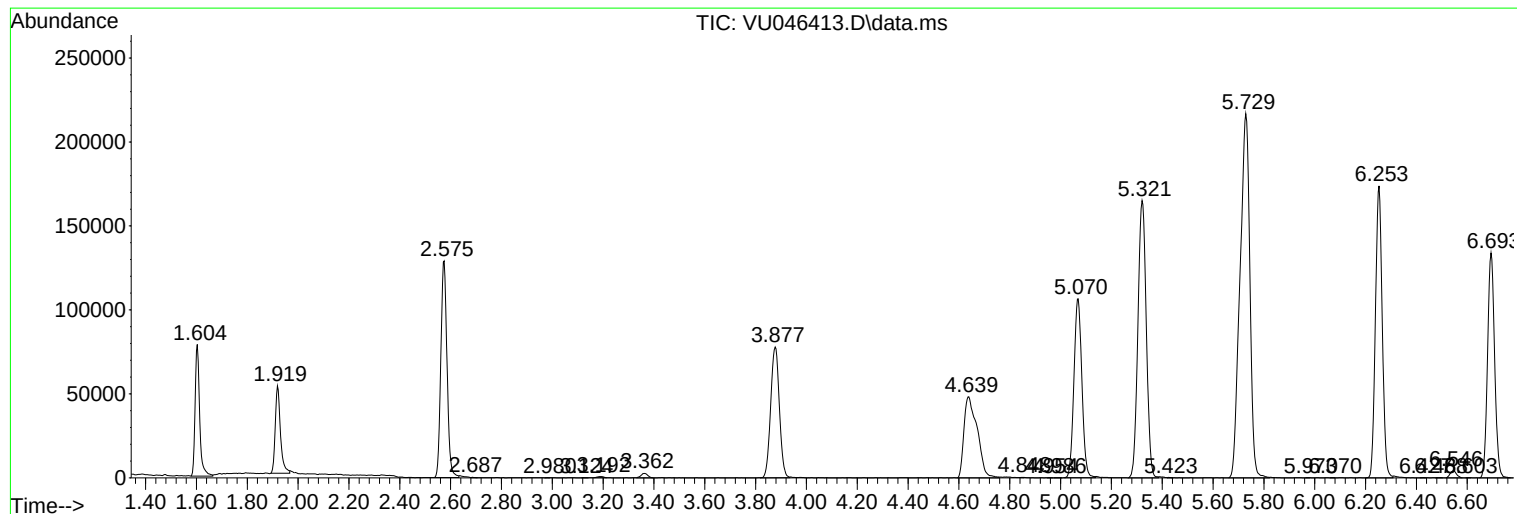

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046413.D
Acq On : 16 Dec 2021 12:15
Operator : SY/MD
Sample : M4997-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5R2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046413.D
Acq On : 16 Dec 2021 12:15
Operator : SY/MD
Sample : M4997-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5R2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------