

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046424.D
 Acq On : 16 Dec 2021 16:24
 Operator : SY/MD
 Sample : M5037-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C00X4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046424.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.363	3	7	14	rVB	2510	2359	0.42%	0.053%
2	1.600	74	81	100	rBV	73201	91482	16.18%	2.038%
3	1.919	171	180	203	rBV	50289	72473	12.82%	1.614%
4	2.346	311	313	316	rVB2	182	107	0.02%	0.002%
5	2.375	318	322	327	rVB2	228	168	0.03%	0.004%
6	2.571	371	383	402	rBV	122729	202482	35.81%	4.510%
7	2.797	448	453	454	rBV	248	159	0.03%	0.004%
8	3.028	522	525	527	rBV	134	118	0.02%	0.003%
9	3.044	527	530	533	rVV2	255	188	0.03%	0.004%
10	3.060	533	535	540	rVB	164	131	0.02%	0.003%
11	3.192	569	576	581	rBB	173	297	0.05%	0.007%
12	3.301	606	610	613	rBV	162	187	0.03%	0.004%
13	3.366	628	630	634	rBB	131	120	0.02%	0.003%
14	3.549	684	687	689	rBV	165	127	0.02%	0.003%
15	4.102	857	859	865	rBB	152	171	0.03%	0.004%
16	4.633	1010	1024	1058	rVV	48781	126379	22.35%	2.815%
17	4.883	1100	1102	1105	rBV	132	112	0.02%	0.002%
18	5.067	1144	1159	1181	rBV	103858	224980	39.78%	5.011%
19	5.163	1187	1189	1191	rVB	265	122	0.02%	0.003%
20	5.186	1195	1196	1199	rVB	338	133	0.02%	0.003%
21	5.247	1211	1215	1218	rBB	157	150	0.03%	0.003%
22	5.427	1268	1271	1275	rBB	121	130	0.02%	0.003%
23	5.565	1311	1314	1317	rBB	120	108	0.02%	0.002%
24	5.729	1344	1365	1386	rBV2	211982	565492	100.00%	12.596%
25	5.848	1399	1402	1405	rVV	150	109	0.02%	0.002%
26	5.864	1405	1407	1411	rVB2	263	237	0.04%	0.005%
27	6.253	1514	1528	1552	rBV	177944	332957	58.88%	7.417%
28	6.433	1581	1584	1587	rBB	155	131	0.02%	0.003%
29	6.694	1652	1665	1686	rVV	129900	249760	44.17%	5.563%
30	6.777	1690	1691	1694	rVB2	254	116	0.02%	0.003%
31	6.803	1694	1699	1703	rBB2	233	223	0.04%	0.005%
32	6.948	1741	1744	1748	rBB	139	141	0.02%	0.003%
33	7.044	1772	1774	1777	rVB2	246	118	0.02%	0.003%
34	7.176	1813	1815	1816	rBV2	248	105	0.02%	0.002%
35	7.568	1925	1937	1959	rBV	68062	118595	20.97%	2.642%
36	7.687	1970	1974	1979	rVB2	277	340	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046424.D
 Acq On : 16 Dec 2021 16:24
 Operator : SY/MD
 Sample : M5037-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C00X4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	7.755	1992	1995	1998	rBB	139	118	0.02%	0.003%
38	7.780	1998	2003	2006	rBB	156	183	0.03%	0.004%
39	7.832	2016	2019	2022	rVV	189	188	0.03%	0.004%
40	7.899	2026	2040	2055	rBV	254263	434441	76.83%	9.677%
41	7.970	2058	2062	2074	rVV2	4673	7101	1.26%	0.158%
42	8.025	2076	2079	2083	rVB2	264	240	0.04%	0.005%
43	8.060	2086	2090	2093	rBB	121	127	0.02%	0.003%
44	8.140	2112	2115	2117	rBV	150	127	0.02%	0.003%
45	8.182	2117	2128	2142	rVV	48787	80568	14.25%	1.795%
46	8.317	2166	2170	2173	rVV	171	159	0.03%	0.004%
47	8.382	2186	2190	2193	rBB	123	129	0.02%	0.003%
48	8.414	2198	2200	2204	rBB	142	120	0.02%	0.003%
49	8.475	2209	2219	2229	rBV2	4232	7608	1.35%	0.169%
50	8.526	2232	2235	2237	rVV	455	342	0.06%	0.008%
51	8.552	2241	2243	2246	rVB	195	119	0.02%	0.003%
52	8.636	2257	2269	2297	rBV	161550	273456	48.36%	6.091%
53	8.767	2306	2310	2312	rBV	160	136	0.02%	0.003%
54	8.912	2351	2355	2360	rBB	176	210	0.04%	0.005%
55	8.938	2360	2363	2368	rBB	175	192	0.03%	0.004%
56	9.057	2397	2400	2401	rBV	151	105	0.02%	0.002%
57	9.121	2416	2420	2422	rBV	132	138	0.02%	0.003%
58	9.179	2433	2438	2444	rBV	148	275	0.05%	0.006%
59	9.420	2500	2513	2536	rBV	264358	480957	85.05%	10.713%
60	9.513	2539	2542	2548	rBV2	252	308	0.05%	0.007%
61	9.578	2559	2562	2563	rBV	275	177	0.03%	0.004%
62	9.648	2581	2584	2589	rBV	146	197	0.03%	0.004%
63	9.693	2594	2598	2605	rBV2	687	834	0.15%	0.019%
64	9.729	2605	2609	2612	rVB	191	183	0.03%	0.004%
65	9.790	2625	2628	2630	rBV	144	123	0.02%	0.003%
66	9.967	2680	2683	2686	rBV	133	141	0.02%	0.003%
67	10.185	2748	2751	2753	rBV	153	131	0.02%	0.003%
68	10.250	2768	2771	2775	rBV	155	181	0.03%	0.004%
69	10.359	2801	2805	2807	rBV	153	150	0.03%	0.003%
70	10.394	2812	2816	2821	rBV	175	265	0.05%	0.006%
71	10.523	2853	2856	2861	rBV	149	219	0.04%	0.005%
72	10.671	2897	2902	2904	rBV4	836	784	0.14%	0.017%
73	10.758	2916	2929	2946	rVV	181447	289398	51.18%	6.446%
74	10.893	2963	2971	2982	rVB2	5074	8077	1.43%	0.180%
75	11.063	3018	3024	3027	rBV	173	256	0.05%	0.006%
76	11.455	3140	3146	3154	rVB4	628	947	0.17%	0.021%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046424.D
 Acq On : 16 Dec 2021 16:24
 Operator : SY/MD
 Sample : M5037-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C00X4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.578	3180	3184	3187	rBV	177	151	0.03%	0.003%
78	11.700	3221	3222	3227	rVB	262	167	0.03%	0.004%
79	11.748	3229	3237	3245	rVB2	5331	7252	1.28%	0.162%
80	11.812	3245	3257	3276	rBV	276949	452963	80.10%	10.090%
81	11.970	3302	3306	3313	rVB3	841	1039	0.18%	0.023%
82	12.063	3328	3335	3346	rBV4	1331	1956	0.35%	0.044%
83	12.140	3355	3359	3361	rBV	190	113	0.02%	0.003%
84	12.195	3363	3376	3393	rVB	259507	409782	72.46%	9.128%
85	12.578	3490	3495	3497	rBV	152	146	0.03%	0.003%
86	12.770	3548	3555	3564	rVB3	1384	2220	0.39%	0.049%
87	12.973	3613	3618	3623	rVB3	784	970	0.17%	0.022%
88	13.841	3878	3888	3899	rBV2	16539	23852	4.22%	0.531%
89	14.095	3964	3967	3972	rVB	308	282	0.05%	0.006%
90	14.137	3977	3980	3986	rBV	122	147	0.03%	0.003%
91	14.330	4033	4040	4050	rVB4	3897	5728	1.01%	0.128%
92	14.577	4113	4117	4124	rVB2	453	594	0.11%	0.013%
93	15.147	4291	4294	4298	rBV	160	121	0.02%	0.003%
94	15.716	4468	4471	4474	rVB2	287	203	0.04%	0.005%
95	15.754	4481	4483	4488	rBV2	195	157	0.03%	0.003%
96	15.854	4511	4514	4518	rVB	274	252	0.04%	0.006%
97	15.880	4518	4522	4524	rBV	192	157	0.03%	0.003%
98	16.208	4621	4624	4627	rBV	216	188	0.03%	0.004%
99	16.285	4646	4648	4651	rBV2	240	129	0.02%	0.003%
100	17.034	4877	4881	4883	rBV2	426	399	0.07%	0.009%




Sum of corrected areas: 4489385

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046424.D
Acq On : 16 Dec 2021 16:24
Operator : SY/MD
Sample : M5037-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C00X4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

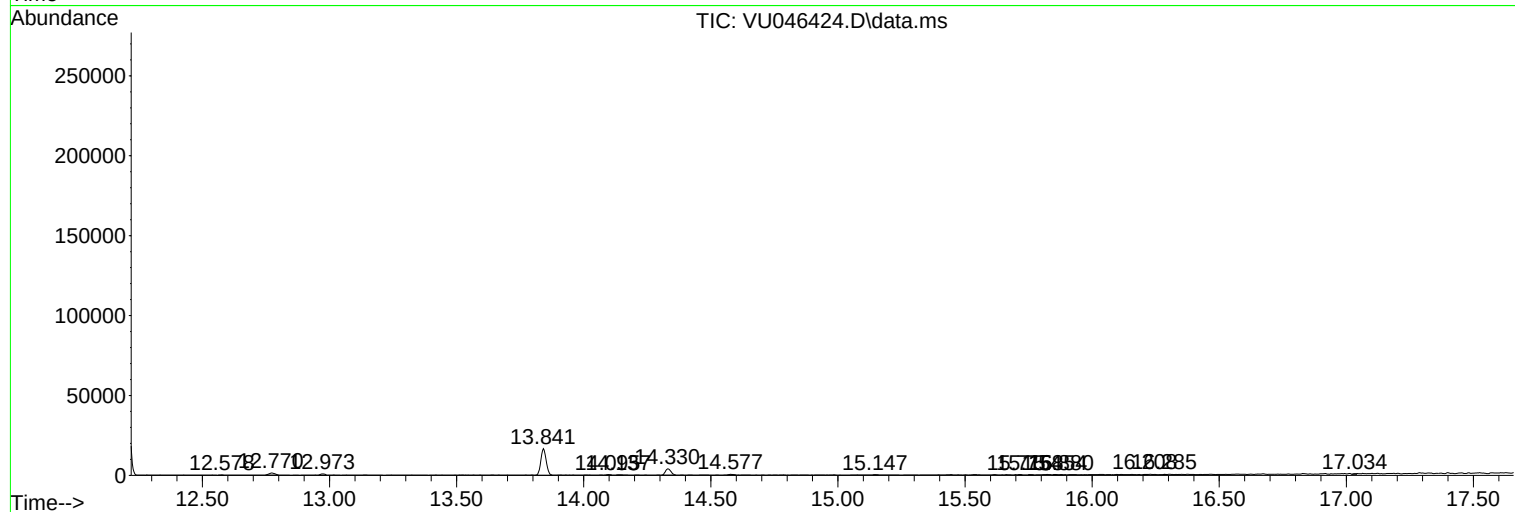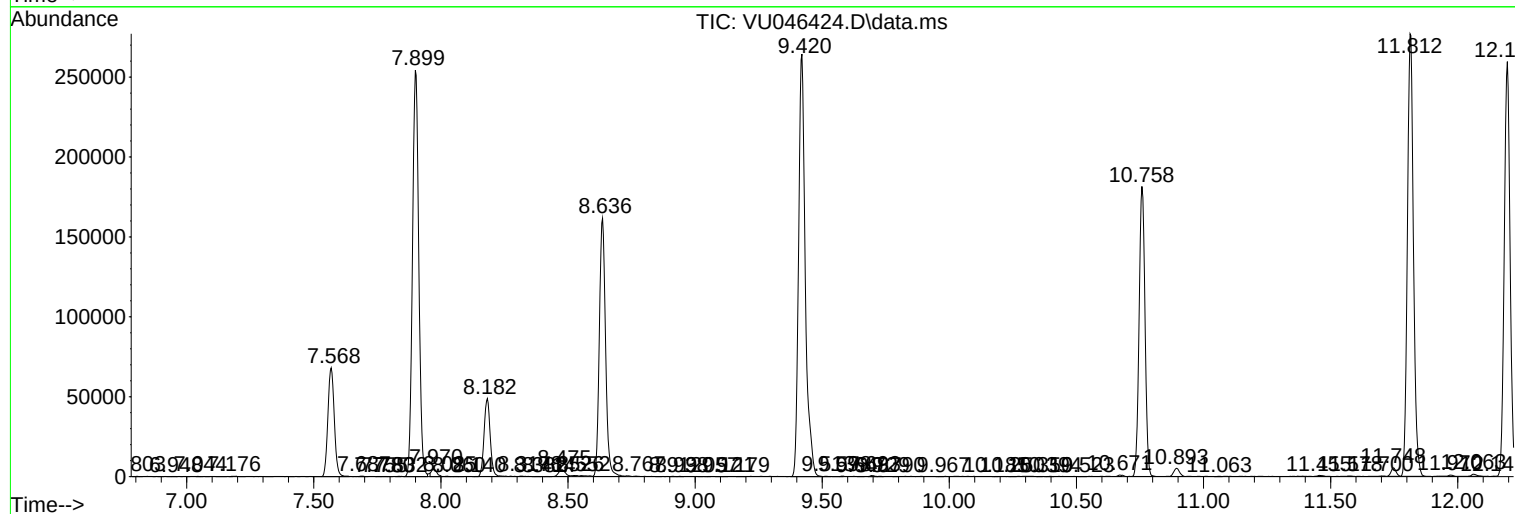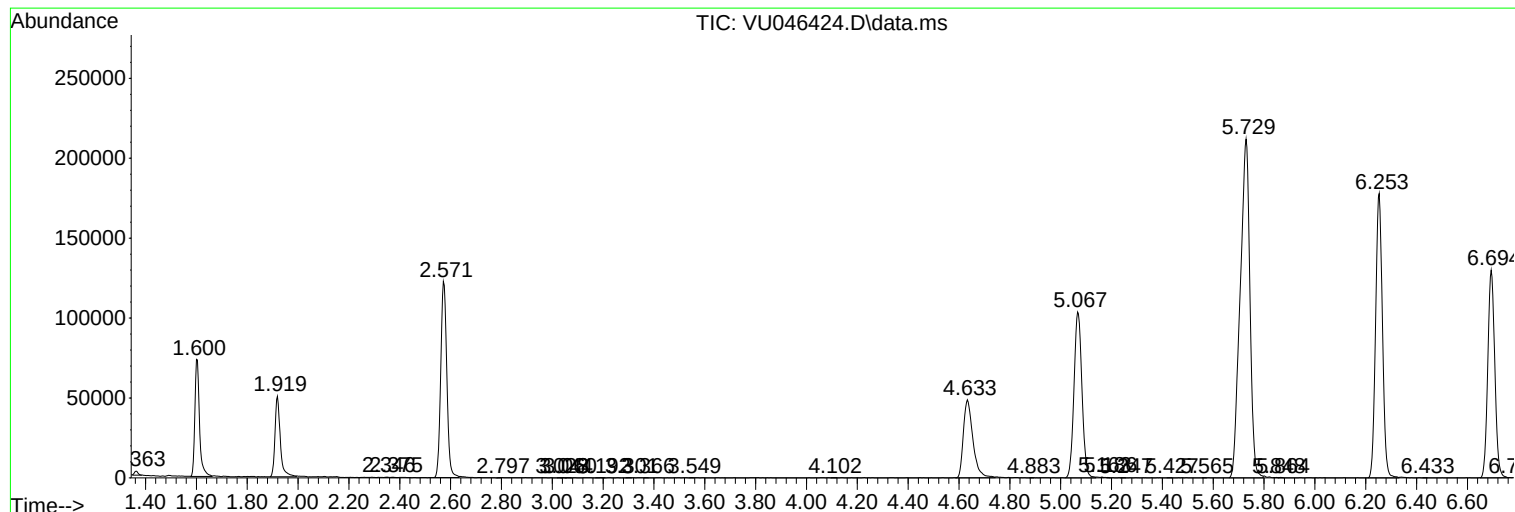

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046424.D
Acq On : 16 Dec 2021 16:24
Operator : SY/MD
Sample : M5037-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C00X4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046424.D
Acq On : 16 Dec 2021 16:24
Operator : SY/MD
Sample : M5037-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C00X4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
