

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046426.D
 Acq On : 16 Dec 2021 17:09
 Operator : SY/MD
 Sample : M5037-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C00X8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046426.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.363	3	7	13	rBV	2028	1812	0.33%	0.043%
2	1.601	74	81	107	rVB	70207	88552	16.24%	2.102%
3	1.919	171	180	204	rBV	48402	68405	12.54%	1.624%
4	2.166	254	257	261	rVB2	452	340	0.06%	0.008%
5	2.247	279	282	286	rBV	211	187	0.03%	0.004%
6	2.511	361	364	366	rBV	157	136	0.02%	0.003%
7	2.572	371	383	404	rVV	118580	198497	36.39%	4.713%
8	2.829	460	463	466	rBV	151	148	0.03%	0.004%
9	2.957	498	503	505	rBV	166	195	0.04%	0.005%
10	2.993	511	514	516	rBV	145	117	0.02%	0.003%
11	3.112	545	551	554	rBV	134	187	0.03%	0.004%
12	3.186	570	574	575	rBV2	381	289	0.05%	0.007%
13	3.195	575	577	582	rVB2	400	322	0.06%	0.008%
14	3.311	610	613	616	rBB	179	137	0.03%	0.003%
15	3.527	678	680	685	rBB	133	139	0.03%	0.003%
16	3.617	705	708	712	rBB	149	152	0.03%	0.004%
17	3.748	747	749	752	rVB	164	113	0.02%	0.003%
18	3.874	781	788	791	rBV2	675	870	0.16%	0.021%
19	4.096	853	857	860	rBV	147	177	0.03%	0.004%
20	4.633	1011	1024	1048	rBV	47865	122864	22.53%	2.917%
21	4.784	1068	1071	1073	rBV	186	149	0.03%	0.004%
22	5.067	1142	1159	1186	rBV	100112	218186	40.00%	5.180%
23	5.179	1191	1194	1195	rBV	249	143	0.03%	0.003%
24	5.321	1228	1238	1247	rBB3	1726	3287	0.60%	0.078%
25	5.485	1287	1289	1292	rBV	145	119	0.02%	0.003%
26	5.729	1344	1365	1386	rBV2	200606	545437	100.00%	12.950%
27	6.253	1514	1528	1552	rBV	166249	311228	57.06%	7.389%
28	6.385	1565	1569	1572	rBB	257	160	0.03%	0.004%
29	6.420	1577	1580	1584	rBB	155	125	0.02%	0.003%
30	6.533	1613	1615	1618	rBB	281	174	0.03%	0.004%
31	6.694	1650	1665	1692	rVB	125116	243909	44.72%	5.791%
32	6.867	1716	1719	1721	rBV	146	130	0.02%	0.003%
33	7.044	1770	1774	1777	rBV	230	216	0.04%	0.005%
34	7.079	1782	1785	1788	rBV	139	118	0.02%	0.003%
35	7.173	1811	1814	1815	rBV	209	109	0.02%	0.003%
36	7.247	1832	1837	1839	rBB	147	150	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046426.D
 Acq On : 16 Dec 2021 17:09
 Operator : SY/MD
 Sample : M5037-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C00X8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	7.362	1870	1873	1877	rBB	143	151	0.03%	0.004%
38	7.504	1915	1917	1921	rBB	188	117	0.02%	0.003%
39	7.568	1924	1937	1952	rVV2	66347	114061	20.91%	2.708%
40	7.899	2027	2040	2056	rBV	247018	421313	77.24%	10.003%
41	7.970	2058	2062	2075	rVV4	3214	5002	0.92%	0.119%
42	8.182	2115	2128	2142	rBV	47332	77599	14.23%	1.842%
43	8.253	2147	2150	2152	rBV	156	115	0.02%	0.003%
44	8.311	2165	2168	2173	rVB2	184	199	0.04%	0.005%
45	8.475	2208	2219	2230	rBV4	2501	5048	0.93%	0.120%
46	8.530	2233	2236	2239	rBV2	187	157	0.03%	0.004%
47	8.575	2248	2250	2253	rBV2	184	126	0.02%	0.003%
48	8.636	2257	2269	2289	rBV	159322	264044	48.41%	6.269%
49	8.780	2311	2314	2316	rBV2	240	189	0.03%	0.004%
50	8.931	2357	2361	2364	rBV	171	185	0.03%	0.004%
51	9.086	2405	2409	2413	rBV	160	209	0.04%	0.005%
52	9.185	2438	2440	2443	rBV	148	130	0.02%	0.003%
53	9.240	2455	2457	2463	rVB	170	164	0.03%	0.004%
54	9.324	2480	2483	2488	rVB	180	206	0.04%	0.005%
55	9.353	2489	2492	2493	rBV	155	109	0.02%	0.003%
56	9.420	2500	2513	2538	rBV	252184	423026	77.56%	10.043%
57	9.549	2548	2553	2558	rBV	145	235	0.04%	0.006%
58	9.642	2579	2582	2584	rBV	171	137	0.03%	0.003%
59	9.693	2595	2598	2599	rBV	417	261	0.05%	0.006%
60	9.793	2626	2629	2634	rBV	146	198	0.04%	0.005%
61	9.980	2682	2687	2690	rBV	168	234	0.04%	0.006%
62	10.057	2708	2711	2714	rBB	193	155	0.03%	0.004%
63	10.176	2745	2748	2750	rBV	156	140	0.03%	0.003%
64	10.224	2760	2763	2767	rBV	135	165	0.03%	0.004%
65	10.346	2799	2801	2806	rBV	165	191	0.04%	0.005%
66	10.465	2835	2838	2846	rVB	178	277	0.05%	0.007%
67	10.504	2846	2850	2853	rBV	184	204	0.04%	0.005%
68	10.674	2895	2903	2911	rBV	985	1199	0.22%	0.028%
69	10.758	2916	2929	2949	rVB	178321	282290	51.75%	6.702%
70	10.896	2964	2972	2983	rVB3	3370	5198	0.95%	0.123%
71	11.018	3007	3010	3015	rBV	150	204	0.04%	0.005%
72	11.455	3140	3146	3147	rBV2	521	431	0.08%	0.010%
73	11.584	3182	3186	3193	rVB2	333	335	0.06%	0.008%
74	11.626	3193	3199	3202	rBV2	181	192	0.04%	0.005%
75	11.687	3215	3218	3220	rBV	158	119	0.02%	0.003%
76	11.812	3244	3257	3275	rVV	255554	402963	73.88%	9.567%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046426.D
 Acq On : 16 Dec 2021 17:09
 Operator : SY/MD
 Sample : M5037-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C00X8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.880	3275	3278	3281	rVB2	167	139	0.03%	0.003%
78	11.944	3291	3298	3301	rBV2	286	410	0.08%	0.010%
79	11.973	3304	3307	3316	rVB3	748	750	0.14%	0.018%
80	12.063	3329	3335	3342	rBV2	721	954	0.17%	0.023%
81	12.131	3353	3356	3360	rBV	242	138	0.03%	0.003%
82	12.195	3363	3376	3389	rBV	245550	389400	71.39%	9.245%
83	12.661	3516	3521	3524	rBV	130	110	0.02%	0.003%
84	12.774	3548	3556	3565	rVB3	812	1236	0.23%	0.029%
85	12.976	3612	3619	3623	rVB2	808	959	0.18%	0.023%
86	13.851	3887	3891	3893	rBV	134	113	0.02%	0.003%
87	14.574	4112	4116	4124	rVB2	357	518	0.09%	0.012%
88	15.005	4246	4250	4253	rBV	172	141	0.03%	0.003%
89	15.565	4421	4424	4428	rBV	195	125	0.02%	0.003%
90	15.613	4435	4439	4443	rBV	220	212	0.04%	0.005%
91	15.658	4450	4453	4455	rBV	225	143	0.03%	0.003%
92	15.722	4468	4473	4476	rBV	236	225	0.04%	0.005%
93	15.745	4476	4480	4484	rBV	329	272	0.05%	0.006%
94	15.809	4497	4500	4502	rBV2	223	129	0.02%	0.003%
95	15.893	4524	4526	4528	rBV2	218	128	0.02%	0.003%
96	15.909	4528	4531	4535	rVV	147	142	0.03%	0.003%
97	16.044	4567	4573	4575	rBV2	245	267	0.05%	0.006%
98	16.513	4716	4719	4722	rBV2	271	213	0.04%	0.005%
99	16.954	4853	4856	4860	rBV2	456	373	0.07%	0.009%
100	17.584	5049	5052	5054	rBV2	500	344	0.06%	0.008%




Sum of corrected areas: 4211998

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046426.D
Acq On : 16 Dec 2021 17:09
Operator : SY/MD
Sample : M5037-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C00X8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

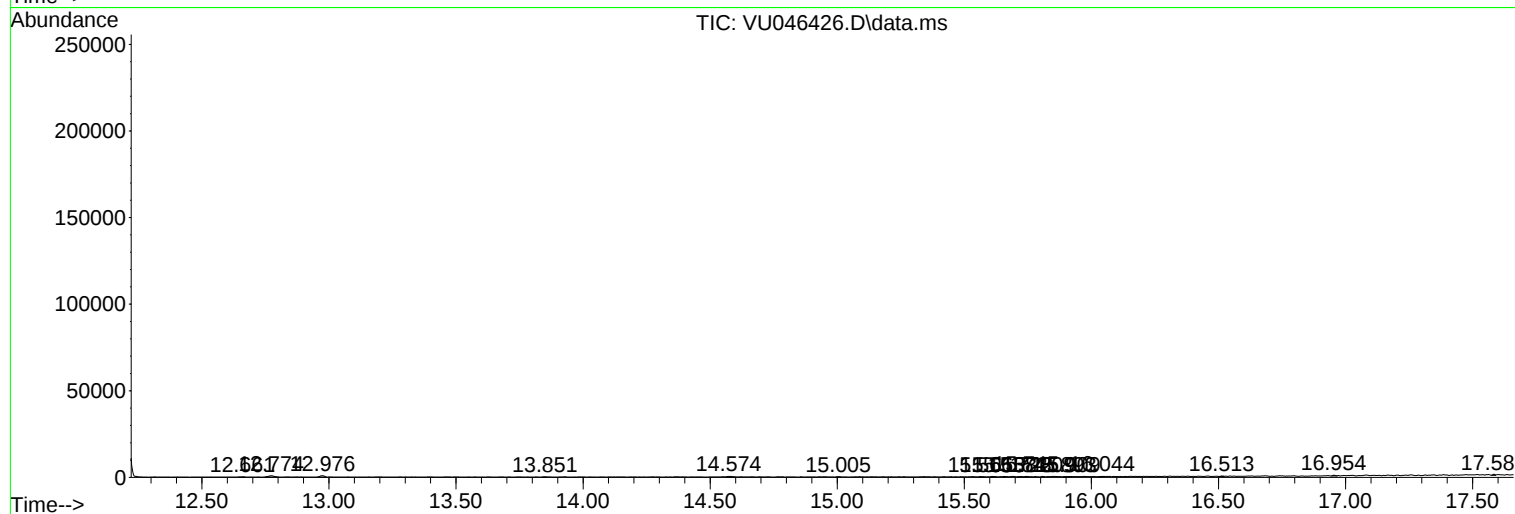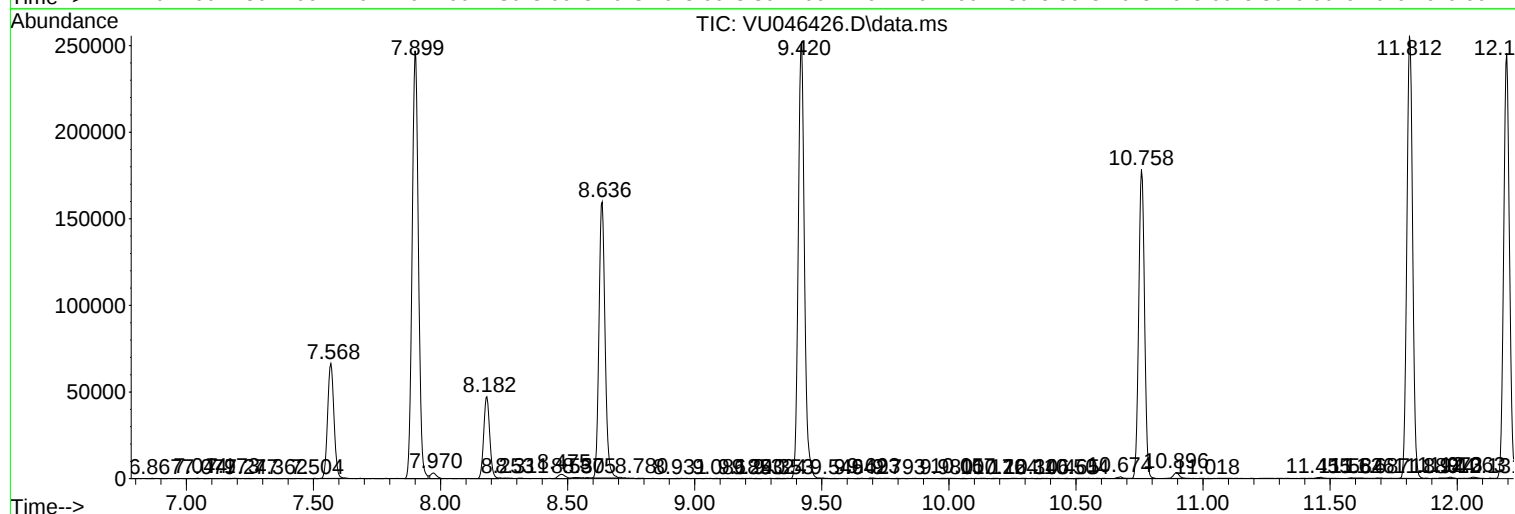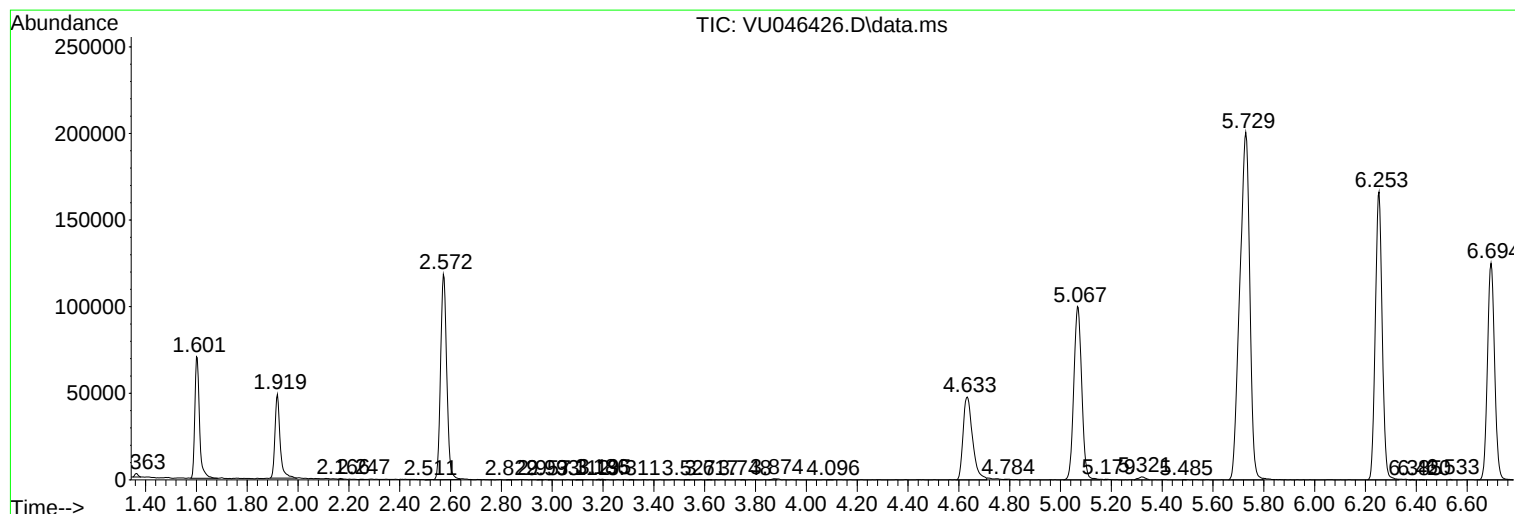

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046426.D
Acq On : 16 Dec 2021 17:09
Operator : SY/MD
Sample : M5037-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C00X8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046426.D
Acq On : 16 Dec 2021 17:09
Operator : SY/MD
Sample : M5037-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C00X8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc