

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046427.D
 Acq On : 16 Dec 2021 17:32
 Operator : SY/MD
 Sample : M5037-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C00Y0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046427.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	101	rBV	72495	89439	15.94%	2.050%
2	1.919	171	180	204	rBV	49771	72153	12.86%	1.654%
3	2.205	265	269	271	rBV2	235	182	0.03%	0.004%
4	2.372	318	321	324	rBV2	191	117	0.02%	0.003%
5	2.572	371	383	406	rBV	121016	200400	35.73%	4.593%
6	2.649	406	407	412	rVB2	486	335	0.06%	0.008%
7	2.752	436	439	442	rBV	213	186	0.03%	0.004%
8	2.793	447	452	455	rBB	151	173	0.03%	0.004%
9	2.916	487	490	494	rBB	163	157	0.03%	0.004%
10	2.993	511	514	516	rBV	132	114	0.02%	0.003%
11	3.642	713	716	720	rBB	169	155	0.03%	0.004%
12	3.681	725	728	731	rBB	131	117	0.02%	0.003%
13	3.793	761	763	766	rBV	126	115	0.02%	0.003%
14	3.903	792	797	799	rBV	138	163	0.03%	0.004%
15	4.031	833	837	843	rBV	133	231	0.04%	0.005%
16	4.179	880	883	885	rBV	145	127	0.02%	0.003%
17	4.391	946	949	952	rBB	150	125	0.02%	0.003%
18	4.633	1011	1024	1060	rBV	47982	124814	22.25%	2.861%
19	4.813	1078	1080	1084	rVB	281	184	0.03%	0.004%
20	4.838	1085	1088	1091	rBV	231	196	0.03%	0.004%
21	4.864	1092	1096	1098	rVB2	258	205	0.04%	0.005%
22	5.067	1143	1159	1187	rBV2	102159	224054	39.94%	5.135%
23	5.186	1193	1196	1199	rVB2	369	257	0.05%	0.006%
24	5.208	1199	1203	1204	rBV	177	146	0.03%	0.003%
25	5.221	1204	1207	1211	rVB2	267	240	0.04%	0.006%
26	5.243	1212	1214	1215	rBV	259	122	0.02%	0.003%
27	5.285	1225	1227	1229	rBV2	249	163	0.03%	0.004%
28	5.295	1229	1230	1232	rVB	344	111	0.02%	0.003%
29	5.729	1344	1365	1391	rBV2	208158	560935	100.00%	12.857%
30	6.115	1482	1485	1488	rBB	186	139	0.02%	0.003%
31	6.253	1514	1528	1551	rBV	178574	337727	60.21%	7.741%
32	6.452	1587	1590	1592	rBV	137	116	0.02%	0.003%
33	6.600	1632	1636	1639	rBB	173	167	0.03%	0.004%
34	6.694	1652	1665	1685	rBV	129399	250662	44.69%	5.745%
35	6.771	1685	1689	1693	rVB2	281	320	0.06%	0.007%
36	6.999	1758	1760	1764	rVB	150	121	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046427.D
 Acq On : 16 Dec 2021 17:32
 Operator : SY/MD
 Sample : M5037-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C00Y0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	7.041	1769	1773	1775	rBB	149	124	0.02%	0.003%
38	7.186	1815	1818	1823	rVB2	350	303	0.05%	0.007%
39	7.311	1854	1857	1860	rBV	131	132	0.02%	0.003%
40	7.385	1878	1880	1883	rBV	148	125	0.02%	0.003%
41	7.568	1925	1937	1953	rBV	68461	118240	21.08%	2.710%
42	7.687	1971	1974	1977	rVB2	364	290	0.05%	0.007%
43	7.732	1985	1988	1990	rBV	128	115	0.02%	0.003%
44	7.899	2025	2040	2056	rBV	250830	432005	77.02%	9.902%
45	8.044	2083	2085	2088	rVB	186	122	0.02%	0.003%
46	8.073	2089	2094	2096	rBV	149	145	0.03%	0.003%
47	8.182	2117	2128	2142	rBV	46566	79328	14.14%	1.818%
48	8.263	2151	2153	2157	rVB	233	182	0.03%	0.004%
49	8.475	2209	2219	2228	rBV2	3558	6239	1.11%	0.143%
50	8.584	2250	2253	2257	rVB3	342	258	0.05%	0.006%
51	8.636	2257	2269	2293	rVV	159572	266861	47.57%	6.116%
52	8.732	2297	2299	2307	rVB2	301	239	0.04%	0.005%
53	9.176	2430	2437	2440	rVB	178	276	0.05%	0.006%
54	9.198	2441	2444	2447	rBV	126	110	0.02%	0.003%
55	9.227	2450	2453	2456	rVV	173	163	0.03%	0.004%
56	9.243	2456	2458	2464	rVB	176	190	0.03%	0.004%
57	9.301	2472	2476	2478	rBV	165	169	0.03%	0.004%
58	9.365	2492	2496	2499	rBV	161	148	0.03%	0.003%
59	9.420	2499	2513	2532	rVV	274756	456415	81.37%	10.461%
60	9.562	2556	2557	2560	rVB	245	115	0.02%	0.003%
61	9.603	2566	2570	2572	rBV	172	166	0.03%	0.004%
62	9.687	2594	2596	2598	rBV	213	149	0.03%	0.003%
63	9.822	2635	2638	2641	rBB	151	129	0.02%	0.003%
64	9.854	2644	2648	2652	rBB	159	185	0.03%	0.004%
65	9.883	2652	2657	2659	rBV	154	180	0.03%	0.004%
66	9.935	2668	2673	2676	rBB	163	175	0.03%	0.004%
67	9.964	2679	2682	2685	rBV	151	151	0.03%	0.003%
68	10.044	2703	2707	2710	rBV	158	154	0.03%	0.004%
69	10.192	2746	2753	2756	rBB	205	233	0.04%	0.005%
70	10.230	2761	2765	2766	rBV	169	145	0.03%	0.003%
71	10.256	2770	2773	2779	rVV	99	112	0.02%	0.003%
72	10.407	2817	2820	2824	rBV	187	214	0.04%	0.005%
73	10.494	2843	2847	2848	rBV	211	166	0.03%	0.004%
74	10.581	2869	2874	2876	rBV	286	267	0.05%	0.006%
75	10.674	2896	2903	2908	rVB2	1152	1325	0.24%	0.030%
76	10.758	2917	2929	2944	rVV	178319	285865	50.96%	6.552%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046427.D
 Acq On : 16 Dec 2021 17:32
 Operator : SY/MD
 Sample : M5037-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C00Y0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	10.812	2944	2946	2949	rVB	194	125	0.02%	0.003%
78	10.896	2962	2972	2984	rVB3	4420	6898	1.23%	0.158%
79	11.189	3055	3063	3068	rBV	200	399	0.07%	0.009%
80	11.455	3139	3146	3157	rBV4	723	1415	0.25%	0.032%
81	11.571	3181	3182	3188	rVB	133	136	0.02%	0.003%
82	11.697	3217	3221	3226	rVB2	238	274	0.05%	0.006%
83	11.742	3232	3235	3238	rBV	168	157	0.03%	0.004%
84	11.812	3245	3257	3280	rVB	273354	434568	77.47%	9.960%
85	11.973	3302	3307	3313	rVB2	606	724	0.13%	0.017%
86	12.070	3329	3337	3346	rVB3	815	1237	0.22%	0.028%
87	12.195	3364	3376	3394	rVV	248431	394926	70.40%	9.052%
88	12.777	3548	3557	3564	rBV3	1269	2020	0.36%	0.046%
89	12.973	3613	3618	3624	rBV4	746	942	0.17%	0.022%
90	13.073	3644	3649	3651	rBV	127	119	0.02%	0.003%
91	14.176	3989	3992	3997	rBV	129	112	0.02%	0.003%
92	14.526	4098	4101	4106	rBV	128	150	0.03%	0.003%
93	15.478	4394	4397	4402	rVB	204	152	0.03%	0.003%
94	15.613	4434	4439	4441	rBV2	229	194	0.03%	0.004%
95	15.690	4460	4463	4466	rVB2	218	134	0.02%	0.003%
96	15.713	4466	4470	4474	rBV2	231	304	0.05%	0.007%
97	15.777	4486	4490	4493	rBV2	184	169	0.03%	0.004%
98	16.095	4585	4589	4590	rBV	283	200	0.04%	0.005%
99	17.269	4951	4954	4957	rBV2	392	282	0.05%	0.006%
100	17.510	5027	5029	5033	rBV3	525	472	0.08%	0.011%




Sum of corrected areas: 4362987

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046427.D
Acq On : 16 Dec 2021 17:32
Operator : SY/MD
Sample : M5037-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C00Y0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

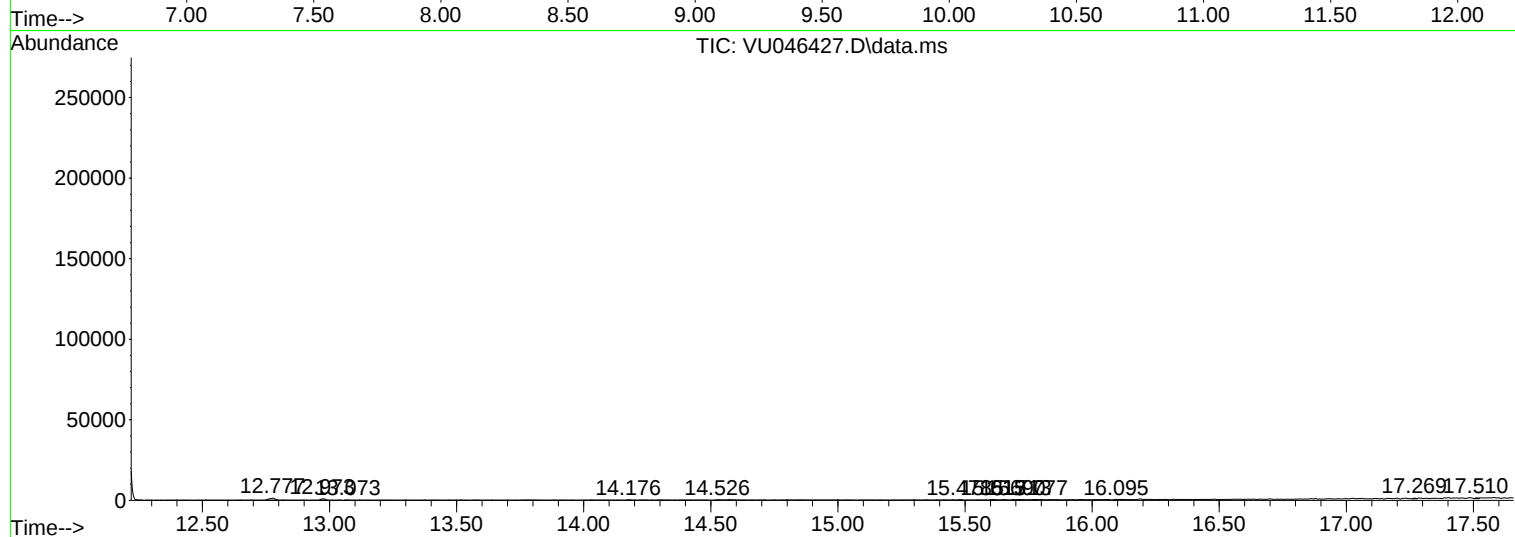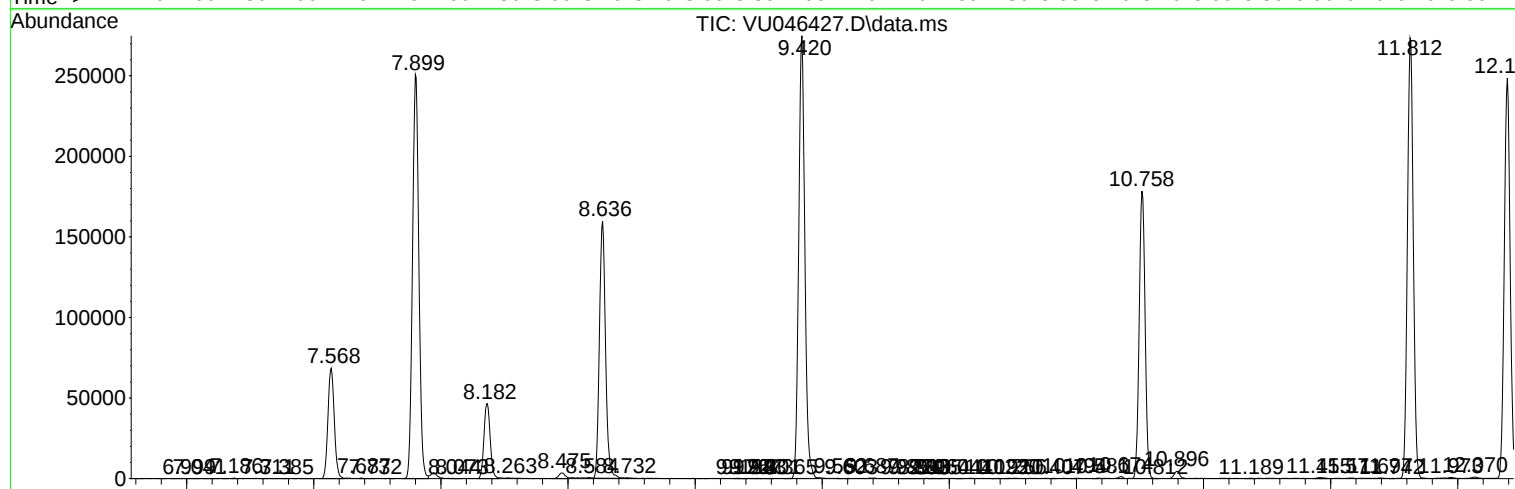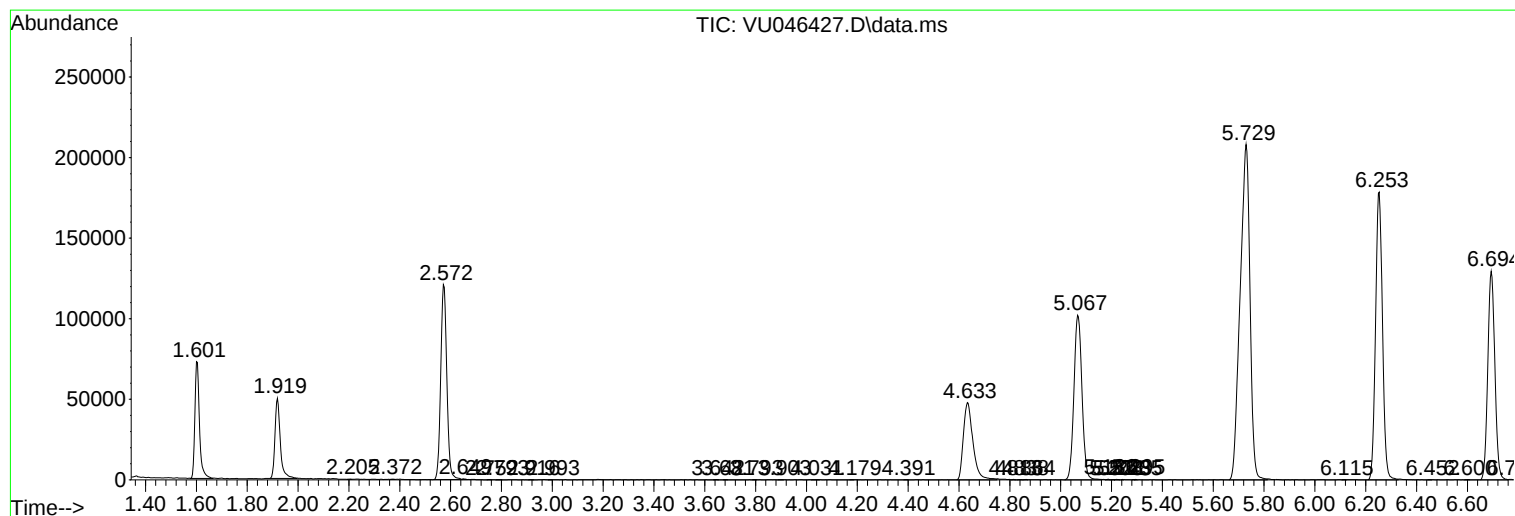

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046427.D
Acq On : 16 Dec 2021 17:32
Operator : SY/MD
Sample : M5037-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C00Y0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046427.D
Acq On : 16 Dec 2021 17:32
Operator : SY/MD
Sample : M5037-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C00Y0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------