

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046428.D
 Acq On : 16 Dec 2021 17:55
 Operator : SY/MD
 Sample : M5037-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C00Y2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046428.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	101	rBV	70463	87901	15.67%	1.996%
2	1.919	171	180	204	rBV	49893	71694	12.78%	1.628%
3	2.279	289	292	296	rVB2	175	113	0.02%	0.003%
4	2.308	296	301	304	rBV2	208	180	0.03%	0.004%
5	2.372	319	321	323	rBV2	233	127	0.02%	0.003%
6	2.520	364	367	372	rVB2	186	219	0.04%	0.005%
7	2.572	372	383	396	rBV	118266	197298	35.18%	4.480%
8	2.646	397	406	430	rVB	10374	24108	4.30%	0.547%
9	2.800	451	454	457	rBV	165	155	0.03%	0.004%
10	2.958	499	503	505	rVV2	226	197	0.04%	0.004%
11	3.186	569	574	576	rBV2	204	215	0.04%	0.005%
12	3.215	579	583	585	rVB	175	142	0.03%	0.003%
13	3.356	625	627	631	rBB	136	115	0.02%	0.003%
14	3.482	663	666	669	rBV	135	141	0.03%	0.003%
15	3.604	702	704	708	rBV	133	140	0.02%	0.003%
16	3.700	730	734	736	rBV	138	149	0.03%	0.003%
17	4.630	1010	1023	1044	rBV	47324	121601	21.68%	2.761%
18	4.797	1073	1075	1077	rBV2	254	158	0.03%	0.004%
19	4.810	1077	1079	1082	rVV	161	129	0.02%	0.003%
20	4.903	1104	1108	1109	rBV	117	105	0.02%	0.002%
21	4.961	1123	1126	1128	rBB	166	108	0.02%	0.002%
22	5.067	1143	1159	1178	rBV	102926	223606	39.87%	5.078%
23	5.212	1201	1204	1207	rBV	227	174	0.03%	0.004%
24	5.263	1217	1220	1223	rBB	156	104	0.02%	0.002%
25	5.286	1224	1227	1228	rBV	224	114	0.02%	0.003%
26	5.302	1230	1232	1235	rVB	153	104	0.02%	0.002%
27	5.369	1249	1253	1256	rBB	268	177	0.03%	0.004%
28	5.729	1344	1365	1387	rBV2	207739	560781	100.00%	12.735%
29	6.109	1480	1483	1485	rBV	137	122	0.02%	0.003%
30	6.253	1511	1528	1561	rBB	176639	333842	59.53%	7.581%
31	6.539	1615	1617	1620	rBV	148	120	0.02%	0.003%
32	6.694	1652	1665	1687	rBV	127694	249330	44.46%	5.662%
33	6.774	1687	1690	1693	rVB	167	107	0.02%	0.002%
34	6.813	1698	1702	1704	rBV	227	164	0.03%	0.004%
35	7.044	1772	1774	1777	rBV2	231	155	0.03%	0.004%
36	7.186	1812	1818	1823	rBB2	381	366	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046428.D
 Acq On : 16 Dec 2021 17:55
 Operator : SY/MD
 Sample : M5037-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C00Y2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	7.568	1925	1937	1955	rBV2	66891	117363	20.93%	2.665%
38	7.768	1996	1999	2002	rBB	143	122	0.02%	0.003%
39	7.900	2027	2040	2054	rBV	252423	429963	76.67%	9.764%
40	7.970	2056	2062	2074	rVB	7770	12686	2.26%	0.288%
41	8.070	2090	2093	2096	rBB	153	125	0.02%	0.003%
42	8.121	2107	2109	2112	rBV	154	129	0.02%	0.003%
43	8.183	2117	2128	2144	rBV	48389	80092	14.28%	1.819%
44	8.289	2157	2161	2162	rBV	167	118	0.02%	0.003%
45	8.417	2198	2201	2204	rBV	143	121	0.02%	0.003%
46	8.475	2208	2219	2232	rBV2	4982	9113	1.63%	0.207%
47	8.523	2232	2234	2237	rVB2	262	155	0.03%	0.004%
48	8.578	2247	2251	2257	rVB2	411	398	0.07%	0.009%
49	8.633	2257	2268	2298	rBV	157255	264283	47.13%	6.002%
50	8.784	2311	2315	2317	rBV3	702	560	0.10%	0.013%
51	8.925	2356	2359	2361	rBV	154	129	0.02%	0.003%
52	8.993	2378	2380	2386	rVB	160	183	0.03%	0.004%
53	9.083	2405	2408	2414	rBV	175	239	0.04%	0.005%
54	9.137	2422	2425	2428	rBV	142	143	0.03%	0.003%
55	9.186	2438	2440	2443	rBV	121	107	0.02%	0.002%
56	9.417	2500	2512	2532	rBV	263482	450069	80.26%	10.221%
57	9.575	2556	2561	2567	rVB2	399	491	0.09%	0.011%
58	9.652	2582	2585	2587	rBV	162	137	0.02%	0.003%
59	9.694	2590	2598	2607	rVB3	1270	2031	0.36%	0.046%
60	9.925	2667	2670	2671	rBV	162	110	0.02%	0.002%
61	10.025	2698	2701	2704	rBB	165	128	0.02%	0.003%
62	10.044	2704	2707	2709	rBV	161	129	0.02%	0.003%
63	10.105	2717	2726	2733	rBB2	701	956	0.17%	0.022%
64	10.182	2748	2750	2753	rBV	132	119	0.02%	0.003%
65	10.456	2833	2835	2838	rBV	145	124	0.02%	0.003%
66	10.526	2850	2857	2860	rBV	218	290	0.05%	0.007%
67	10.571	2865	2871	2880	rVB4	1190	1699	0.30%	0.039%
68	10.674	2897	2903	2909	rVB4	1184	1463	0.26%	0.033%
69	10.707	2910	2913	2915	rBV	150	122	0.02%	0.003%
70	10.758	2917	2929	2945	rVV	178610	284846	50.79%	6.469%
71	10.893	2962	2971	2982	rVB	6116	10065	1.79%	0.229%
72	10.999	3001	3004	3011	rVB2	174	187	0.03%	0.004%
73	11.356	3112	3115	3117	rBV	191	163	0.03%	0.004%
74	11.385	3122	3124	3127	rVB	209	140	0.02%	0.003%
75	11.465	3141	3149	3159	rVB5	948	1734	0.31%	0.039%
76	11.697	3215	3221	3226	rVB3	349	492	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046428.D
 Acq On : 16 Dec 2021 17:55
 Operator : SY/MD
 Sample : M5037-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C00Y2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.813	3245	3257	3276	rBV	273830	431005	76.86%	9.788%
78	11.903	3282	3285	3288	rBV	187	194	0.03%	0.004%
79	11.941	3294	3297	3302	rBV2	355	375	0.07%	0.009%
80	11.977	3305	3308	3319	rVB2	804	736	0.13%	0.017%
81	12.060	3325	3334	3344	rBV3	5911	9322	1.66%	0.212%
82	12.195	3363	3376	3394	rVB	249955	400954	71.50%	9.105%
83	12.530	3472	3480	3488	rBV2	5344	6792	1.21%	0.154%
84	12.774	3548	3556	3566	rVB2	2025	3076	0.55%	0.070%
85	12.841	3575	3577	3580	rVB2	434	240	0.04%	0.005%
86	12.890	3587	3592	3594	rBV	834	717	0.13%	0.016%
87	12.973	3613	3618	3624	rBV4	975	1050	0.19%	0.024%
88	13.096	3653	3656	3660	rVB	150	112	0.02%	0.003%
89	13.459	3764	3769	3773	rBV	102	104	0.02%	0.002%
90	13.655	3826	3830	3835	rVB	156	143	0.03%	0.003%
91	13.922	3908	3913	3920	rVB2	501	593	0.11%	0.013%
92	14.099	3963	3968	3974	rVB2	276	302	0.05%	0.007%
93	14.575	4112	4116	4117	rBV	374	240	0.04%	0.005%
94	14.983	4241	4243	4251	rVB3	431	340	0.06%	0.008%
95	15.504	4402	4405	4408	rVB	201	116	0.02%	0.003%
96	15.526	4408	4412	4415	rBV	237	221	0.04%	0.005%
97	15.777	4487	4490	4493	rBV	234	191	0.03%	0.004%
98	16.291	4647	4650	4654	rBV	286	220	0.04%	0.005%
99	16.687	4769	4773	4775	rBV2	359	270	0.05%	0.006%
100	16.835	4813	4819	4821	rBV2	338	415	0.07%	0.009%




Sum of corrected areas: 4403513

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046428.D
Acq On : 16 Dec 2021 17:55
Operator : SY/MD
Sample : M5037-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C00Y2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

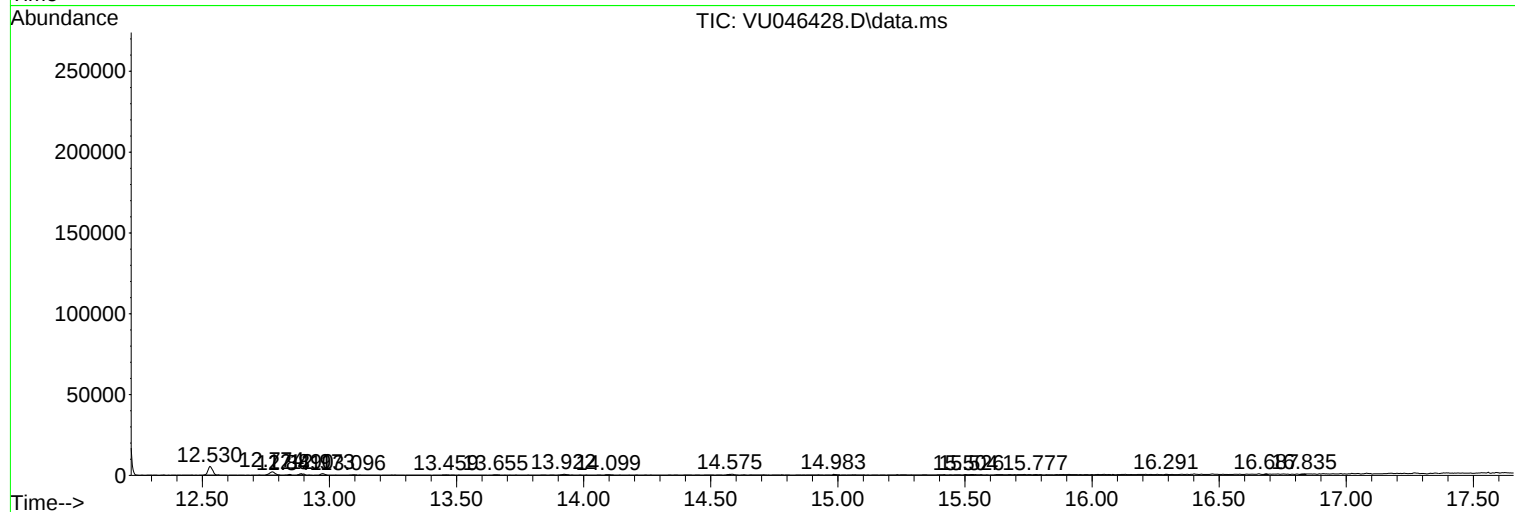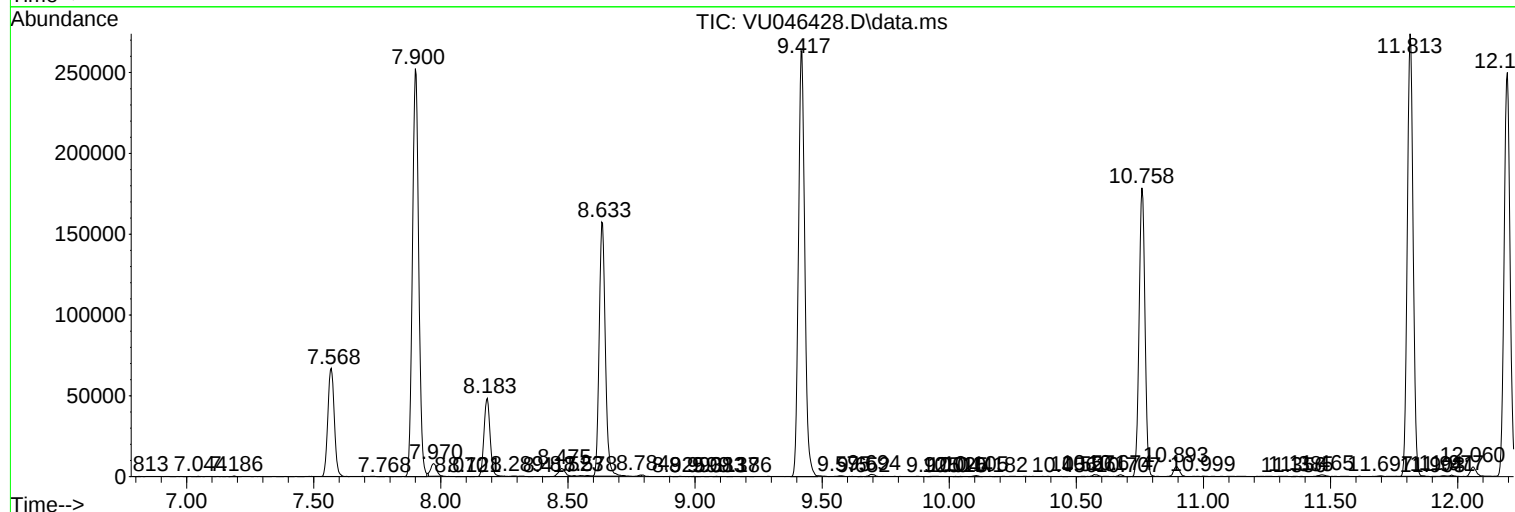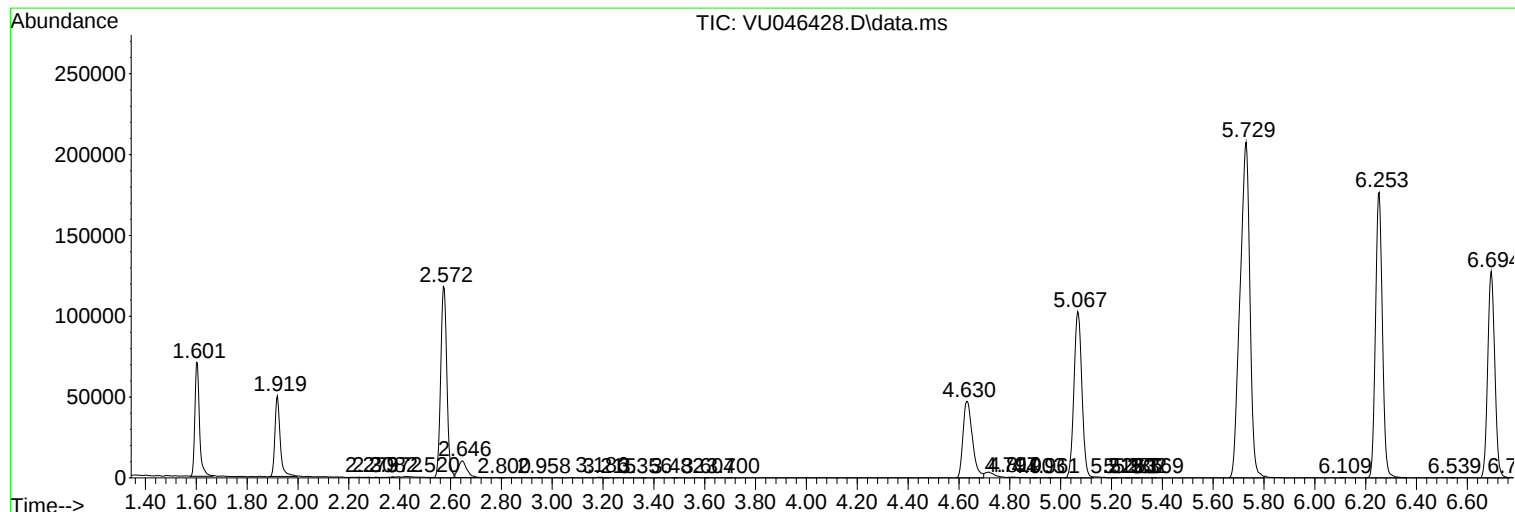

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046428.D
Acq On : 16 Dec 2021 17:55
Operator : SY/MD
Sample : M5037-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C00Y2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046428.D
Acq On : 16 Dec 2021 17:55
Operator : SY/MD
Sample : M5037-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C00Y2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc