

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046429.D
 Acq On : 16 Dec 2021 18:17
 Operator : SY/MD
 Sample : M5037-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C00Y4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046429.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	73	82	102	rBV	71638	87153	15.95%	2.063%
2	1.919	171	180	202	rBV	48961	70590	12.92%	1.671%
3	2.041	215	218	220	rBV	341	188	0.03%	0.004%
4	2.108	236	239	242	rBV	312	234	0.04%	0.006%
5	2.231	275	277	279	rBV	189	125	0.02%	0.003%
6	2.385	323	325	328	rVB	224	111	0.02%	0.003%
7	2.575	370	384	405	rBV	116202	193784	35.47%	4.586%
8	2.842	465	467	470	rBV	119	109	0.02%	0.003%
9	2.877	475	478	482	rBB	169	163	0.03%	0.004%
10	2.903	483	486	490	rBB	131	134	0.02%	0.003%
11	2.993	509	514	518	rBB	186	222	0.04%	0.005%
12	3.083	540	542	545	rVB	158	106	0.02%	0.003%
13	3.121	549	554	559	rBV	157	245	0.04%	0.006%
14	3.179	569	572	575	rBV	327	299	0.05%	0.007%
15	3.205	578	580	583	rVB	299	184	0.03%	0.004%
16	3.234	586	589	592	rBB	145	128	0.02%	0.003%
17	3.366	627	630	632	rBV	131	117	0.02%	0.003%
18	3.504	666	673	675	rBV	147	209	0.04%	0.005%
19	3.610	703	706	713	rBB	162	225	0.04%	0.005%
20	3.645	714	717	720	rBB	128	112	0.02%	0.003%
21	3.739	744	746	749	rBV	121	110	0.02%	0.003%
22	4.304	920	922	926	rBB	136	119	0.02%	0.003%
23	4.632	1011	1024	1048	rVV2	46061	118328	21.66%	2.800%
24	4.787	1069	1072	1076	rVV2	192	158	0.03%	0.004%
25	4.829	1083	1085	1088	rVB	255	142	0.03%	0.003%
26	4.931	1115	1117	1122	rBV	113	144	0.03%	0.003%
27	5.067	1144	1159	1180	rBV	100735	219293	40.14%	5.190%
28	5.173	1189	1192	1194	rBV2	196	138	0.03%	0.003%
29	5.234	1209	1211	1215	rBB	239	141	0.03%	0.003%
30	5.269	1219	1222	1226	rBV	145	168	0.03%	0.004%
31	5.343	1242	1245	1248	rBV	136	141	0.03%	0.003%
32	5.729	1343	1365	1399	rBV2	202644	546372	100.00%	12.931%
33	5.989	1444	1446	1450	rBV	139	147	0.03%	0.003%
34	6.253	1514	1528	1546	rBV	172163	325724	59.62%	7.709%
35	6.382	1567	1568	1573	rVB	240	136	0.02%	0.003%
36	6.591	1631	1633	1636	rBB	164	111	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046429.D
 Acq On : 16 Dec 2021 18:17
 Operator : SY/MD
 Sample : M5037-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C00Y4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	6.693	1652	1665	1689	rBB	125927	243634	44.59%	5.766%
38	6.835	1705	1709	1710	rBV	447	293	0.05%	0.007%
39	7.018	1764	1766	1770	rBB	126	112	0.02%	0.003%
40	7.050	1773	1776	1778	rBV	148	125	0.02%	0.003%
41	7.185	1815	1818	1821	rVV	158	115	0.02%	0.003%
42	7.568	1926	1937	1950	rBV	65541	114017	20.87%	2.698%
43	7.690	1972	1975	1979	rBV2	277	241	0.04%	0.006%
44	7.809	2007	2012	2014	rBV	162	158	0.03%	0.004%
45	7.899	2027	2040	2056	rBV	244493	420033	76.88%	9.941%
46	7.970	2058	2062	2072	rVB	3354	4460	0.82%	0.106%
47	8.131	2109	2112	2114	rBV	144	125	0.02%	0.003%
48	8.182	2117	2128	2140	rBV	46294	77330	14.15%	1.830%
49	8.343	2176	2178	2181	rBV	189	140	0.03%	0.003%
50	8.472	2209	2218	2230	rVV2	3230	5824	1.07%	0.138%
51	8.517	2230	2232	2236	rVB2	284	164	0.03%	0.004%
52	8.636	2257	2269	2290	rBV	153652	256561	46.96%	6.072%
53	8.774	2308	2312	2317	rVB	202	232	0.04%	0.005%
54	8.951	2363	2367	2370	rBB	136	133	0.02%	0.003%
55	8.980	2371	2376	2380	rBV	173	234	0.04%	0.006%
56	9.166	2431	2434	2438	rBV	156	175	0.03%	0.004%
57	9.243	2456	2458	2461	rBV	158	134	0.02%	0.003%
58	9.420	2499	2513	2533	rBV	261828	436729	79.93%	10.336%
59	9.697	2594	2599	2603	rVB3	437	496	0.09%	0.012%
60	9.828	2636	2640	2644	rBV	182	215	0.04%	0.005%
61	9.915	2663	2667	2673	rBV	196	258	0.05%	0.006%
62	9.983	2682	2688	2691	rBV	192	268	0.05%	0.006%
63	10.041	2703	2706	2708	rBV	131	114	0.02%	0.003%
64	10.198	2752	2755	2760	rBB	183	196	0.04%	0.005%
65	10.234	2761	2766	2770	rBV	178	250	0.05%	0.006%
66	10.507	2848	2851	2855	rVB	182	176	0.03%	0.004%
67	10.539	2856	2861	2863	rBV	144	172	0.03%	0.004%
68	10.674	2896	2903	2908	rBV3	1302	1526	0.28%	0.036%
69	10.703	2908	2912	2915	rVB	146	157	0.03%	0.004%
70	10.758	2915	2929	2950	rBV	173505	279835	51.22%	6.623%
71	10.893	2961	2971	2983	rVB	3588	5827	1.07%	0.138%
72	11.182	3058	3061	3063	rBV	191	151	0.03%	0.004%
73	11.240	3075	3079	3080	rBV	177	144	0.03%	0.003%
74	11.378	3115	3122	3125	rBV	170	264	0.05%	0.006%
75	11.455	3141	3146	3147	rBV	644	465	0.09%	0.011%
76	11.690	3217	3219	3223	rBV2	151	120	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046429.D
 Acq On : 16 Dec 2021 18:17
 Operator : SY/MD
 Sample : M5037-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C00Y4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.812	3245	3257	3274	rBV	269590	414917	75.94%	9.820%
78	11.941	3294	3297	3302	rVV	212	265	0.05%	0.006%
79	11.976	3304	3308	3314	rVB2	596	642	0.12%	0.015%
80	12.063	3328	3335	3344	rBV3	1196	1539	0.28%	0.036%
81	12.195	3363	3376	3393	rVB	239807	384693	70.41%	9.105%
82	12.774	3548	3556	3563	rVB2	1009	1544	0.28%	0.037%
83	12.973	3612	3618	3625	rVB4	851	961	0.18%	0.023%
84	14.786	4179	4182	4186	rBV	149	122	0.02%	0.003%
85	15.275	4331	4334	4337	rBV2	183	114	0.02%	0.003%
86	15.474	4393	4396	4399	rBV2	230	201	0.04%	0.005%
87	15.497	4399	4403	4409	rVV2	228	291	0.05%	0.007%
88	15.545	4415	4418	4422	rBV	202	135	0.02%	0.003%
89	15.581	4426	4429	4433	rBV2	233	144	0.03%	0.003%
90	15.610	4434	4438	4441	rBV2	180	150	0.03%	0.004%
91	15.635	4441	4446	4450	rVB	212	228	0.04%	0.005%
92	15.677	4457	4459	4462	rBV2	171	118	0.02%	0.003%
93	15.754	4481	4483	4489	rVB2	192	160	0.03%	0.004%
94	15.902	4525	4529	4531	rBV	235	210	0.04%	0.005%
95	15.973	4548	4551	4555	rVB	324	242	0.04%	0.006%
96	16.066	4577	4580	4582	rBV	213	145	0.03%	0.003%
97	16.529	4721	4724	4730	rVB2	325	226	0.04%	0.005%
98	16.603	4745	4747	4751	rVB3	303	158	0.03%	0.004%
99	16.664	4763	4766	4774	rBV3	389	437	0.08%	0.010%
100	16.986	4864	4866	4869	rBV2	431	206	0.04%	0.005%




Sum of corrected areas: 4225261

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046429.D
Acq On : 16 Dec 2021 18:17
Operator : SY/MD
Sample : M5037-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C00Y4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

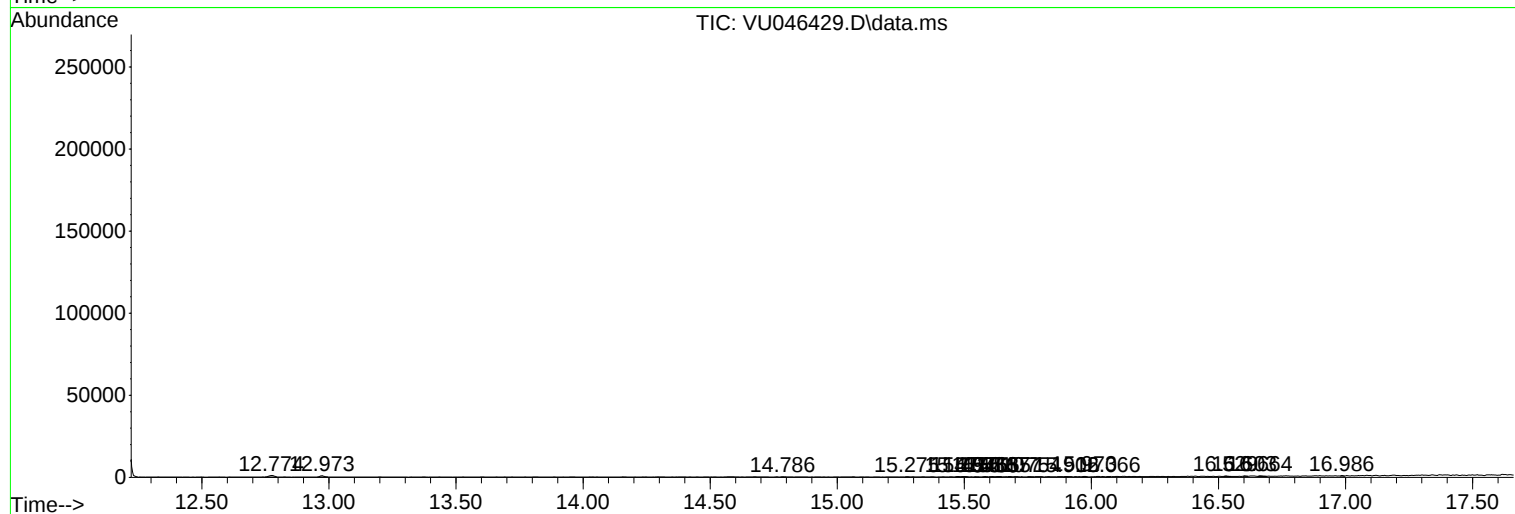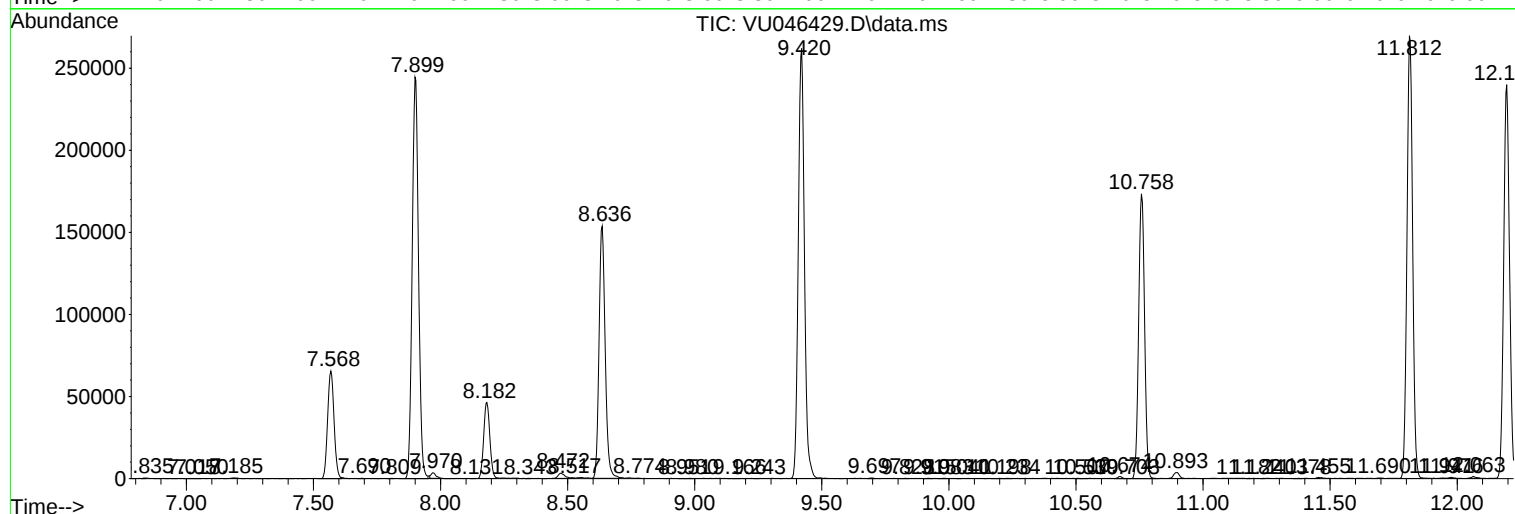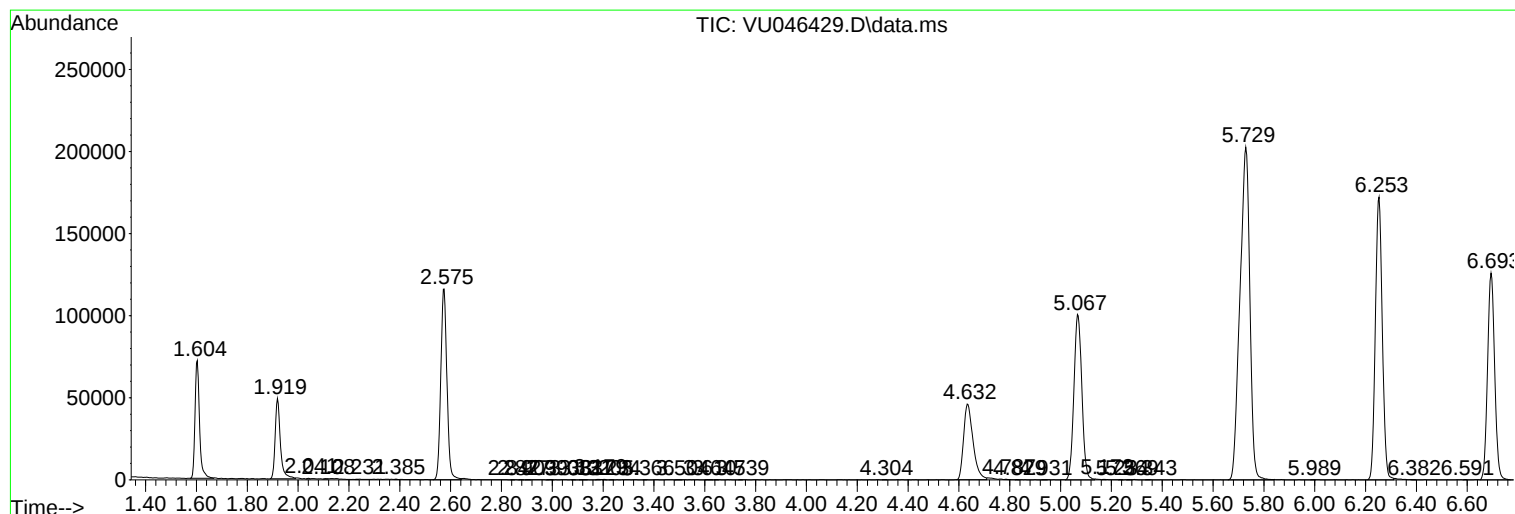

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046429.D
Acq On : 16 Dec 2021 18:17
Operator : SY/MD
Sample : M5037-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C00Y4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046429.D
Acq On : 16 Dec 2021 18:17
Operator : SY/MD
Sample : M5037-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C00Y4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc