

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046432.D
 Acq On : 16 Dec 2021 19:25
 Operator : SY/MD
 Sample : M5037-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C00Z0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046432.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	100	rBV	67991	82795	15.46%	1.927%
2	1.919	171	180	206	rBV	48086	70186	13.10%	1.634%
3	2.134	244	247	249	rBV	214	124	0.02%	0.003%
4	2.575	371	384	401	rBV2	119074	206935	38.64%	4.817%
5	2.809	454	457	460	rBV	184	174	0.03%	0.004%
6	3.189	571	575	579	rBV2	454	432	0.08%	0.010%
7	3.256	592	596	600	rBB	135	141	0.03%	0.003%
8	3.510	670	675	679	rBB	157	187	0.03%	0.004%
9	3.536	680	683	686	rBV	139	140	0.03%	0.003%
10	3.877	774	789	805	rBV2	24106	54863	10.24%	1.277%
11	3.931	805	806	808	rVV2	266	106	0.02%	0.002%
12	4.411	953	955	959	rBB	121	109	0.02%	0.003%
13	4.636	1011	1025	1066	rBV	44189	121893	22.76%	2.838%
14	4.816	1079	1081	1084	rBV	128	122	0.02%	0.003%
15	4.857	1090	1094	1096	rBV	186	128	0.02%	0.003%
16	5.066	1144	1159	1182	rBV2	98454	215687	40.27%	5.021%
17	5.214	1202	1205	1207	rBB2	240	132	0.02%	0.003%
18	5.321	1224	1238	1254	rBB2	31408	68710	12.83%	1.600%
19	5.401	1261	1263	1267	rBV	141	137	0.03%	0.003%
20	5.652	1337	1341	1344	rBV	154	153	0.03%	0.004%
21	5.729	1344	1365	1385	rBV2	196626	535594	100.00%	12.468%
22	5.960	1434	1437	1439	rBV	123	108	0.02%	0.003%
23	6.099	1476	1480	1482	rBV	141	150	0.03%	0.003%
24	6.253	1514	1528	1553	rBV	167600	317096	59.20%	7.382%
25	6.385	1567	1569	1573	rBB	121	108	0.02%	0.003%
26	6.513	1606	1609	1613	rBB	127	132	0.02%	0.003%
27	6.642	1646	1649	1651	rBV	147	122	0.02%	0.003%
28	6.693	1651	1665	1687	rVV	126149	240992	45.00%	5.610%
29	6.812	1700	1702	1705	rBV	233	151	0.03%	0.004%
30	7.140	1800	1804	1808	rBB	141	163	0.03%	0.004%
31	7.189	1812	1819	1822	rBB2	330	402	0.08%	0.009%
32	7.230	1829	1832	1835	rBV	126	133	0.02%	0.003%
33	7.452	1897	1901	1905	rBB	145	144	0.03%	0.003%
34	7.484	1906	1911	1915	rBB	157	188	0.04%	0.004%
35	7.568	1924	1937	1958	rVV	64599	111296	20.78%	2.591%
36	7.899	2027	2040	2057	rBV	242609	415878	77.65%	9.681%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046432.D
 Acq On : 16 Dec 2021 19:25
 Operator : SY/MD
 Sample : M5037-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C00Z0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	7.973	2058	2063	2071	rVB2	2818	4330	0.81%	0.101%
38	8.182	2116	2128	2141	rBV2	45573	75931	14.18%	1.768%
39	8.243	2146	2147	2151	rVB	267	134	0.03%	0.003%
40	8.291	2160	2162	2168	rBV2	150	185	0.03%	0.004%
41	8.475	2209	2219	2228	rBV3	3464	6897	1.29%	0.161%
42	8.635	2257	2269	2288	rBV	154412	257879	48.15%	6.003%
43	8.909	2352	2354	2359	rVB	176	180	0.03%	0.004%
44	8.941	2362	2364	2369	rBV	162	187	0.03%	0.004%
45	9.044	2393	2396	2399	rBB	130	113	0.02%	0.003%
46	9.095	2410	2412	2415	rVB	161	110	0.02%	0.003%
47	9.211	2446	2448	2451	rBV	141	126	0.02%	0.003%
48	9.317	2479	2481	2484	rBV	150	123	0.02%	0.003%
49	9.346	2487	2490	2493	rBV	156	149	0.03%	0.003%
50	9.420	2500	2513	2533	rBV	254543	424794	79.31%	9.889%
51	9.668	2586	2590	2594	rBV	148	202	0.04%	0.005%
52	9.690	2594	2597	2606	rVB2	345	458	0.09%	0.011%
53	9.729	2607	2609	2612	rBV	138	114	0.02%	0.003%
54	9.787	2624	2627	2629	rBV	150	120	0.02%	0.003%
55	10.076	2714	2717	2719	rBV	127	113	0.02%	0.003%
56	10.089	2719	2721	2728	rVB	182	200	0.04%	0.005%
57	10.153	2738	2741	2744	rBB	159	133	0.02%	0.003%
58	10.179	2745	2749	2752	rBV	173	157	0.03%	0.004%
59	10.243	2766	2769	2771	rBV	116	104	0.02%	0.002%
60	10.346	2797	2801	2803	rBV	130	113	0.02%	0.003%
61	10.459	2831	2836	2839	rBV	203	252	0.05%	0.006%
62	10.494	2843	2847	2852	rBB	133	186	0.03%	0.004%
63	10.520	2852	2855	2857	rBV	149	125	0.02%	0.003%
64	10.632	2887	2890	2894	rBV	175	184	0.03%	0.004%
65	10.661	2895	2899	2900	rVV	253	179	0.03%	0.004%
66	10.674	2900	2903	2909	rVB	597	643	0.12%	0.015%
67	10.758	2917	2929	2947	rBV	173803	278675	52.03%	6.487%
68	10.893	2961	2971	2982	rBV2	4299	6676	1.25%	0.155%
69	10.947	2984	2988	2991	rBV	242	252	0.05%	0.006%
70	11.047	3013	3019	3026	rBV	225	418	0.08%	0.010%
71	11.098	3032	3035	3037	rBV	170	145	0.03%	0.003%
72	11.156	3050	3053	3057	rVB	186	178	0.03%	0.004%
73	11.179	3057	3060	3063	rBV	147	149	0.03%	0.003%
74	11.459	3141	3147	3148	rBV2	487	416	0.08%	0.010%
75	11.696	3216	3221	3223	rBV2	285	225	0.04%	0.005%
76	11.812	3246	3257	3273	rBV	257772	400521	74.78%	9.324%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046432.D
 Acq On : 16 Dec 2021 19:25
 Operator : SY/MD
 Sample : M5037-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C00Z0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.973	3302	3307	3312	rVB2	503	562	0.10%	0.013%
78	12.066	3330	3336	3342	rVV2	822	815	0.15%	0.019%
79	12.195	3363	3376	3390	rBV	238786	380274	71.00%	8.853%
80	12.777	3547	3557	3564	rBV2	1418	2184	0.41%	0.051%
81	12.838	3573	3576	3580	rBV	148	104	0.02%	0.002%
82	12.973	3613	3618	3622	rBV3	687	656	0.12%	0.015%
83	13.076	3646	3650	3657	rBV	99	127	0.02%	0.003%
84	13.696	3839	3843	3847	rBV	141	129	0.02%	0.003%
85	14.066	3953	3958	3965	rBV	136	208	0.04%	0.005%
86	14.571	4111	4115	4118	rBV	320	319	0.06%	0.007%
87	14.648	4136	4139	4144	rBV	121	142	0.03%	0.003%
88	14.847	4199	4201	4205	rVB	250	118	0.02%	0.003%
89	15.256	4326	4328	4332	rVB	199	117	0.02%	0.003%
90	15.400	4370	4373	4378	rVB	220	157	0.03%	0.004%
91	15.561	4420	4423	4426	rBV2	188	148	0.03%	0.003%
92	15.603	4433	4436	4444	rVB2	230	232	0.04%	0.005%
93	15.638	4444	4447	4450	rBV2	211	186	0.03%	0.004%
94	15.757	4482	4484	4486	rBV	194	125	0.02%	0.003%
95	15.799	4492	4497	4501	rVB	250	287	0.05%	0.007%
96	15.831	4504	4507	4511	rBV	192	211	0.04%	0.005%
97	15.892	4523	4526	4528	rBB	161	109	0.02%	0.003%
98	15.921	4533	4535	4538	rBV2	199	163	0.03%	0.004%
99	16.500	4713	4715	4723	rVB3	356	261	0.05%	0.006%
100	16.539	4724	4727	4729	rBV2	235	138	0.03%	0.003%




Sum of corrected areas: 4295659

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046432.D
Acq On : 16 Dec 2021 19:25
Operator : SY/MD
Sample : M5037-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C00Z0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

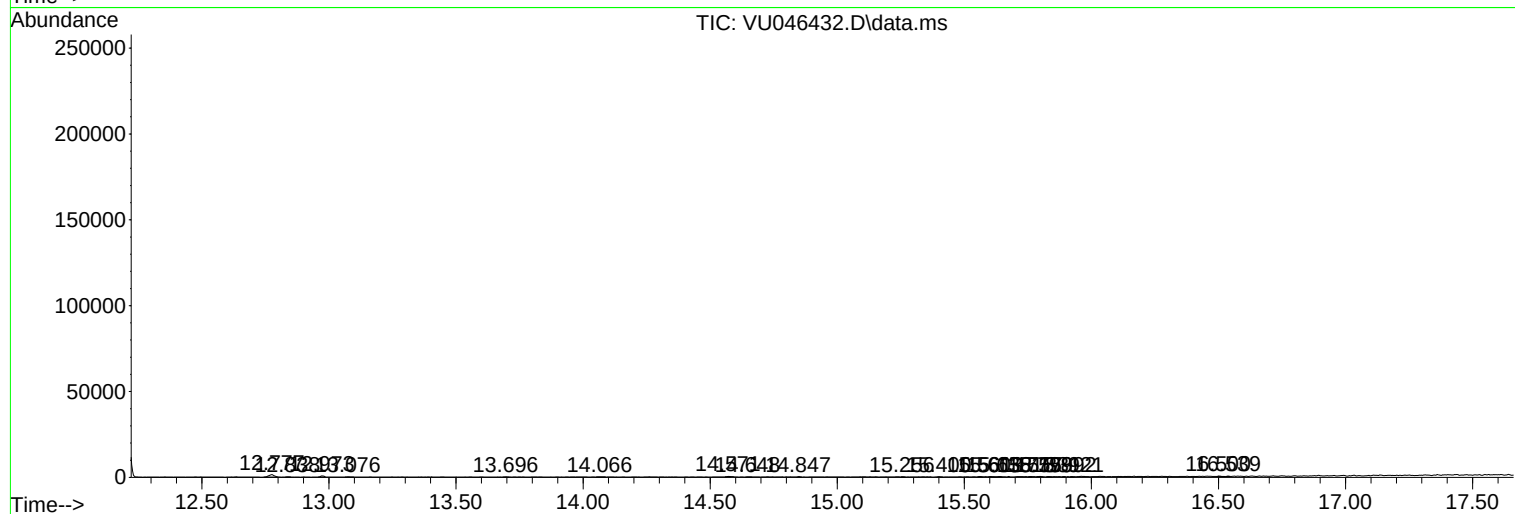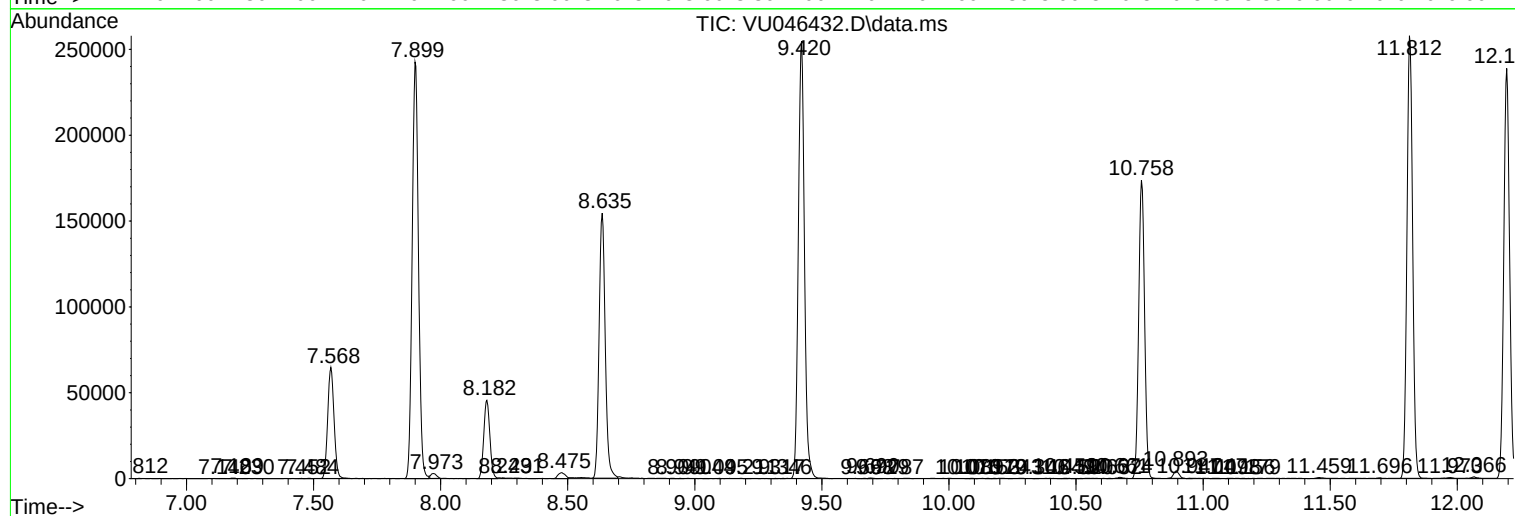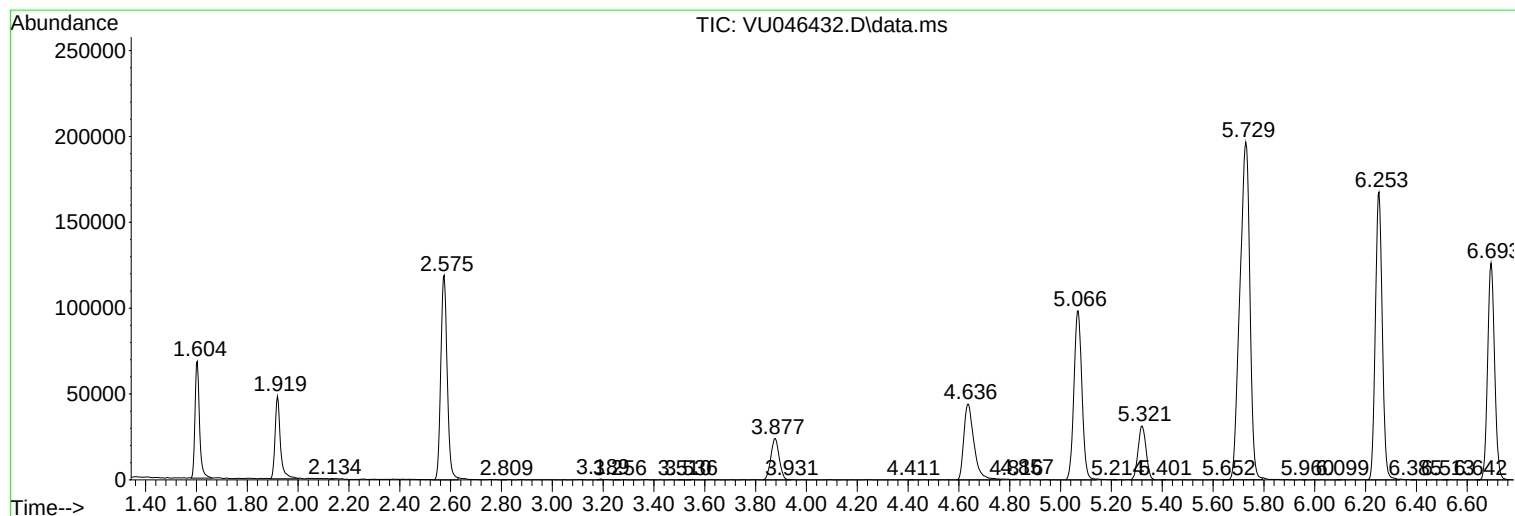

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046432.D
Acq On : 16 Dec 2021 19:25
Operator : SY/MD
Sample : M5037-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C00Z0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046432.D
Acq On : 16 Dec 2021 19:25
Operator : SY/MD
Sample : M5037-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C00Z0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------