

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046433.D
 Acq On : 16 Dec 2021 19:48
 Operator : SY/MD
 Sample : M5037-22
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C00Z2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046433.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	105	rBV	66984	83609	15.35%	1.961%
2	1.919	171	180	207	rBV	47310	71008	13.04%	1.665%
3	2.572	371	383	399	rBV	115970	190442	34.97%	4.466%
4	2.713	424	427	431	rVB	155	156	0.03%	0.004%
5	2.768	440	444	448	rBV	146	208	0.04%	0.005%
6	2.800	448	454	461	rVB	618	729	0.13%	0.017%
7	2.855	467	471	474	rBV	128	160	0.03%	0.004%
8	2.948	495	500	501	rBV	159	156	0.03%	0.004%
9	3.041	526	529	532	rBB	154	123	0.02%	0.003%
10	3.112	548	551	557	rBB	169	217	0.04%	0.005%
11	3.189	571	575	576	rVV	361	246	0.05%	0.006%
12	3.199	576	578	584	rVB2	233	198	0.04%	0.005%
13	3.314	611	614	617	rBV	123	131	0.02%	0.003%
14	3.401	638	641	644	rBV2	289	214	0.04%	0.005%
15	3.417	644	646	648	rVV	252	162	0.03%	0.004%
16	3.430	648	650	654	rVV	201	195	0.04%	0.005%
17	3.552	686	688	692	rBV	140	145	0.03%	0.003%
18	3.713	734	738	741	rBB	150	157	0.03%	0.004%
19	3.739	742	746	749	rBV	160	149	0.03%	0.003%
20	4.211	889	893	896	rBB	161	149	0.03%	0.003%
21	4.498	980	982	986	rBV	123	134	0.02%	0.003%
22	4.517	986	988	992	rVB	157	130	0.02%	0.003%
23	4.565	1000	1003	1006	rBB	151	129	0.02%	0.003%
24	4.636	1011	1025	1054	rBV	43735	121387	22.29%	2.846%
25	4.893	1102	1105	1107	rBV2	252	182	0.03%	0.004%
26	5.067	1143	1159	1180	rBV	100281	218170	40.06%	5.116%
27	5.170	1189	1191	1194	rVB2	325	163	0.03%	0.004%
28	5.263	1217	1220	1222	rBB	221	124	0.02%	0.003%
29	5.552	1306	1310	1313	rBB	130	135	0.02%	0.003%
30	5.729	1344	1365	1396	rBV2	202513	544653	100.00%	12.772%
31	6.253	1514	1528	1561	rBV	171543	325985	59.85%	7.644%
32	6.568	1623	1626	1630	rBB	126	135	0.02%	0.003%
33	6.694	1652	1665	1687	rBB	127093	242720	44.56%	5.692%
34	7.063	1775	1780	1783	rBV	198	228	0.04%	0.005%
35	7.157	1806	1809	1813	rBB	136	143	0.03%	0.003%
36	7.179	1813	1816	1818	rBV	313	271	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046433.D
 Acq On : 16 Dec 2021 19:48
 Operator : SY/MD
 Sample : M5037-22
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C00Z2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	7.346	1865	1868	1872	rBB	174	133	0.02%	0.003%
38	7.449	1897	1900	1903	rBV	137	140	0.03%	0.003%
39	7.568	1925	1937	1953	rVV	64831	112935	20.74%	2.648%
40	7.652	1961	1963	1967	rBV	118	128	0.02%	0.003%
41	7.690	1973	1975	1978	rBV2	176	140	0.03%	0.003%
42	7.748	1990	1993	1995	rBV	156	130	0.02%	0.003%
43	7.800	2006	2009	2013	rBB	163	161	0.03%	0.004%
44	7.899	2027	2040	2056	rBV	245080	419832	77.08%	9.845%
45	8.015	2074	2076	2082	rVB2	260	253	0.05%	0.006%
46	8.182	2117	2128	2141	rBV	45948	76088	13.97%	1.784%
47	8.231	2141	2143	2147	rVB2	299	132	0.02%	0.003%
48	8.266	2152	2154	2158	rVV	301	277	0.05%	0.006%
49	8.288	2158	2161	2164	rVV	135	143	0.03%	0.003%
50	8.311	2164	2168	2173	rVB2	312	316	0.06%	0.007%
51	8.478	2208	2220	2230	rVV3	3450	6650	1.22%	0.156%
52	8.520	2230	2233	2239	rVV2	251	343	0.06%	0.008%
53	8.581	2250	2252	2257	rVB	183	139	0.03%	0.003%
54	8.636	2257	2269	2291	rBV	158135	262946	48.28%	6.166%
55	9.005	2381	2384	2387	rBB	180	145	0.03%	0.003%
56	9.028	2387	2391	2394	rBV	174	199	0.04%	0.005%
57	9.112	2413	2417	2420	rBB	161	152	0.03%	0.004%
58	9.131	2421	2423	2428	rBV	192	195	0.04%	0.005%
59	9.276	2464	2468	2470	rBV	145	158	0.03%	0.004%
60	9.321	2479	2482	2485	rBB	154	125	0.02%	0.003%
61	9.353	2489	2492	2495	rVB	223	167	0.03%	0.004%
62	9.420	2500	2513	2533	rBV	260160	439840	80.76%	10.314%
63	9.578	2560	2562	2566	rBV	147	149	0.03%	0.003%
64	9.690	2595	2597	2598	rBV	353	172	0.03%	0.004%
65	9.819	2631	2637	2640	rBV	159	239	0.04%	0.006%
66	10.067	2711	2714	2717	rBV	161	165	0.03%	0.004%
67	10.481	2840	2843	2850	rBB	198	249	0.05%	0.006%
68	10.523	2850	2856	2859	rBV	189	261	0.05%	0.006%
69	10.575	2867	2872	2873	rBV	174	143	0.03%	0.003%
70	10.665	2895	2900	2901	rBV	628	393	0.07%	0.009%
71	10.758	2916	2929	2954	rVB	178323	281671	51.72%	6.605%
72	10.896	2963	2972	2985	rBV2	4186	6384	1.17%	0.150%
73	11.140	3043	3048	3051	rBV	157	206	0.04%	0.005%
74	11.185	3056	3062	3065	rBV	188	251	0.05%	0.006%
75	11.214	3067	3071	3076	rBV	186	264	0.05%	0.006%
76	11.452	3141	3145	3146	rBV	268	199	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046433.D
 Acq On : 16 Dec 2021 19:48
 Operator : SY/MD
 Sample : M5037-22
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C00Z2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.462	3146	3148	3151	rVB	356	218	0.04%	0.005%
78	11.700	3220	3222	3225	rVV	287	150	0.03%	0.004%
79	11.748	3229	3237	3246	rVV3	4268	6402	1.18%	0.150%
80	11.812	3246	3257	3277	rVV	273726	446279	81.94%	10.465%
81	11.938	3292	3296	3297	rBV	176	129	0.02%	0.003%
82	11.976	3303	3308	3316	rVB3	619	690	0.13%	0.016%
83	12.060	3328	3334	3336	rBV	879	769	0.14%	0.018%
84	12.195	3364	3376	3392	rVB	246725	387136	71.08%	9.078%
85	12.774	3548	3556	3565	rBV2	1376	2040	0.37%	0.048%
86	12.970	3614	3617	3619	rBV2	751	488	0.09%	0.011%
87	13.118	3658	3663	3666	rBV	143	152	0.03%	0.004%
88	13.848	3882	3890	3895	rVB3	1147	1192	0.22%	0.028%
89	14.574	4112	4116	4121	rVB	369	410	0.08%	0.010%
90	15.375	4362	4365	4369	rBV2	207	170	0.03%	0.004%
91	15.443	4382	4386	4388	rBV	242	169	0.03%	0.004%
92	15.491	4399	4401	4405	rVB2	234	142	0.03%	0.003%
93	15.603	4432	4436	4440	rBV2	190	210	0.04%	0.005%
94	15.664	4452	4455	4458	rVB2	178	128	0.02%	0.003%
95	15.822	4500	4504	4507	rBV	276	283	0.05%	0.007%
96	15.883	4519	4523	4530	rVB2	337	447	0.08%	0.010%
97	15.925	4530	4536	4540	rVB2	250	295	0.05%	0.007%
98	16.047	4569	4574	4578	rBV2	244	334	0.06%	0.008%
99	16.658	4760	4764	4768	rVB3	407	279	0.05%	0.007%
100	16.680	4768	4771	4772	rBV	265	133	0.02%	0.003%




Sum of corrected areas: 4264501

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046433.D
Acq On : 16 Dec 2021 19:48
Operator : SY/MD
Sample : M5037-22
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C00Z2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

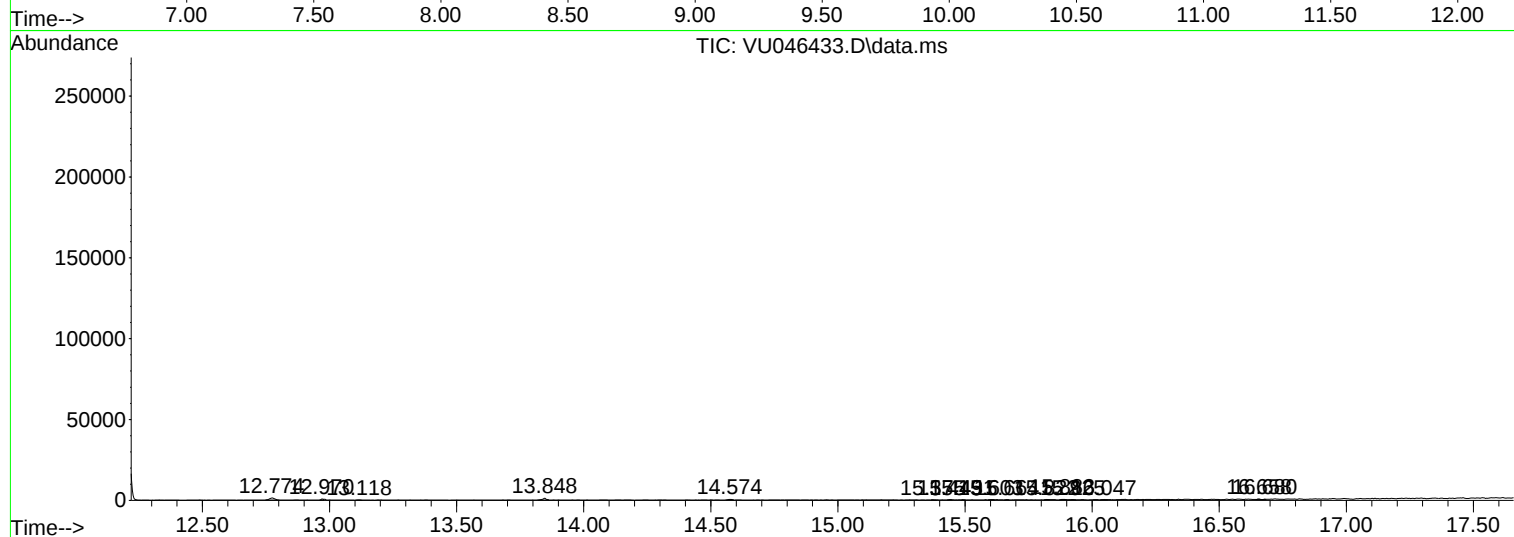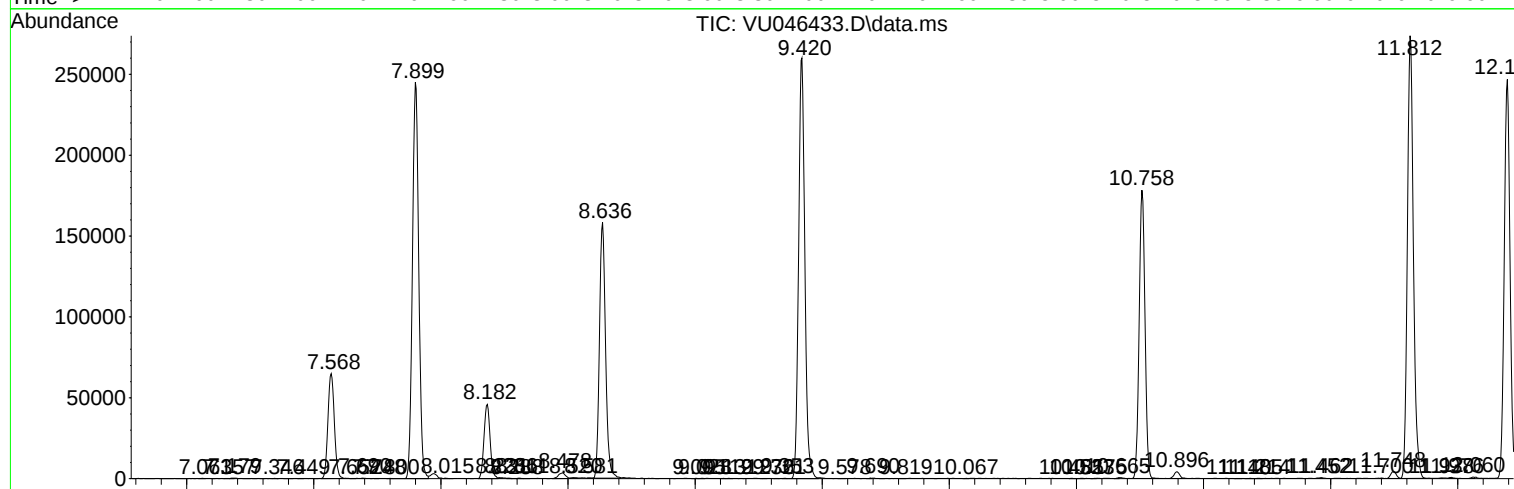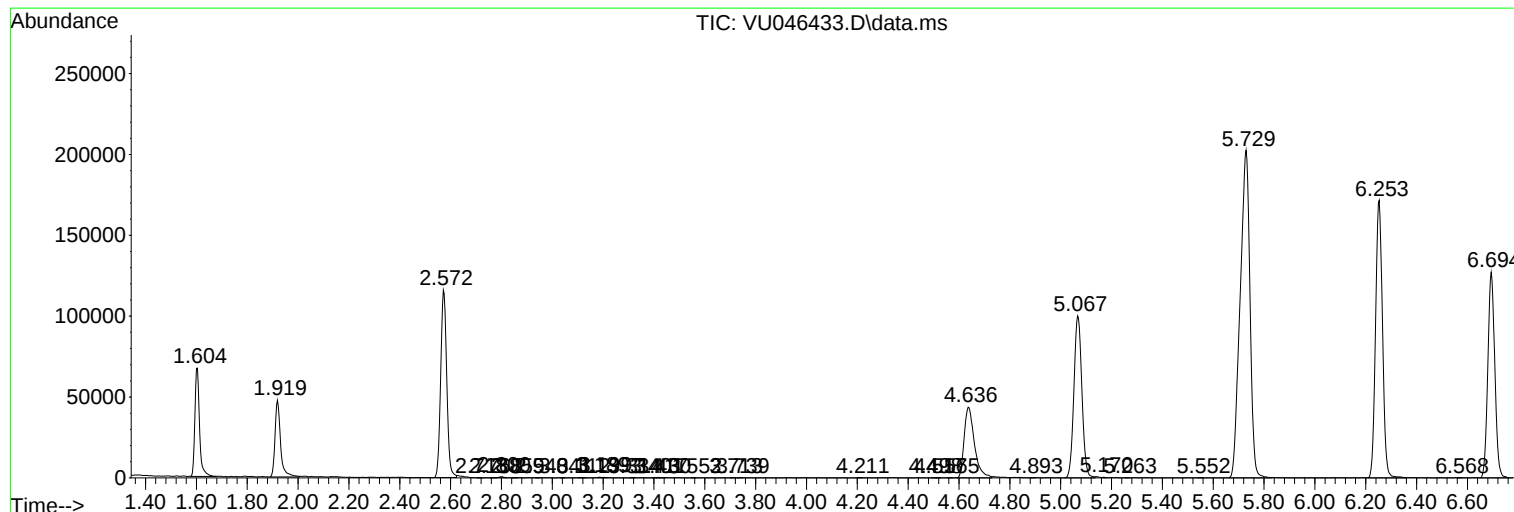

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046433.D
Acq On : 16 Dec 2021 19:48
Operator : SY/MD
Sample : M5037-22
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C00Z2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046433.D
Acq On : 16 Dec 2021 19:48
Operator : SY/MD
Sample : M5037-22
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C00Z2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------