

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046439.D
 Acq On : 16 Dec 2021 22:54
 Operator : SY/MD
 Sample : M5101-11ME
 Misc : 7.06g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL35ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046439.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	111	rVB	42332	78759	15.10%	1.757%
2	1.861	157	162	167	rBV3	815	1115	0.21%	0.025%
3	1.916	170	179	205	rBV	25129	56324	10.80%	1.257%
4	2.546	363	375	404	rBV	94522	181227	34.75%	4.044%
5	2.768	440	444	445	rBV	264	196	0.04%	0.004%
6	2.861	470	473	475	rBV	244	164	0.03%	0.004%
7	2.964	501	505	506	rBV	164	138	0.03%	0.003%
8	3.034	522	527	540	rVB3	984	1639	0.31%	0.037%
9	3.121	550	554	555	rBV	165	144	0.03%	0.003%
10	3.179	559	572	590	rBV2	12430	30285	5.81%	0.676%
11	3.288	601	606	609	rBV3	193	216	0.04%	0.005%
12	3.327	614	618	621	rBV2	170	186	0.04%	0.004%
13	3.372	630	632	637	rVB2	214	201	0.04%	0.004%
14	3.398	637	640	648	rVB3	337	289	0.06%	0.006%
15	3.536	680	683	686	rBV	132	138	0.03%	0.003%
16	3.806	763	767	771	rBV	158	200	0.04%	0.004%
17	3.861	774	784	791	rBV4	824	1469	0.28%	0.033%
18	4.092	852	856	859	rBV	142	164	0.03%	0.004%
19	4.584	1006	1009	1013	rBV	137	161	0.03%	0.004%
20	4.652	1016	1030	1077	rBV2	27878	131040	25.12%	2.924%
21	4.980	1129	1132	1138	rVB2	369	423	0.08%	0.009%
22	5.063	1142	1158	1182	rBV2	94386	207821	39.85%	4.637%
23	5.147	1182	1184	1189	rVB	236	158	0.03%	0.004%
24	5.314	1222	1236	1250	rBV3	14371	31880	6.11%	0.711%
25	5.459	1279	1281	1285	rBB	250	176	0.03%	0.004%
26	5.722	1343	1363	1380	rBV2	204664	521573	100.00%	11.637%
27	5.976	1433	1442	1459	rVV3	3234	7134	1.37%	0.159%
28	6.250	1512	1527	1551	rBV	188724	363686	69.73%	8.115%
29	6.539	1608	1617	1626	rBB7	3385	6334	1.21%	0.141%
30	6.603	1629	1637	1649	rBV5	1473	2925	0.56%	0.065%
31	6.690	1651	1664	1685	rVB	115364	230687	44.23%	5.147%
32	7.009	1760	1763	1767	rBV	148	168	0.03%	0.004%
33	7.179	1812	1816	1817	rBV	212	137	0.03%	0.003%
34	7.214	1825	1827	1828	rVV	425	210	0.04%	0.005%
35	7.230	1828	1832	1837	rVV2	655	719	0.14%	0.016%
36	7.263	1840	1842	1845	rBV	341	199	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046439.D
 Acq On : 16 Dec 2021 22:54
 Operator : SY/MD
 Sample : M5101-11ME
 Misc : 7.06g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL35ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	7.378	1874	1878	1880	rBV	145	139	0.03%	0.003%
38	7.433	1889	1895	1898	rBB	140	194	0.04%	0.004%
39	7.497	1912	1915	1918	rBV	133	142	0.03%	0.003%
40	7.568	1925	1937	1958	rBV	57568	111316	21.34%	2.484%
41	7.642	1958	1960	1963	rVB	294	163	0.03%	0.004%
42	7.697	1974	1977	1980	rBB	258	164	0.03%	0.004%
43	7.716	1980	1983	1985	rBV	154	124	0.02%	0.003%
44	7.790	1998	2006	2017	rBV	1174	2005	0.38%	0.045%
45	7.899	2027	2040	2056	rBV	238134	416141	79.79%	9.285%
46	7.970	2056	2062	2065	rBV3	1934	2371	0.45%	0.053%
47	8.102	2098	2103	2106	rBB	163	187	0.04%	0.004%
48	8.131	2109	2112	2117	rBV	159	202	0.04%	0.005%
49	8.185	2117	2129	2152	rVB2	33566	76311	14.63%	1.703%
50	8.404	2194	2197	2200	rBV	157	153	0.03%	0.003%
51	8.475	2213	2219	2220	rBV2	485	452	0.09%	0.010%
52	8.510	2228	2230	2233	rVB2	215	130	0.02%	0.003%
53	8.552	2233	2243	2257	rVB	50882	84768	16.25%	1.891%
54	8.603	2257	2259	2261	rVB	274	144	0.03%	0.003%
55	8.681	2261	2283	2304	rBV	90483	254062	48.71%	5.669%
56	8.880	2342	2345	2351	rBV	174	235	0.05%	0.005%
57	8.941	2361	2364	2367	rVV2	355	315	0.06%	0.007%
58	8.960	2367	2370	2375	rVB3	496	499	0.10%	0.011%
59	8.989	2376	2379	2384	rBB	174	198	0.04%	0.004%
60	9.086	2406	2409	2415	rVB	180	243	0.05%	0.005%
61	9.253	2458	2461	2465	rBV	181	195	0.04%	0.004%
62	9.423	2500	2514	2533	rBV	242412	492201	94.37%	10.982%
63	9.568	2555	2559	2567	rBV2	293	411	0.08%	0.009%
64	9.700	2594	2600	2606	rVB2	566	893	0.17%	0.020%
65	9.835	2640	2642	2647	rBV	152	179	0.03%	0.004%
66	9.918	2665	2668	2671	rBB	148	123	0.02%	0.003%
67	10.105	2723	2726	2728	rBV	286	208	0.04%	0.005%
68	10.176	2740	2748	2751	rBV	193	289	0.06%	0.006%
69	10.468	2832	2839	2843	rBV	172	270	0.05%	0.006%
70	10.491	2844	2846	2851	rVB2	167	173	0.03%	0.004%
71	10.561	2865	2868	2870	rBV	162	135	0.03%	0.003%
72	10.674	2896	2903	2912	rVB4	1008	1514	0.29%	0.034%
73	10.770	2921	2933	2949	rVV	167500	277306	53.17%	6.187%
74	10.877	2959	2966	2967	rBV2	334	398	0.08%	0.009%
75	10.902	2970	2974	2982	rVB	681	981	0.19%	0.022%
76	10.973	2990	2996	2999	rBV	144	227	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046439.D
 Acq On : 16 Dec 2021 22:54
 Operator : SY/MD
 Sample : M5101-11ME
 Misc : 7.06g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL35ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.118	3036	3041	3047	rBV3	849	867	0.17%	0.019%
78	11.452	3140	3145	3146	rBV3	399	279	0.05%	0.006%
79	11.696	3217	3221	3228	rBV	428	452	0.09%	0.010%
80	11.754	3235	3239	3243	rBV2	502	456	0.09%	0.010%
81	11.819	3246	3259	3277	rVV	318695	499202	95.71%	11.138%
82	11.947	3294	3299	3301	rVV	190	214	0.04%	0.005%
83	11.976	3303	3308	3318	rVB3	531	716	0.14%	0.016%
84	12.201	3365	3378	3392	rVV	238887	387620	74.32%	8.649%
85	12.774	3550	3556	3562	rBV	749	989	0.19%	0.022%
86	13.015	3628	3631	3638	rVB	128	131	0.03%	0.003%
87	13.230	3693	3698	3702	rBV2	448	481	0.09%	0.011%
88	13.430	3756	3760	3765	rBV	134	140	0.03%	0.003%
89	13.841	3884	3888	3889	rBV	558	313	0.06%	0.007%
90	14.092	3960	3966	3972	rBV2	411	596	0.11%	0.013%
91	14.336	4036	4042	4045	rBV	328	328	0.06%	0.007%
92	14.581	4109	4118	4127	rBV2	938	1455	0.28%	0.032%
93	15.082	4271	4274	4277	rBV2	201	150	0.03%	0.003%
94	15.391	4367	4370	4374	rVB2	193	136	0.03%	0.003%
95	15.677	4456	4459	4462	rBV	197	149	0.03%	0.003%
96	15.693	4462	4464	4468	rBV	189	153	0.03%	0.003%
97	16.191	4609	4619	4628	rBV2	1148	1911	0.37%	0.043%
98	16.439	4693	4696	4700	rBV	321	234	0.04%	0.005%
99	17.040	4880	4883	4885	rBV2	399	256	0.05%	0.006%
100	17.185	4926	4928	4929	rBV2	470	161	0.03%	0.004%




Sum of corrected areas: 4481835

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046439.D
Acq On : 16 Dec 2021 22:54
Operator : SY/MD
Sample : M5101-11ME
Misc : 7.06g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL35ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

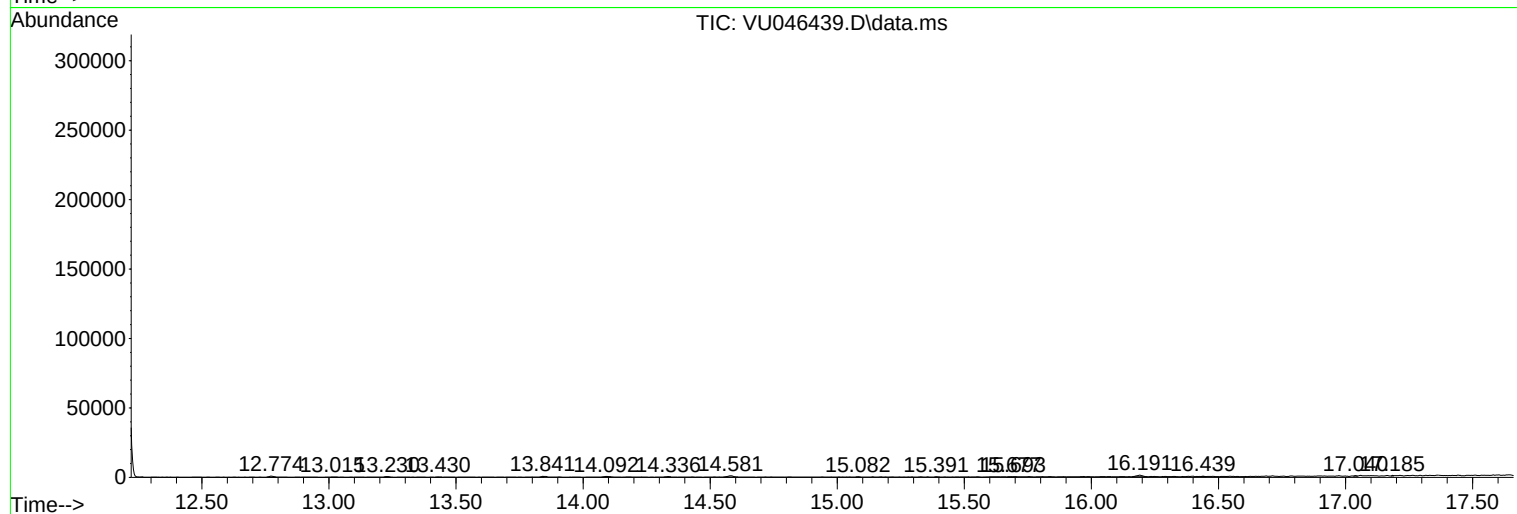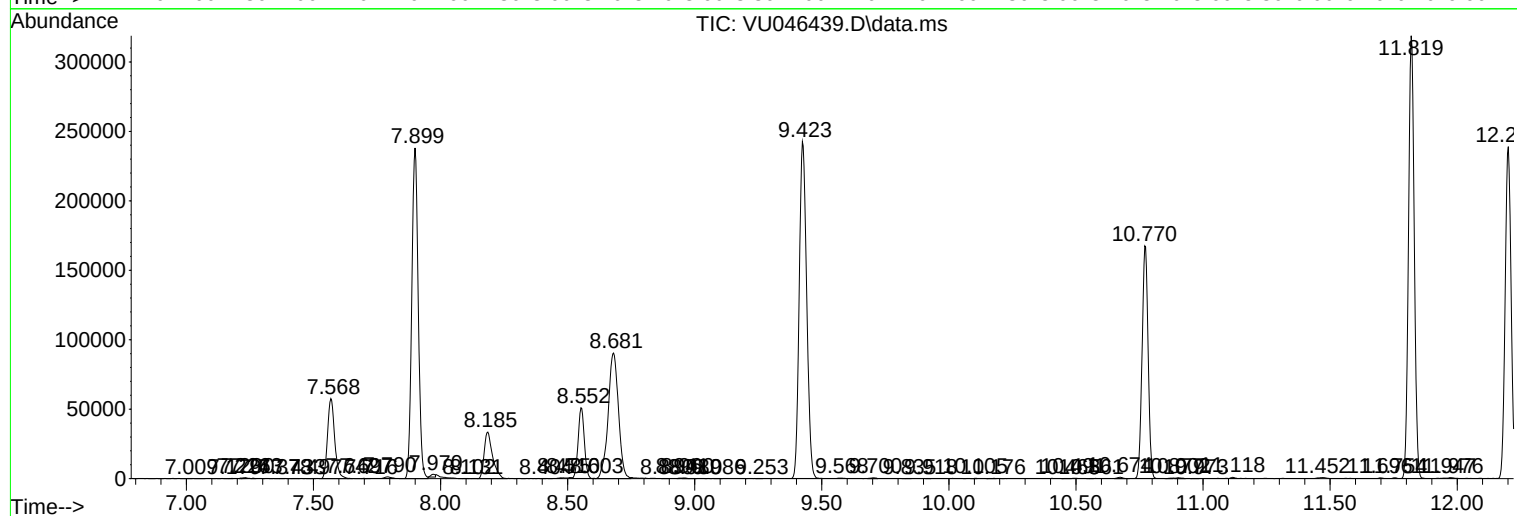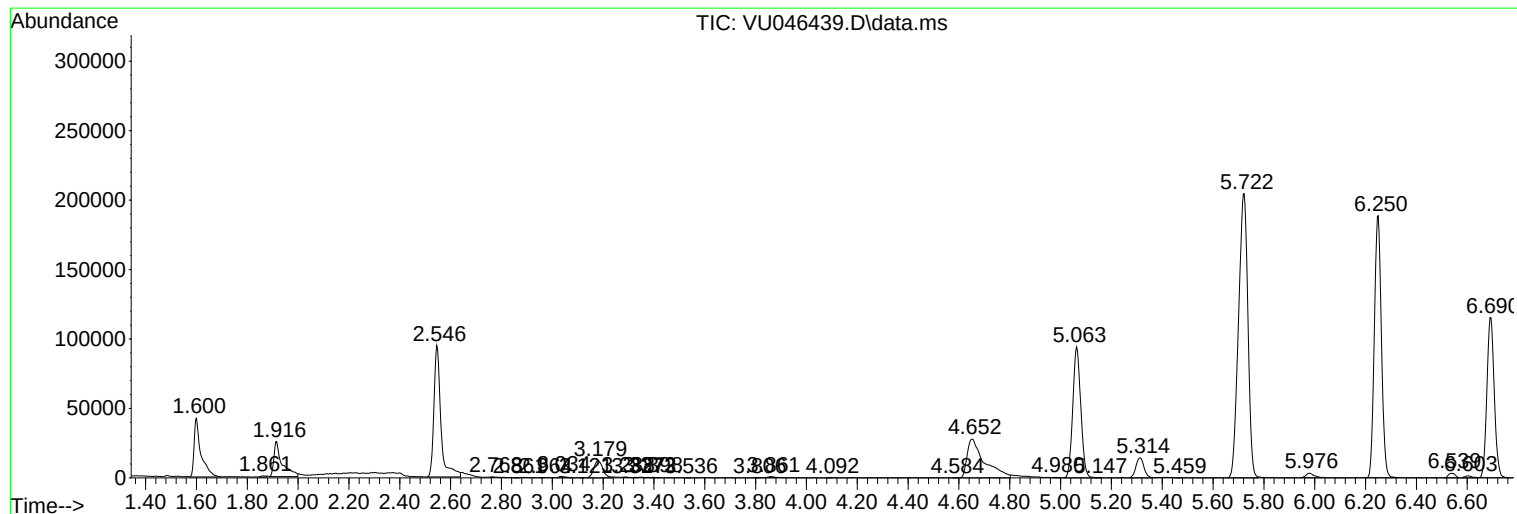

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046439.D
Acq On : 16 Dec 2021 22:54
Operator : SY/MD
Sample : M5101-11ME
Misc : 7.06g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL35ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046439.D
Acq On : 16 Dec 2021 22:54
Operator : SY/MD
Sample : M5101-11ME
Misc : 7.06g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL35ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc