

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046445.D
 Acq On : 17 Dec 2021 01:10
 Operator : SY/MD
 Sample : M5101-14DL 20X
 Misc : 6.90g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL38DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046445.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	101	rBV	61616	77644	14.73%	1.774%
2	1.839	152	155	157	rBV	226	136	0.03%	0.003%
3	1.919	171	180	198	rBV	43404	62790	11.91%	1.434%
4	2.231	274	277	280	rBV	172	145	0.03%	0.003%
5	2.572	370	383	412	rBV2	114143	192288	36.48%	4.392%
6	2.703	421	424	428	rBV	179	196	0.04%	0.004%
7	2.768	441	444	450	rVB	181	236	0.04%	0.005%
8	2.800	450	454	457	rBB	277	224	0.04%	0.005%
9	2.819	457	460	463	rBV	170	163	0.03%	0.004%
10	2.880	477	479	482	rBV	175	138	0.03%	0.003%
11	2.935	494	496	499	rBV	147	132	0.03%	0.003%
12	3.051	525	532	540	rBB3	892	1537	0.29%	0.035%
13	3.134	556	558	562	rBV	125	137	0.03%	0.003%
14	3.189	562	575	592	rVB	7775	16623	3.15%	0.380%
15	3.366	624	630	633	rBB	161	203	0.04%	0.005%
16	3.530	679	681	686	rBV	124	150	0.03%	0.003%
17	3.623	707	710	713	rBV	145	151	0.03%	0.003%
18	3.729	739	743	745	rBV	121	128	0.02%	0.003%
19	3.871	777	787	801	rBB3	2808	5719	1.08%	0.131%
20	4.301	918	921	925	rBV	156	168	0.03%	0.004%
21	4.636	1009	1025	1061	rBV	49372	130943	24.84%	2.991%
22	5.067	1144	1159	1187	rVV	97399	210951	40.02%	4.819%
23	5.234	1208	1211	1215	rVB2	211	185	0.04%	0.004%
24	5.340	1240	1244	1249	rBV2	182	194	0.04%	0.004%
25	5.729	1343	1365	1388	rBV2	196954	527161	100.00%	12.042%
26	5.809	1388	1390	1392	rVV	347	222	0.04%	0.005%
27	5.835	1396	1398	1403	rVV	207	192	0.04%	0.004%
28	5.867	1405	1408	1410	rBV	241	136	0.03%	0.003%
29	6.250	1513	1527	1554	rBV	179096	335947	63.73%	7.674%
30	6.546	1608	1619	1631	rBB2	18851	34333	6.51%	0.784%
31	6.694	1652	1665	1683	rBV	121677	235652	44.70%	5.383%
32	6.800	1696	1698	1700	rBV	238	133	0.03%	0.003%
33	6.813	1700	1702	1705	rVB	275	178	0.03%	0.004%
34	7.089	1786	1788	1792	rBV	139	138	0.03%	0.003%
35	7.568	1925	1937	1953	rBV	63876	109254	20.72%	2.496%
36	7.787	1999	2005	2014	rVB3	658	952	0.18%	0.022%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046445.D
 Acq On : 17 Dec 2021 01:10
 Operator : SY/MD
 Sample : M5101-14DL 20X
 Misc : 6.90g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL38DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	7.835	2015	2020	2023	rBB	170	193	0.04%	0.004%
38	7.899	2027	2040	2055	rBV	239659	405862	76.99%	9.271%
39	7.970	2057	2062	2071	rVB	4105	6063	1.15%	0.138%
40	8.108	2102	2105	2109	rBB	156	151	0.03%	0.003%
41	8.182	2117	2128	2143	rBV	44538	73806	14.00%	1.686%
42	8.266	2151	2154	2156	rVV	244	192	0.04%	0.004%
43	8.279	2156	2158	2162	rVV	293	234	0.04%	0.005%
44	8.301	2162	2165	2167	rVV2	284	210	0.04%	0.005%
45	8.314	2167	2169	2172	rVV2	265	192	0.04%	0.004%
46	8.475	2213	2219	2224	rBV	492	673	0.13%	0.015%
47	8.497	2224	2226	2229	rVV	329	218	0.04%	0.005%
48	8.555	2232	2244	2257	rVB	80034	132932	25.22%	3.036%
49	8.636	2257	2269	2293	rBV	154629	260288	49.38%	5.946%
50	8.912	2349	2355	2360	rBV	1154	1417	0.27%	0.032%
51	9.150	2426	2429	2432	rBB	140	119	0.02%	0.003%
52	9.179	2433	2438	2443	rBV	150	219	0.04%	0.005%
53	9.301	2473	2476	2480	rBB	139	144	0.03%	0.003%
54	9.321	2480	2482	2485	rBV	146	130	0.02%	0.003%
55	9.420	2498	2513	2531	rBV	266786	435746	82.66%	9.954%
56	9.542	2548	2551	2556	rBB	168	197	0.04%	0.004%
57	9.649	2582	2584	2589	rVB	180	167	0.03%	0.004%
58	9.677	2589	2593	2594	rBV	172	141	0.03%	0.003%
59	9.694	2594	2598	2603	rVV	239	314	0.06%	0.007%
60	9.829	2638	2640	2644	rBB	140	121	0.02%	0.003%
61	9.854	2645	2648	2654	rBV	187	249	0.05%	0.006%
62	9.960	2678	2681	2684	rBB	164	130	0.02%	0.003%
63	10.021	2696	2700	2702	rBV	168	168	0.03%	0.004%
64	10.153	2739	2741	2746	rBV	145	170	0.03%	0.004%
65	10.214	2755	2760	2763	rBV	177	224	0.04%	0.005%
66	10.671	2895	2902	2910	rVB2	719	844	0.16%	0.019%
67	10.758	2917	2929	2945	rBV	175221	274929	52.15%	6.280%
68	10.902	2966	2974	2978	rVV	458	477	0.09%	0.011%
69	11.073	3024	3027	3032	rBV	189	214	0.04%	0.005%
70	11.108	3035	3038	3042	rVB	212	202	0.04%	0.005%
71	11.131	3042	3045	3047	rBV	186	148	0.03%	0.003%
72	11.147	3047	3050	3055	rVB	135	122	0.02%	0.003%
73	11.462	3142	3148	3158	rBV4	706	989	0.19%	0.023%
74	11.690	3213	3219	3222	rBV2	212	227	0.04%	0.005%
75	11.812	3245	3257	3272	rBV	283461	439113	83.30%	10.030%
76	11.925	3287	3292	3294	rBV	168	195	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046445.D
 Acq On : 17 Dec 2021 01:10
 Operator : SY/MD
 Sample : M5101-14DL 20X
 Misc : 6.90g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL38DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.941	3294	3297	3301	rVV2	288	322	0.06%	0.007%
78	11.967	3301	3305	3314	rVB3	456	676	0.13%	0.015%
79	12.021	3319	3322	3330	rVB	148	173	0.03%	0.004%
80	12.195	3362	3376	3390	rBV	242324	387849	73.57%	8.859%
81	12.774	3549	3556	3561	rVB3	597	814	0.15%	0.019%
82	14.105	3965	3970	3974	rBV2	245	240	0.05%	0.005%
83	14.581	4110	4118	4126	rBV2	611	826	0.16%	0.019%
84	15.278	4332	4335	4341	rVB	183	167	0.03%	0.004%
85	15.314	4342	4346	4349	rBV2	181	149	0.03%	0.003%
86	15.417	4374	4378	4383	rVB2	201	179	0.03%	0.004%
87	15.439	4383	4385	4389	rVB	229	129	0.02%	0.003%
88	15.465	4389	4393	4394	rBV	249	174	0.03%	0.004%
89	15.475	4394	4396	4399	rVB2	207	126	0.02%	0.003%
90	15.516	4406	4409	4412	rBV2	204	144	0.03%	0.003%
91	15.619	4437	4441	4443	rBV2	200	170	0.03%	0.004%
92	15.700	4463	4466	4469	rBV2	159	141	0.03%	0.003%
93	15.748	4477	4481	4484	rBV2	233	203	0.04%	0.005%
94	15.799	4495	4497	4499	rVB	316	146	0.03%	0.003%
95	15.838	4506	4509	4515	rVB2	239	283	0.05%	0.006%
96	16.436	4692	4695	4697	rBV2	246	180	0.03%	0.004%
97	16.594	4740	4744	4748	rBV2	315	314	0.06%	0.007%
98	16.661	4762	4765	4768	rBV2	284	238	0.05%	0.005%
99	16.854	4822	4825	4829	rVB2	496	341	0.06%	0.008%
100	17.147	4914	4916	4919	rBV	359	218	0.04%	0.005%




Sum of corrected areas: 4377811

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046445.D
Acq On : 17 Dec 2021 01:10
Operator : SY/MD
Sample : M5101-14DL 20X
Misc : 6.90g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL38DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

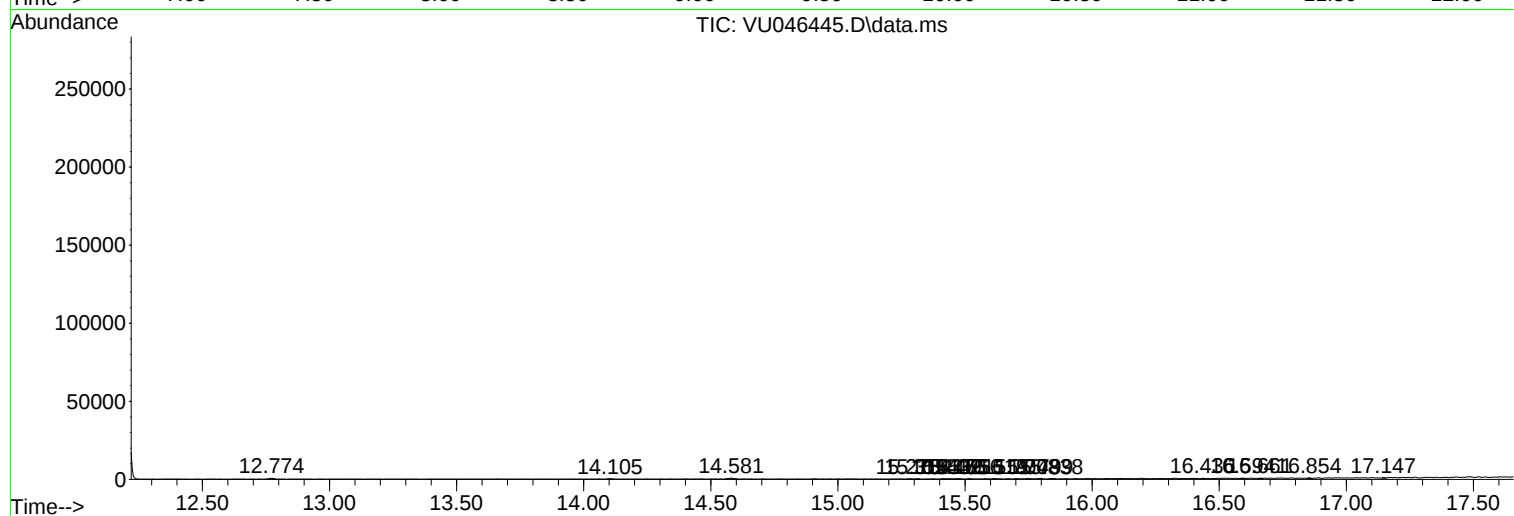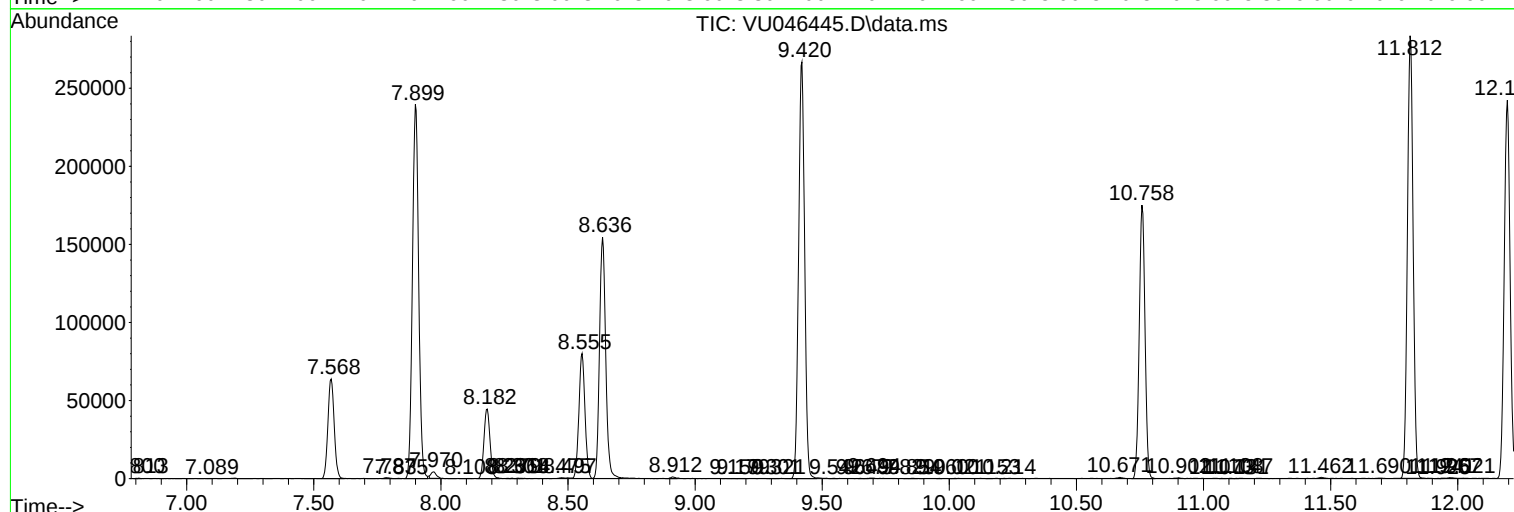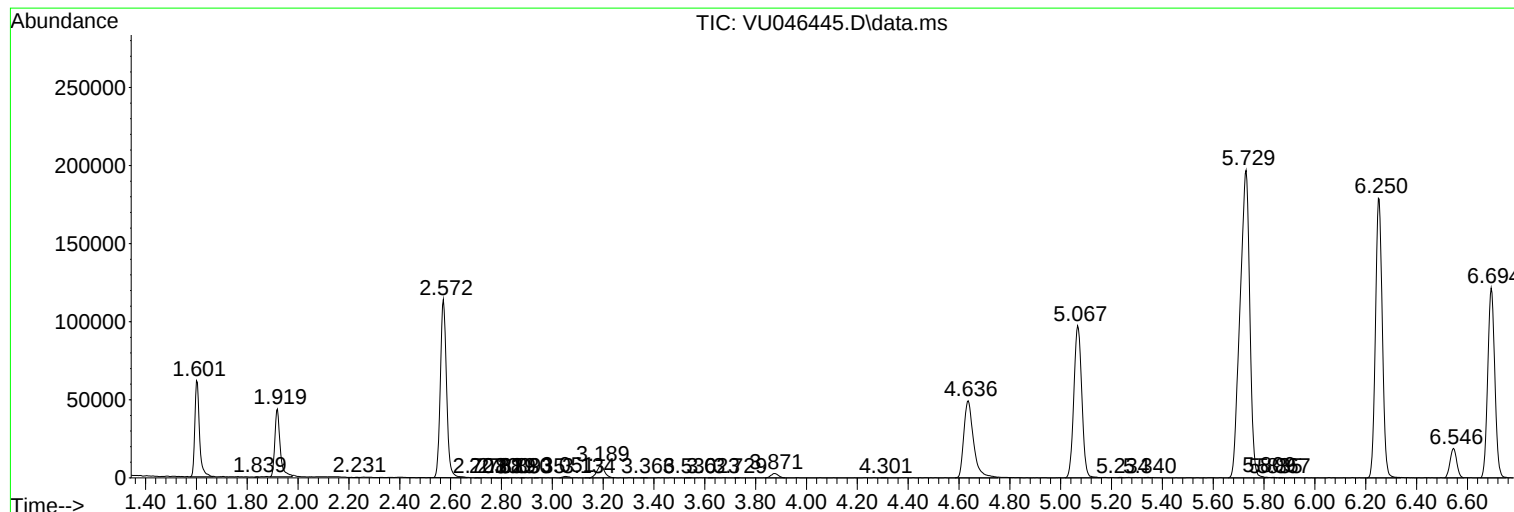

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046445.D
Acq On : 17 Dec 2021 01:10
Operator : SY/MD
Sample : M5101-14DL 20X
Misc : 6.90g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL38DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046445.D
Acq On : 17 Dec 2021 01:10
Operator : SY/MD
Sample : M5101-14DL 20X
Misc : 6.90g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL38DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc