

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046446.D
 Acq On : 17 Dec 2021 01:33
 Operator : SY/MD
 Sample : M5101-15ME 20X
 Misc : 6.30g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL39ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046446.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	105	rVB	60865	75879	14.63%	1.843%
2	1.694	108	110	112	rBV	321	180	0.03%	0.004%
3	1.919	171	180	200	rVB	43727	61884	11.93%	1.503%
4	2.154	250	253	254	rBV	231	161	0.03%	0.004%
5	2.192	263	265	268	rBV2	213	157	0.03%	0.004%
6	2.302	296	299	301	rBV2	147	125	0.02%	0.003%
7	2.414	332	334	338	rVB	288	204	0.04%	0.005%
8	2.572	371	383	411	rBV	110599	181513	34.99%	4.410%
9	2.739	433	435	440	rVB	155	152	0.03%	0.004%
10	2.774	443	446	448	rBV	150	126	0.02%	0.003%
11	2.897	481	484	490	rBB	148	172	0.03%	0.004%
12	3.012	518	520	525	rVV	160	176	0.03%	0.004%
13	3.054	525	533	542	rVB3	1090	2034	0.39%	0.049%
14	3.189	561	575	592	rVB	8486	18460	3.56%	0.448%
15	4.636	1011	1025	1052	rBV2	49121	131263	25.30%	3.189%
16	4.819	1079	1082	1086	rVV	201	208	0.04%	0.005%
17	4.851	1090	1092	1095	rVV	198	121	0.02%	0.003%
18	4.913	1108	1111	1114	rBV	139	140	0.03%	0.003%
19	4.977	1126	1131	1135	rBB	154	202	0.04%	0.005%
20	5.067	1143	1159	1177	rBV	96848	208912	40.27%	5.075%
21	5.202	1197	1201	1205	rVV2	252	219	0.04%	0.005%
22	5.292	1226	1229	1231	rVB2	268	137	0.03%	0.003%
23	5.324	1236	1239	1241	rBV	146	116	0.02%	0.003%
24	5.729	1342	1365	1390	rBV2	192051	518788	100.00%	12.604%
25	6.067	1467	1470	1474	rBB	135	120	0.02%	0.003%
26	6.250	1513	1527	1544	rBV	171789	322218	62.11%	7.828%
27	6.437	1583	1585	1589	rBB	145	123	0.02%	0.003%
28	6.694	1652	1665	1684	rBV	121659	232642	44.84%	5.652%
29	7.015	1761	1765	1768	rBB	136	135	0.03%	0.003%
30	7.183	1813	1817	1821	rBV	327	235	0.05%	0.006%
31	7.372	1874	1876	1880	rBB	149	126	0.02%	0.003%
32	7.568	1921	1937	1956	rBV	62602	107345	20.69%	2.608%
33	7.691	1973	1975	1978	rVB2	241	139	0.03%	0.003%
34	7.790	1999	2006	2012	rBB2	726	1156	0.22%	0.028%
35	7.900	2026	2040	2056	rVV	238142	402773	77.64%	9.785%
36	7.970	2057	2062	2077	rVV3	3064	5069	0.98%	0.123%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046446.D
 Acq On : 17 Dec 2021 01:33
 Operator : SY/MD
 Sample : M5101-15ME 20X
 Misc : 6.30g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL39ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	8.086	2095	2098	2101	rBB	139	120	0.02%	0.003%
38	8.179	2117	2127	2141	rVV	43298	71532	13.79%	1.738%
39	8.314	2166	2169	2172	rVV	147	123	0.02%	0.003%
40	8.340	2174	2177	2180	rBV	256	190	0.04%	0.005%
41	8.395	2190	2194	2196	rBV	140	120	0.02%	0.003%
42	8.472	2213	2218	2219	rBV	429	372	0.07%	0.009%
43	8.584	2251	2253	2257	rVB2	263	185	0.04%	0.004%
44	8.636	2257	2269	2297	rBV	151604	256636	49.47%	6.235%
45	8.764	2305	2309	2313	rVB2	268	282	0.05%	0.007%
46	8.800	2318	2320	2323	rVB	183	118	0.02%	0.003%
47	8.822	2324	2327	2329	rBV	143	119	0.02%	0.003%
48	8.838	2329	2332	2335	rVB	176	140	0.03%	0.003%
49	8.861	2337	2339	2342	rBV	147	128	0.02%	0.003%
50	8.916	2348	2356	2366	rVB3	1163	1985	0.38%	0.048%
51	8.993	2377	2380	2383	rBV	138	149	0.03%	0.004%
52	9.028	2388	2391	2394	rBV	153	145	0.03%	0.004%
53	9.147	2426	2428	2431	rBV	144	121	0.02%	0.003%
54	9.244	2454	2458	2461	rBV	137	141	0.03%	0.003%
55	9.420	2500	2513	2535	rVV	253380	421572	81.26%	10.242%
56	9.501	2535	2538	2539	rVV	198	133	0.03%	0.003%
57	9.584	2560	2564	2568	rBB	163	152	0.03%	0.004%
58	9.645	2581	2583	2589	rBV	189	221	0.04%	0.005%
59	9.697	2594	2599	2604	rVV2	232	274	0.05%	0.007%
60	9.790	2626	2628	2631	rBV	130	114	0.02%	0.003%
61	9.822	2634	2638	2643	rBV	154	233	0.04%	0.006%
62	10.031	2697	2703	2708	rBV	164	273	0.05%	0.007%
63	10.215	2757	2760	2764	rBB	169	157	0.03%	0.004%
64	10.247	2767	2770	2772	rBV	165	135	0.03%	0.003%
65	10.282	2778	2781	2784	rBB	135	115	0.02%	0.003%
66	10.305	2784	2788	2791	rBV	129	155	0.03%	0.004%
67	10.379	2803	2811	2814	rBV	208	349	0.07%	0.008%
68	10.430	2824	2827	2830	rBV	134	143	0.03%	0.003%
69	10.459	2833	2836	2839	rVB	159	132	0.03%	0.003%
70	10.536	2857	2860	2863	rBB	138	122	0.02%	0.003%
71	10.671	2898	2902	2909	rVB2	587	624	0.12%	0.015%
72	10.758	2916	2929	2945	rBV	172864	274568	52.92%	6.670%
73	10.899	2968	2973	2981	rBV	292	470	0.09%	0.011%
74	11.028	3008	3013	3016	rBB	172	172	0.03%	0.004%
75	11.366	3114	3118	3121	rBV	182	217	0.04%	0.005%
76	11.465	3142	3149	3156	rVB3	499	870	0.17%	0.021%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046446.D
 Acq On : 17 Dec 2021 01:33
 Operator : SY/MD
 Sample : M5101-15ME 20X
 Misc : 6.30g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL39ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.652	3204	3207	3210	rBV	135	140	0.03%	0.003%
78	11.690	3218	3219	3224	rVB	160	120	0.02%	0.003%
79	11.813	3246	3257	3278	rBV	274494	422233	81.39%	10.258%
80	11.944	3292	3298	3303	rBV	202	246	0.05%	0.006%
81	11.970	3303	3306	3309	rBV	360	256	0.05%	0.006%
82	12.079	3335	3340	3343	rBV	195	252	0.05%	0.006%
83	12.195	3364	3376	3393	rVB	239981	381258	73.49%	9.262%
84	12.777	3548	3557	3562	rVB3	422	639	0.12%	0.016%
85	12.922	3599	3602	3607	rBV	177	183	0.04%	0.004%
86	13.243	3699	3702	3708	rBV	147	129	0.02%	0.003%
87	14.571	4109	4115	4117	rBV	409	397	0.08%	0.010%
88	14.742	4162	4168	4172	rBV	178	215	0.04%	0.005%
89	15.436	4382	4384	4388	rVB	225	125	0.02%	0.003%
90	15.546	4415	4418	4425	rVB2	240	263	0.05%	0.006%
91	15.607	4432	4437	4440	rBV2	224	274	0.05%	0.007%
92	15.668	4448	4456	4460	rVB2	284	414	0.08%	0.010%
93	15.716	4468	4471	4476	rBB2	161	177	0.03%	0.004%
94	15.761	4483	4485	4489	rVB2	161	122	0.02%	0.003%
95	15.793	4492	4495	4499	rBV	160	154	0.03%	0.004%
96	15.848	4508	4512	4516	rBV	246	291	0.06%	0.007%
97	16.626	4751	4754	4756	rBV2	285	176	0.03%	0.004%
98	16.841	4819	4821	4823	rVB2	346	142	0.03%	0.003%
99	17.037	4878	4882	4886	rBV4	472	460	0.09%	0.011%
100	17.349	4977	4979	4981	rBV	459	303	0.06%	0.007%




Sum of corrected areas: 4116186

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046446.D
Acq On : 17 Dec 2021 01:33
Operator : SY/MD
Sample : M5101-15ME 20X
Misc : 6.30g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL39ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

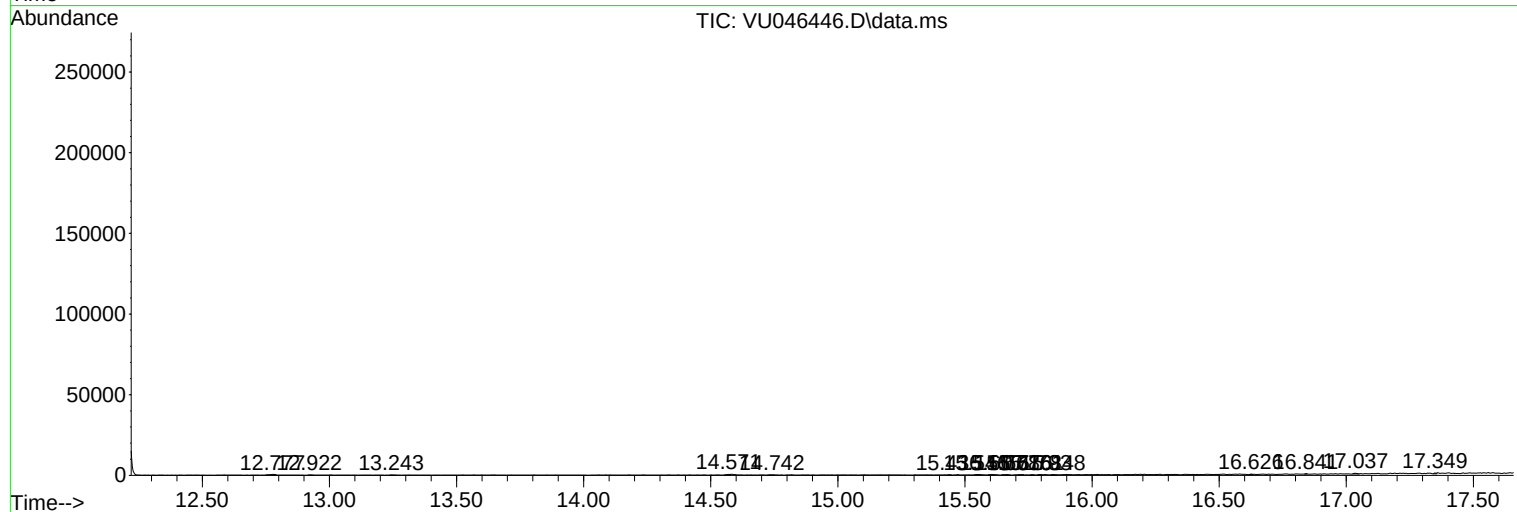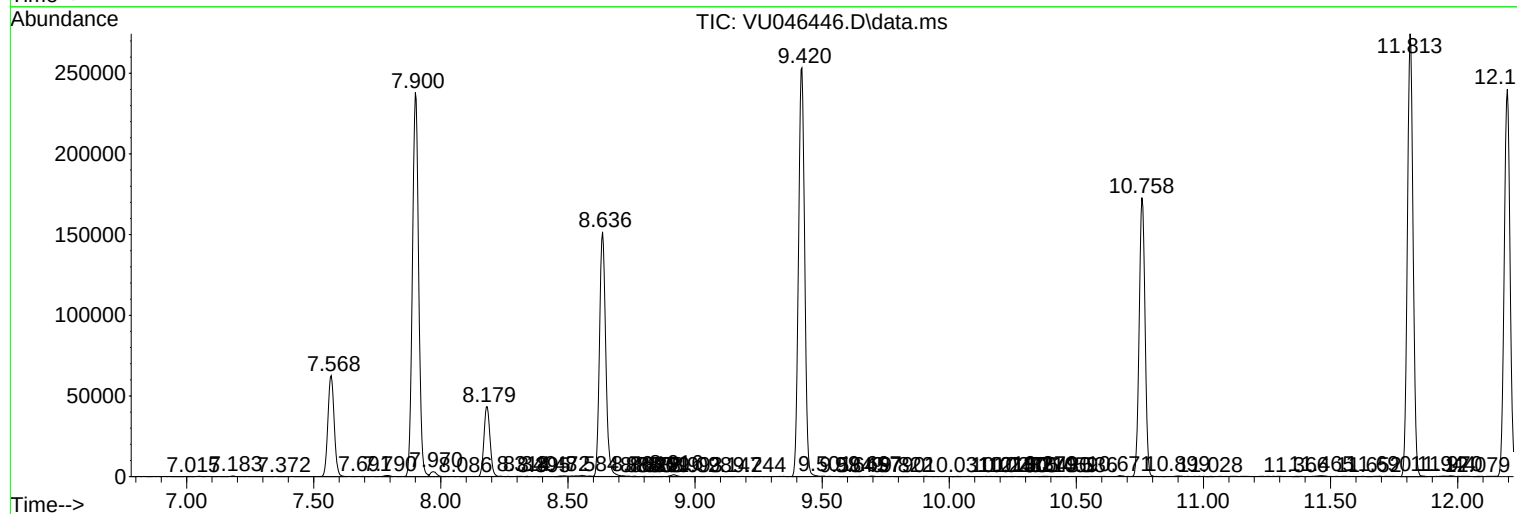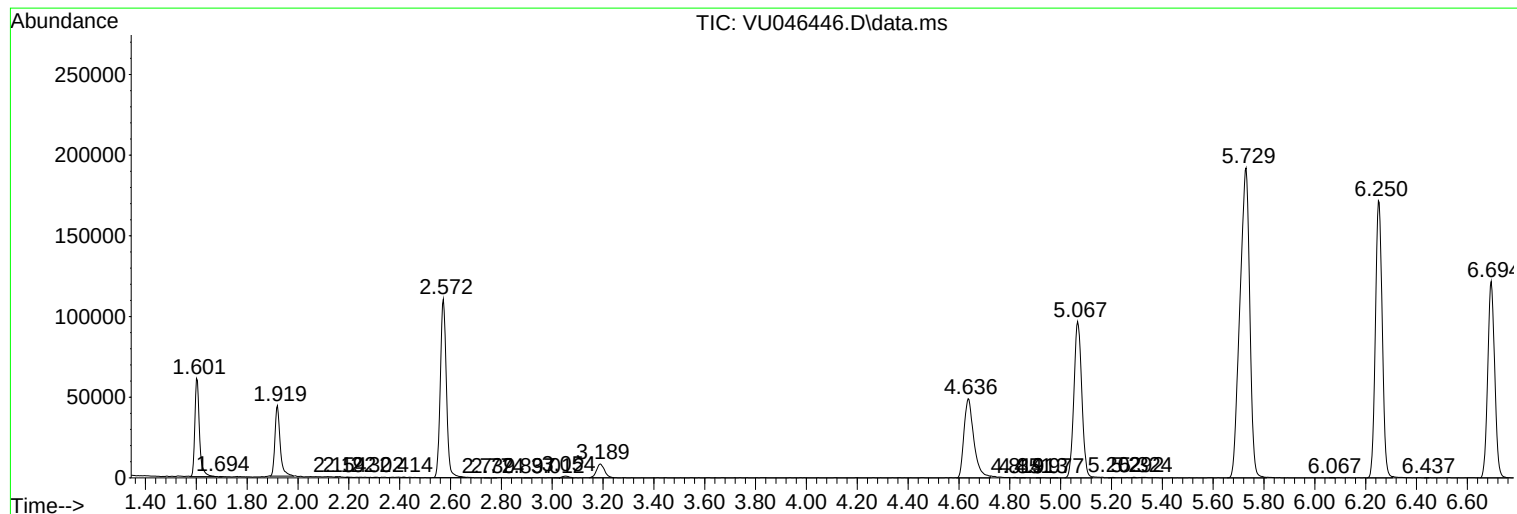

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046446.D
Acq On : 17 Dec 2021 01:33
Operator : SY/MD
Sample : M5101-15ME 20X
Misc : 6.30g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL39ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046446.D
Acq On : 17 Dec 2021 01:33
Operator : SY/MD
Sample : M5101-15ME 20X
Misc : 6.30g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL39ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc