

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046447.D
 Acq On : 17 Dec 2021 01:55
 Operator : SY/MD
 Sample : M5121-01 20X
 Misc : 4.41g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL50

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046447.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	73	82	106	rVB	58720	75281	14.90%	1.869%
2	1.919	171	180	206	rVB	42692	61876	12.24%	1.537%
3	2.228	274	276	280	rVB2	346	200	0.04%	0.005%
4	2.430	335	339	340	rBV	164	128	0.03%	0.003%
5	2.572	371	383	408	rBV	103028	171863	34.01%	4.268%
6	2.864	471	474	476	rBV	164	139	0.03%	0.003%
7	3.054	525	533	540	rVB5	1160	2031	0.40%	0.050%
8	3.092	541	545	548	rBB	166	141	0.03%	0.004%
9	3.189	563	575	591	rBB	8413	19071	3.77%	0.474%
10	3.260	591	597	601	rBV	155	258	0.05%	0.006%
11	3.395	634	639	642	rBB	165	174	0.03%	0.004%
12	3.491	666	669	673	rBB	136	138	0.03%	0.003%
13	3.533	679	682	688	rBB	153	202	0.04%	0.005%
14	4.170	877	880	885	rBB	142	168	0.03%	0.004%
15	4.289	914	917	920	rBB	141	119	0.02%	0.003%
16	4.636	1011	1025	1050	rBV2	48448	128707	25.47%	3.196%
17	4.803	1074	1077	1080	rVB	168	118	0.02%	0.003%
18	4.842	1087	1089	1091	rBV	232	155	0.03%	0.004%
19	4.854	1091	1093	1097	rVB2	241	168	0.03%	0.004%
20	5.006	1138	1140	1144	rBV	126	134	0.03%	0.003%
21	5.067	1144	1159	1179	rVV	94752	203627	40.29%	5.057%
22	5.160	1185	1188	1191	rBV2	154	123	0.02%	0.003%
23	5.292	1226	1229	1231	rBV	267	197	0.04%	0.005%
24	5.343	1242	1245	1248	rVV2	199	160	0.03%	0.004%
25	5.385	1254	1258	1261	rBB	286	217	0.04%	0.005%
26	5.729	1344	1365	1389	rBV2	186389	505347	100.00%	12.549%
27	5.809	1389	1390	1394	rVV2	444	313	0.06%	0.008%
28	5.829	1394	1396	1402	rVB	326	300	0.06%	0.007%
29	6.070	1469	1471	1475	rBB	140	120	0.02%	0.003%
30	6.250	1514	1527	1550	rBV	176377	327932	64.89%	8.143%
31	6.533	1610	1615	1619	rBB3	619	555	0.11%	0.014%
32	6.694	1652	1665	1683	rBV	117983	226085	44.74%	5.614%
33	6.809	1697	1701	1702	rBB	215	120	0.02%	0.003%
34	7.047	1772	1775	1777	rVB2	254	144	0.03%	0.004%
35	7.182	1813	1817	1821	rBV	342	308	0.06%	0.008%
36	7.234	1830	1833	1836	rBB	149	123	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046447.D
 Acq On : 17 Dec 2021 01:55
 Operator : SY/MD
 Sample : M5121-01 20X
 Misc : 4.41g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL50

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	7.568	1925	1937	1956	rBB	59931	103548	20.49%	2.571%
38	7.687	1971	1974	1976	rBV	249	194	0.04%	0.005%
39	7.700	1976	1978	1981	rVB2	266	132	0.03%	0.003%
40	7.726	1981	1986	1988	rBB	139	139	0.03%	0.003%
41	7.787	1999	2005	2009	rBV2	527	760	0.15%	0.019%
42	7.899	2025	2040	2056	rBV	222366	378999	75.00%	9.412%
43	7.973	2059	2063	2072	rVV5	2995	4054	0.80%	0.101%
44	8.182	2117	2128	2144	rBV	42002	70471	13.95%	1.750%
45	8.288	2158	2161	2165	rBB	136	135	0.03%	0.003%
46	8.484	2213	2222	2225	rBV2	533	901	0.18%	0.022%
47	8.526	2232	2235	2238	rBV2	374	242	0.05%	0.006%
48	8.636	2257	2269	2291	rBV	154251	257140	50.88%	6.385%
49	8.835	2328	2331	2334	rBB	154	129	0.03%	0.003%
50	8.919	2349	2357	2366	rBB3	1318	2050	0.41%	0.051%
51	8.960	2366	2370	2375	rBB	173	214	0.04%	0.005%
52	8.989	2375	2379	2382	rBB	171	158	0.03%	0.004%
53	9.047	2394	2397	2400	rBV	136	139	0.03%	0.003%
54	9.198	2440	2444	2447	rBV	146	190	0.04%	0.005%
55	9.365	2494	2496	2499	rBV	170	133	0.03%	0.003%
56	9.420	2500	2513	2534	rVV	254780	418934	82.90%	10.403%
57	9.497	2534	2537	2540	rVB	281	218	0.04%	0.005%
58	9.661	2583	2588	2591	rBV	143	176	0.03%	0.004%
59	9.783	2623	2626	2628	rBV	152	127	0.03%	0.003%
60	9.938	2671	2674	2680	rBV	206	265	0.05%	0.007%
61	9.992	2688	2691	2693	rBV	130	119	0.02%	0.003%
62	10.031	2700	2703	2706	rBV	170	170	0.03%	0.004%
63	10.308	2782	2789	2790	rBV	138	172	0.03%	0.004%
64	10.359	2801	2805	2807	rBV	140	144	0.03%	0.004%
65	10.558	2861	2867	2871	rBB	141	218	0.04%	0.005%
66	10.671	2896	2902	2910	rBV2	492	646	0.13%	0.016%
67	10.758	2917	2929	2945	rVB	172382	271634	53.75%	6.745%
68	10.841	2952	2955	2958	rBV	169	173	0.03%	0.004%
69	10.902	2966	2974	2981	rVB	278	516	0.10%	0.013%
70	10.963	2990	2993	2996	rVB	204	154	0.03%	0.004%
71	10.983	2996	2999	3003	rBB	177	166	0.03%	0.004%
72	11.131	3041	3045	3048	rBV	161	188	0.04%	0.005%
73	11.150	3048	3051	3055	rVB	123	118	0.02%	0.003%
74	11.279	3086	3091	3094	rBV	157	203	0.04%	0.005%
75	11.324	3102	3105	3107	rBV	173	148	0.03%	0.004%
76	11.433	3136	3139	3141	rBV	173	142	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046447.D
 Acq On : 17 Dec 2021 01:55
 Operator : SY/MD
 Sample : M5121-01 20X
 Misc : 4.41g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL50

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.465	3141	3149	3153	rVV3	459	683	0.14%	0.017%
78	11.703	3220	3223	3226	rBV	159	138	0.03%	0.003%
79	11.812	3244	3257	3274	rBV	268640	418274	82.77%	10.387%
80	11.967	3301	3305	3308	rBV2	277	317	0.06%	0.008%
81	12.195	3363	3376	3392	rVB	227734	360952	71.43%	8.963%
82	12.774	3551	3556	3563	rVB2	574	761	0.15%	0.019%
83	13.172	3673	3680	3685	rBV	159	232	0.05%	0.006%
84	13.899	3903	3906	3910	rBV	144	128	0.03%	0.003%
85	14.092	3963	3966	3969	rBV	181	125	0.02%	0.003%
86	14.577	4109	4117	4124	rBV2	556	856	0.17%	0.021%
87	15.397	4369	4372	4374	rBV2	263	171	0.03%	0.004%
88	15.462	4390	4392	4398	rVB2	246	205	0.04%	0.005%
89	15.504	4402	4405	4411	rVB2	195	159	0.03%	0.004%
90	15.532	4411	4414	4416	rBV	210	146	0.03%	0.004%
91	15.674	4453	4458	4460	rBV2	179	178	0.04%	0.004%
92	15.786	4491	4493	4497	rBV	171	147	0.03%	0.004%
93	15.960	4542	4547	4552	rBV2	223	270	0.05%	0.007%
94	16.188	4616	4618	4620	rBV	225	125	0.02%	0.003%
95	16.455	4699	4701	4707	rBV2	267	238	0.05%	0.006%
96	16.503	4713	4716	4719	rBV	255	217	0.04%	0.005%
97	16.825	4814	4816	4818	rBV	333	130	0.03%	0.003%
98	16.867	4821	4829	4832	rBV3	333	482	0.10%	0.012%
99	16.886	4832	4835	4839	rBV2	366	289	0.06%	0.007%
100	17.384	4987	4990	4997	rBV4	532	639	0.13%	0.016%




Sum of corrected areas: 4026963

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046447.D
Acq On : 17 Dec 2021 01:55
Operator : SY/MD
Sample : M5121-01 20X
Misc : 4.41g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

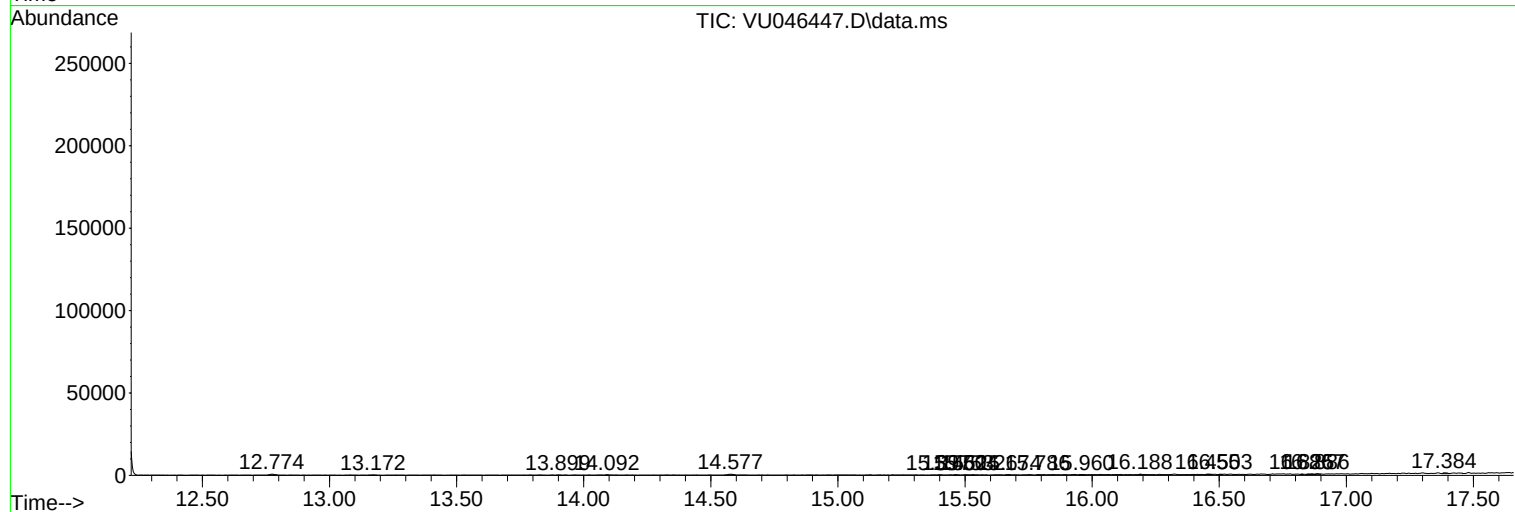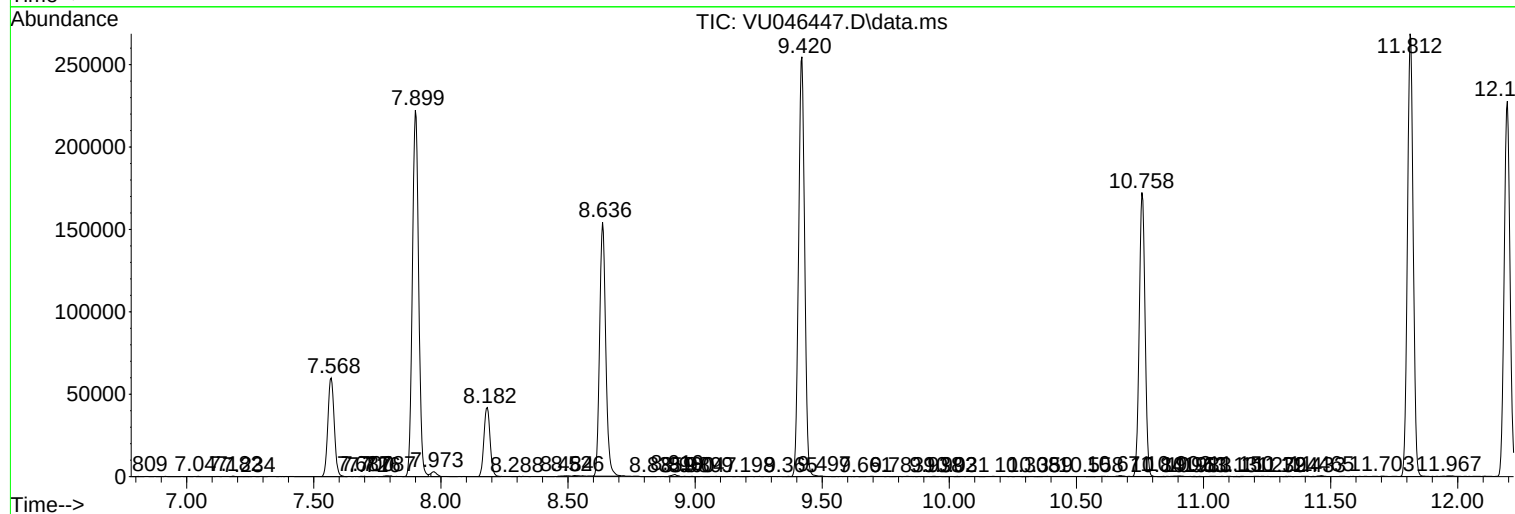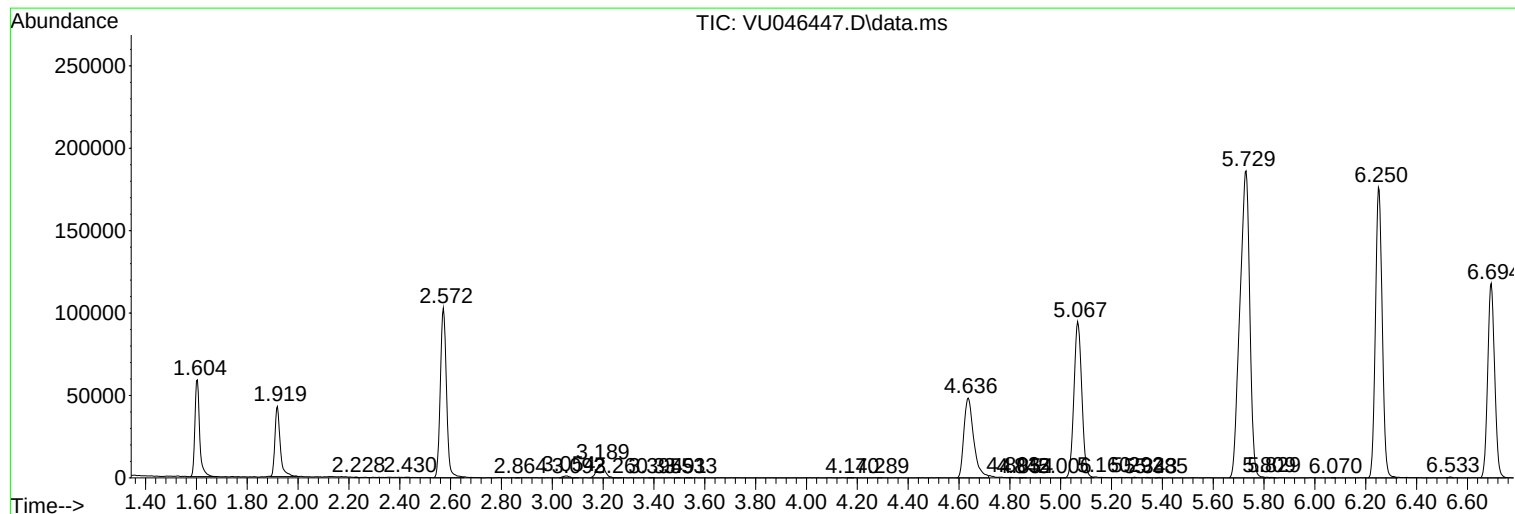

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046447.D
Acq On : 17 Dec 2021 01:55
Operator : SY/MD
Sample : M5121-01 20X
Misc : 4.41g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046447.D
Acq On : 17 Dec 2021 01:55
Operator : SY/MD
Sample : M5121-01 20X
Misc : 4.41g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc