

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046451.D
 Acq On : 17 Dec 2021 03:26
 Operator : SY/MD
 Sample : M5121-05 20X
 Misc : 6.79g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL55

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046451.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	100	rBV	59794	75878	14.96%	1.837%
2	1.919	171	180	201	rBV	43827	61664	12.15%	1.493%
3	2.572	372	383	403	rBV	106187	175585	34.61%	4.250%
4	2.797	449	453	454	rBV	143	120	0.02%	0.003%
5	2.900	483	485	487	rBV	231	132	0.03%	0.003%
6	2.938	494	497	501	rBV	153	171	0.03%	0.004%
7	2.970	505	507	510	rBV	140	118	0.02%	0.003%
8	3.054	526	533	541	rBB2	978	1622	0.32%	0.039%
9	3.192	562	576	590	rBB	7168	15988	3.15%	0.387%
10	3.343	621	623	627	rBB	154	125	0.02%	0.003%
11	3.665	720	723	725	rBV	141	126	0.02%	0.003%
12	3.954	809	813	816	rBV	151	172	0.03%	0.004%
13	4.633	1010	1024	1054	rBV	48963	125537	24.74%	3.039%
14	5.067	1144	1159	1179	rBV	93194	202942	40.00%	4.913%
15	5.237	1209	1212	1214	rVB2	275	176	0.03%	0.004%
16	5.276	1221	1224	1227	rBV	171	174	0.03%	0.004%
17	5.292	1227	1229	1232	rVV	303	224	0.04%	0.005%
18	5.308	1232	1234	1236	rVV	258	167	0.03%	0.004%
19	5.324	1237	1239	1241	rVV	268	156	0.03%	0.004%
20	5.346	1244	1246	1249	rVB	252	122	0.02%	0.003%
21	5.729	1344	1365	1387	rBV2	189090	507358	100.00%	12.282%
22	6.253	1513	1528	1553	rBV	175768	331306	65.30%	8.020%
23	6.533	1609	1615	1619	rBB2	538	575	0.11%	0.014%
24	6.694	1652	1665	1685	rBV2	117193	227583	44.86%	5.509%
25	7.031	1768	1770	1773	rBV	156	133	0.03%	0.003%
26	7.189	1812	1819	1825	rBB2	306	486	0.10%	0.012%
27	7.250	1835	1838	1841	rBB	149	122	0.02%	0.003%
28	7.456	1897	1902	1905	rBV	132	164	0.03%	0.004%
29	7.568	1924	1937	1956	rBV	61092	105795	20.85%	2.561%
30	7.652	1960	1963	1966	rBV	210	150	0.03%	0.004%
31	7.690	1973	1975	1979	rVB2	425	281	0.06%	0.007%
32	7.787	2000	2005	2008	rBV2	492	598	0.12%	0.014%
33	7.899	2027	2040	2056	rBV	233427	395649	77.98%	9.578%
34	8.182	2116	2128	2143	rBV	41862	70654	13.93%	1.710%
35	8.269	2152	2155	2159	rVB	272	236	0.05%	0.006%
36	8.301	2163	2165	2167	rBV	251	164	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046451.D
 Acq On : 17 Dec 2021 03:26
 Operator : SY/MD
 Sample : M5121-05 20X
 Misc : 6.79g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL55

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	8.481	2213	2221	2225	rBV2	508	869	0.17%	0.021%
38	8.636	2257	2269	2291	rBV	148289	249435	49.16%	6.038%
39	8.915	2348	2356	2363	rBV3	947	1448	0.29%	0.035%
40	8.986	2374	2378	2381	rBV	153	186	0.04%	0.005%
41	9.115	2414	2418	2420	rBV	145	145	0.03%	0.004%
42	9.156	2426	2431	2434	rBV	161	212	0.04%	0.005%
43	9.420	2498	2513	2531	rBV	268683	436658	86.07%	10.570%
44	9.546	2549	2552	2556	rBB	150	131	0.03%	0.003%
45	9.571	2557	2560	2564	rBV2	262	259	0.05%	0.006%
46	9.613	2571	2573	2577	rBB	153	123	0.02%	0.003%
47	9.674	2589	2592	2594	rBV	145	120	0.02%	0.003%
48	9.693	2594	2598	2600	rBV	265	249	0.05%	0.006%
49	9.726	2605	2608	2612	rVB2	242	200	0.04%	0.005%
50	9.774	2618	2623	2624	rBV	176	175	0.03%	0.004%
51	10.034	2702	2704	2707	rVV	230	130	0.03%	0.003%
52	10.076	2713	2717	2719	rBV	147	118	0.02%	0.003%
53	10.195	2751	2754	2758	rBV	138	163	0.03%	0.004%
54	10.250	2768	2771	2773	rBV	250	129	0.03%	0.003%
55	10.337	2794	2798	2801	rBV	180	200	0.04%	0.005%
56	10.359	2801	2805	2808	rVB	492	422	0.08%	0.010%
57	10.439	2828	2830	2833	rBV	162	143	0.03%	0.003%
58	10.523	2852	2856	2858	rBV	147	148	0.03%	0.004%
59	10.584	2872	2875	2877	rBV	192	153	0.03%	0.004%
60	10.645	2890	2894	2896	rBV	156	157	0.03%	0.004%
61	10.671	2896	2902	2912	rVB5	1244	1687	0.33%	0.041%
62	10.758	2917	2929	2942	rBV	168949	270741	53.36%	6.554%
63	10.873	2962	2965	2968	rVV	277	208	0.04%	0.005%
64	10.896	2968	2972	2980	rVV2	410	642	0.13%	0.016%
65	11.057	3019	3022	3024	rBV	269	210	0.04%	0.005%
66	11.127	3042	3044	3046	rVB2	270	124	0.02%	0.003%
67	11.224	3068	3074	3076	rBV	182	232	0.05%	0.006%
68	11.314	3099	3102	3105	rBV	450	343	0.07%	0.008%
69	11.378	3118	3122	3126	rVV3	586	549	0.11%	0.013%
70	11.417	3129	3134	3139	rVV3	1023	1362	0.27%	0.033%
71	11.459	3139	3147	3157	rVB5	1528	2752	0.54%	0.067%
72	11.536	3169	3171	3174	rBV	179	140	0.03%	0.003%
73	11.574	3177	3183	3188	rBV3	554	647	0.13%	0.016%
74	11.635	3200	3202	3205	rVB2	286	145	0.03%	0.004%
75	11.700	3215	3222	3227	rBV5	1177	1596	0.31%	0.039%
76	11.812	3245	3257	3272	rBV	296276	458903	90.45%	11.109%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046451.D
 Acq On : 17 Dec 2021 03:26
 Operator : SY/MD
 Sample : M5121-05 20X
 Misc : 6.79g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL55

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.941	3293	3297	3301	rBV	924	881	0.17%	0.021%
78	12.118	3348	3352	3356	rBV	328	319	0.06%	0.008%
79	12.195	3361	3376	3389	rBV	240191	387146	76.31%	9.372%
80	12.327	3411	3417	3418	rBV2	931	741	0.15%	0.018%
81	12.401	3432	3440	3450	rVB4	479	854	0.17%	0.021%
82	12.462	3456	3459	3462	rBV2	170	135	0.03%	0.003%
83	12.481	3462	3465	3470	rVB4	426	391	0.08%	0.009%
84	12.513	3470	3475	3476	rBV2	439	348	0.07%	0.008%
85	12.526	3476	3479	3482	rBV3	422	315	0.06%	0.008%
86	12.590	3496	3499	3501	rBV2	347	222	0.04%	0.005%
87	12.893	3591	3593	3595	rBV	280	133	0.03%	0.003%
88	12.941	3604	3608	3610	rVV2	542	352	0.07%	0.009%
89	12.979	3617	3620	3624	rBV	308	175	0.03%	0.004%
90	13.105	3656	3659	3662	rBV	302	169	0.03%	0.004%
91	13.590	3802	3810	3815	rVV4	1028	1410	0.28%	0.034%
92	13.655	3828	3830	3832	rBV4	372	188	0.04%	0.005%
93	13.899	3904	3906	3910	rVB2	221	122	0.02%	0.003%
94	14.574	4112	4116	4117	rBV	970	653	0.13%	0.016%
95	14.623	4129	4131	4134	rVB2	255	125	0.02%	0.003%
96	14.680	4144	4149	4152	rBV2	318	338	0.07%	0.008%
97	14.828	4192	4195	4197	rBV	321	214	0.04%	0.005%
98	14.864	4203	4206	4207	rBV2	222	128	0.03%	0.003%
99	15.095	4275	4278	4280	rBV	206	140	0.03%	0.003%
100	15.208	4309	4313	4315	rBV3	988	782	0.15%	0.019%




Sum of corrected areas: 4130988

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046451.D
Acq On : 17 Dec 2021 03:26
Operator : SY/MD
Sample : M5121-05 20X
Misc : 6.79g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

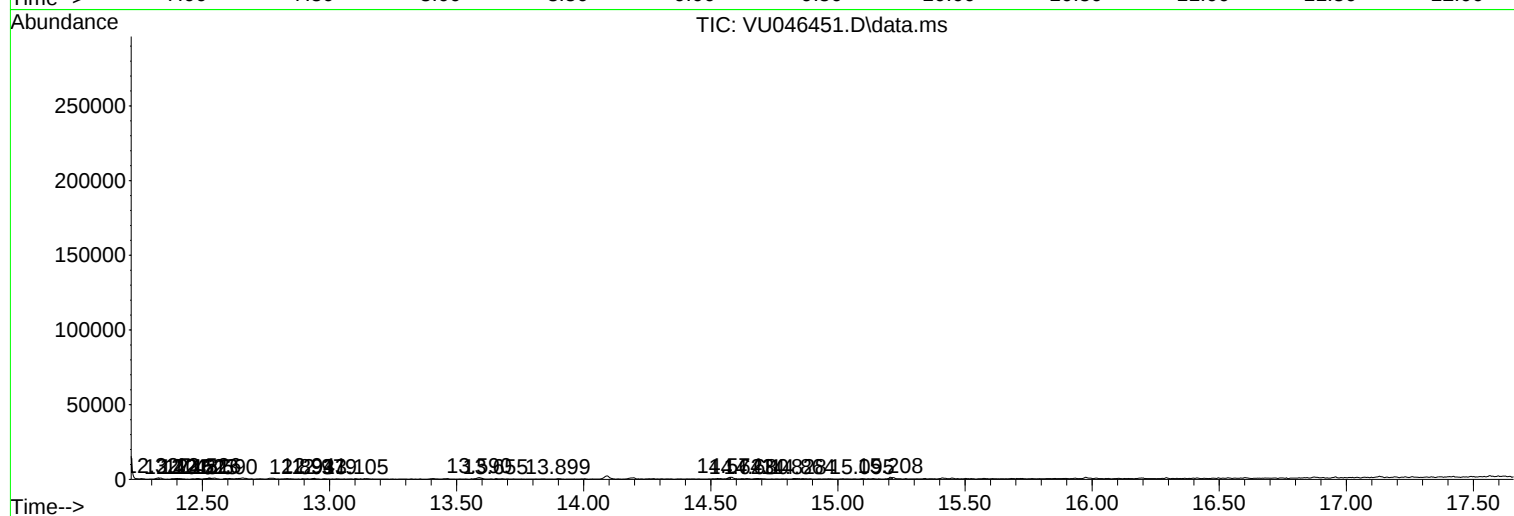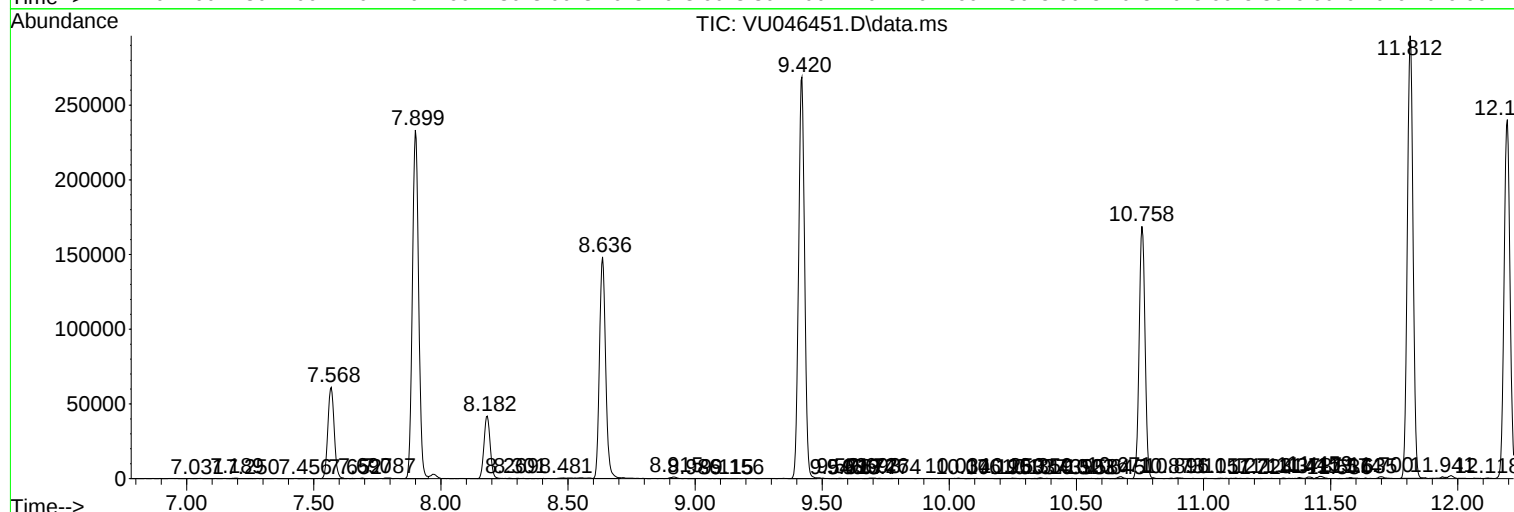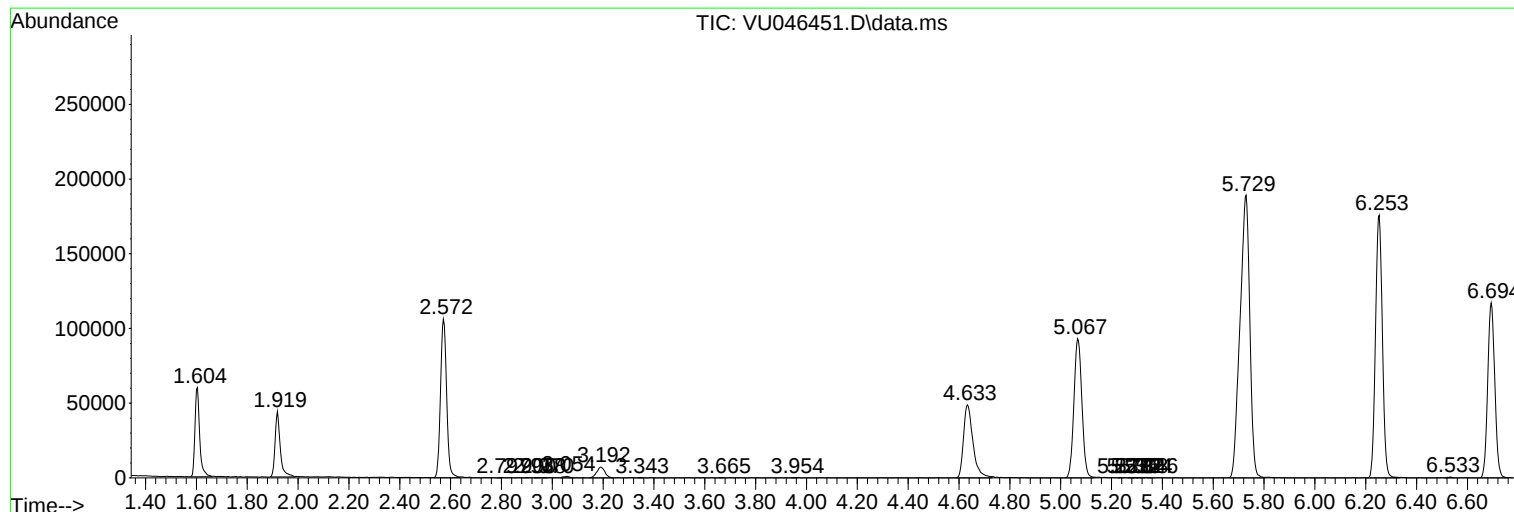

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046451.D
Acq On : 17 Dec 2021 03:26
Operator : SY/MD
Sample : M5121-05 20X
Misc : 6.79g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046451.D
Acq On : 17 Dec 2021 03:26
Operator : SY/MD
Sample : M5121-05 20X
Misc : 6.79g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------