

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046452.D
 Acq On : 17 Dec 2021 03:48
 Operator : SY/MD
 Sample : M5121-07 20X
 Misc : 5.76g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL59

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046452.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	104	rBV	60928	77684	14.93%	1.859%
2	1.919	171	180	202	rBV	43354	62889	12.09%	1.505%
3	2.260	283	286	288	rVB	254	125	0.02%	0.003%
4	2.453	342	346	352	rVV2	251	240	0.05%	0.006%
5	2.572	370	383	405	rBV	107312	178489	34.30%	4.270%
6	2.822	457	461	463	rVB	188	151	0.03%	0.004%
7	2.845	464	468	471	rBB	160	131	0.03%	0.003%
8	2.919	487	491	495	rBB	157	188	0.04%	0.004%
9	2.964	500	505	510	rBV	186	269	0.05%	0.006%
10	3.054	527	533	540	rBV2	939	1451	0.28%	0.035%
11	3.141	557	560	562	rBV	155	129	0.02%	0.003%
12	3.189	562	575	592	rVB2	7352	16833	3.23%	0.403%
13	4.224	893	897	901	rBB	148	172	0.03%	0.004%
14	4.636	1009	1025	1050	rBV	47534	129347	24.86%	3.095%
15	4.838	1086	1088	1090	rVV2	235	139	0.03%	0.003%
16	4.854	1090	1093	1096	rVB	241	177	0.03%	0.004%
17	5.067	1142	1159	1181	rBV	95878	207428	39.86%	4.963%
18	5.192	1195	1198	1201	rBV	259	193	0.04%	0.005%
19	5.218	1203	1206	1208	rVB2	370	220	0.04%	0.005%
20	5.237	1208	1212	1214	rBV	159	161	0.03%	0.004%
21	5.253	1216	1217	1220	rVB	269	124	0.02%	0.003%
22	5.269	1220	1222	1225	rBV	219	129	0.02%	0.003%
23	5.729	1344	1365	1388	rBV2	193333	520364	100.00%	12.450%
24	6.253	1512	1528	1552	rBV	179089	335160	64.41%	8.019%
25	6.340	1552	1555	1561	rVB2	202	200	0.04%	0.005%
26	6.533	1609	1615	1618	rBV2	630	556	0.11%	0.013%
27	6.694	1650	1665	1685	rBV	121823	232293	44.64%	5.558%
28	7.179	1812	1816	1817	rBV	316	195	0.04%	0.005%
29	7.350	1866	1869	1873	rBB	169	159	0.03%	0.004%
30	7.443	1895	1898	1901	rBB	152	122	0.02%	0.003%
31	7.568	1925	1937	1955	rBV	61979	107034	20.57%	2.561%
32	7.684	1971	1973	1974	rBV	258	121	0.02%	0.003%
33	7.700	1974	1978	1983	rVB2	262	338	0.06%	0.008%
34	7.726	1983	1986	1989	rBV	129	136	0.03%	0.003%
35	7.790	2001	2006	2013	rBB3	708	923	0.18%	0.022%
36	7.899	2027	2040	2054	rBV	238711	406196	78.06%	9.718%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046452.D
 Acq On : 17 Dec 2021 03:48
 Operator : SY/MD
 Sample : M5121-07 20X
 Misc : 5.76g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL59

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	7.970	2057	2062	2073	rVV2	2953	5004	0.96%	0.120%
38	8.018	2075	2077	2079	rVV	232	132	0.03%	0.003%
39	8.179	2117	2127	2143	rBV	44443	72307	13.90%	1.730%
40	8.237	2143	2145	2148	rVV	257	209	0.04%	0.005%
41	8.253	2148	2150	2155	rVV	298	259	0.05%	0.006%
42	8.285	2155	2160	2164	rVB	265	327	0.06%	0.008%
43	8.321	2168	2171	2174	rVV2	229	195	0.04%	0.005%
44	8.340	2175	2177	2181	rVB	260	170	0.03%	0.004%
45	8.436	2204	2207	2210	rBB	141	119	0.02%	0.003%
46	8.475	2214	2219	2222	rBV	382	447	0.09%	0.011%
47	8.562	2243	2246	2248	rVB2	256	145	0.03%	0.003%
48	8.575	2248	2250	2254	rVB2	219	143	0.03%	0.003%
49	8.636	2257	2269	2290	rBV	154367	257778	49.54%	6.167%
50	8.819	2323	2326	2328	rBV	254	174	0.03%	0.004%
51	8.915	2347	2356	2364	rBB3	964	1617	0.31%	0.039%
52	8.957	2364	2369	2371	rBV	144	175	0.03%	0.004%
53	9.028	2388	2391	2396	rBB	142	174	0.03%	0.004%
54	9.186	2437	2440	2442	rBV	152	129	0.02%	0.003%
55	9.362	2491	2495	2499	rBV	156	197	0.04%	0.005%
56	9.417	2499	2512	2528	rBV	265916	436721	83.93%	10.449%
57	9.616	2571	2574	2578	rBB	149	152	0.03%	0.004%
58	9.655	2582	2586	2589	rBB	145	146	0.03%	0.003%
59	9.687	2592	2596	2600	rBV2	256	281	0.05%	0.007%
60	9.854	2645	2648	2650	rBV	135	121	0.02%	0.003%
61	9.999	2689	2693	2695	rBV	144	148	0.03%	0.004%
62	10.073	2714	2716	2719	rBV	141	121	0.02%	0.003%
63	10.237	2765	2767	2770	rBV	157	128	0.02%	0.003%
64	10.340	2796	2799	2803	rBB	144	141	0.03%	0.003%
65	10.411	2818	2821	2827	rBB	187	220	0.04%	0.005%
66	10.472	2837	2840	2845	rBV	170	199	0.04%	0.005%
67	10.578	2869	2873	2875	rBV	145	123	0.02%	0.003%
68	10.626	2884	2888	2890	rBV	135	142	0.03%	0.003%
69	10.671	2895	2902	2911	rVB3	747	1113	0.21%	0.027%
70	10.758	2917	2929	2944	rVV	174013	275468	52.94%	6.591%
71	10.893	2967	2971	2972	rBV2	255	171	0.03%	0.004%
72	10.903	2972	2974	2980	rVB	367	390	0.07%	0.009%
73	10.983	2994	2999	3003	rBV	206	264	0.05%	0.006%
74	11.054	3018	3021	3023	rBV	145	125	0.02%	0.003%
75	11.179	3055	3060	3063	rBV	160	177	0.03%	0.004%
76	11.205	3066	3068	3073	rBV	173	204	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046452.D
 Acq On : 17 Dec 2021 03:48
 Operator : SY/MD
 Sample : M5121-07 20X
 Misc : 5.76g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL59

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.417	3128	3134	3138	rBV	189	299	0.06%	0.007%
78	11.446	3141	3143	3144	rBV	309	134	0.03%	0.003%
79	11.661	3207	3210	3213	rVB	217	174	0.03%	0.004%
80	11.700	3218	3222	3226	rVV2	337	306	0.06%	0.007%
81	11.812	3245	3257	3277	rVB	287225	449319	86.35%	10.750%
82	11.944	3290	3298	3301	rVB2	230	278	0.05%	0.007%
83	11.970	3301	3306	3312	rVB3	662	791	0.15%	0.019%
84	12.002	3312	3316	3318	rBV	203	203	0.04%	0.005%
85	12.105	3345	3348	3350	rBV	166	138	0.03%	0.003%
86	12.131	3353	3356	3360	rVV	222	211	0.04%	0.005%
87	12.153	3360	3363	3364	rVV	240	157	0.03%	0.004%
88	12.195	3364	3376	3393	rVB	244872	386765	74.33%	9.253%
89	12.636	3510	3513	3516	rVB	210	122	0.02%	0.003%
90	12.771	3549	3555	3562	rVB3	646	977	0.19%	0.023%
91	14.484	4085	4088	4096	rVB	135	138	0.03%	0.003%
92	14.578	4110	4117	4127	rVB3	897	1473	0.28%	0.035%
93	15.304	4341	4343	4347	rVB	223	155	0.03%	0.004%
94	15.378	4362	4366	4369	rBV2	203	194	0.04%	0.005%
95	15.642	4445	4448	4452	rBV2	181	183	0.04%	0.004%
96	15.770	4485	4488	4490	rBV	212	175	0.03%	0.004%
97	15.835	4505	4508	4509	rBV	212	128	0.02%	0.003%
98	15.861	4513	4516	4519	rBV2	218	196	0.04%	0.005%
99	17.031	4878	4880	4883	rBV2	384	211	0.04%	0.005%
100	17.259	4949	4951	4953	rBV2	489	295	0.06%	0.007%




Sum of corrected areas: 4179744

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046452.D
Acq On : 17 Dec 2021 03:48
Operator : SY/MD
Sample : M5121-07 20X
Misc : 5.76g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

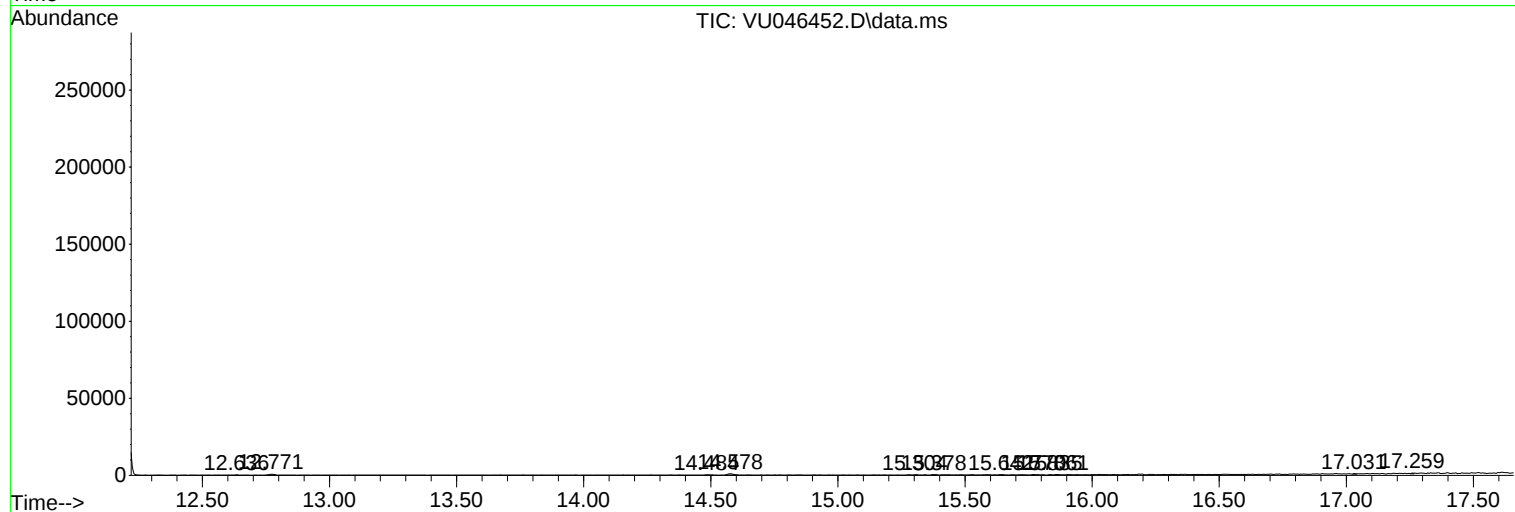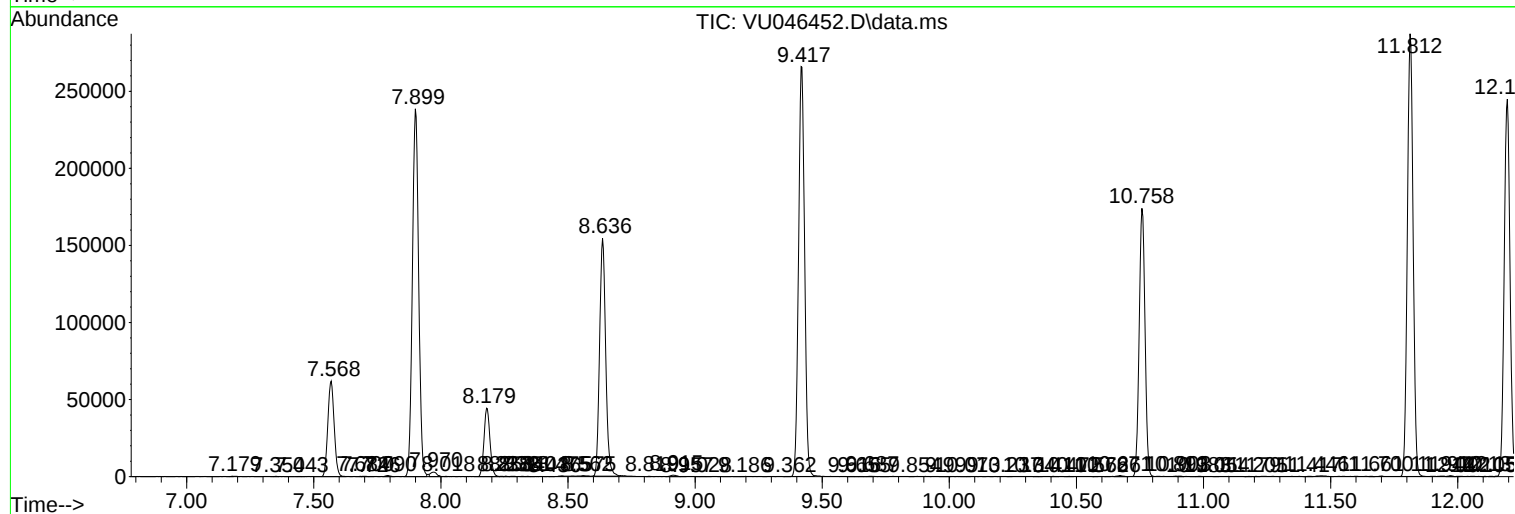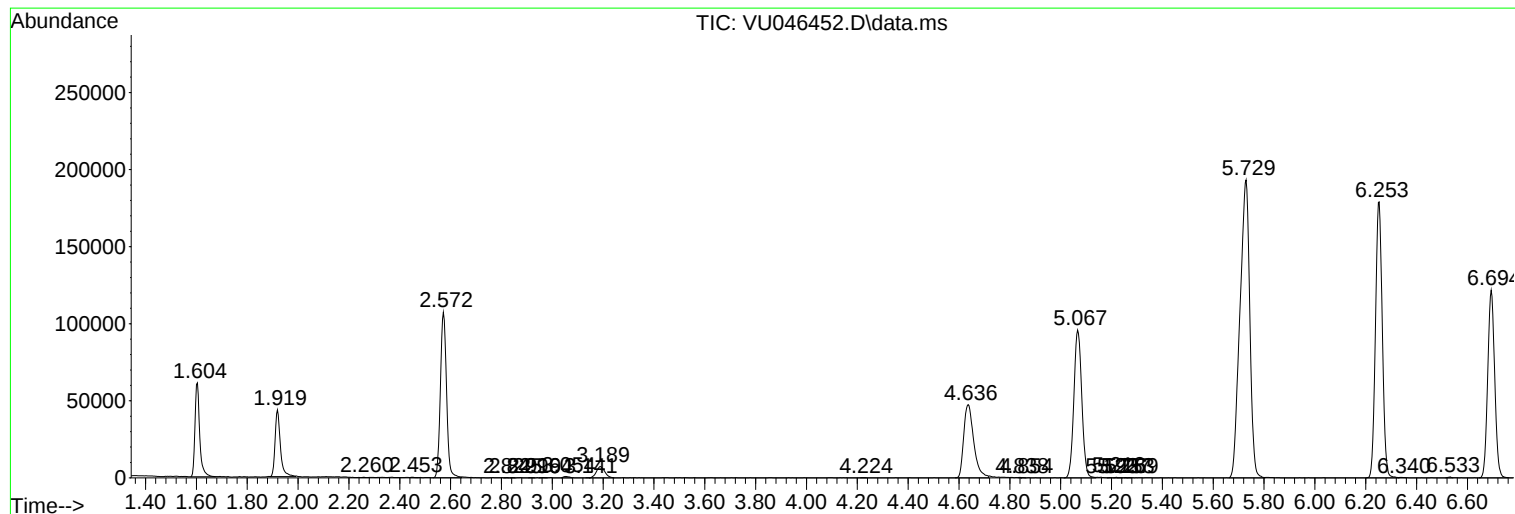

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046452.D
Acq On : 17 Dec 2021 03:48
Operator : SY/MD
Sample : M5121-07 20X
Misc : 5.76g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046452.D
Acq On : 17 Dec 2021 03:48
Operator : SY/MD
Sample : M5121-07 20X
Misc : 5.76g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc