

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046455.D
 Acq On : 17 Dec 2021 04:56
 Operator : SY/MD
 Sample : M5121-10 20X
 Misc : 5.77g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL57

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046455.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	105	rVB	60484	76444	14.54%	1.793%
2	1.919	171	180	200	rBV	42915	62824	11.95%	1.474%
3	2.392	325	327	331	rVB	232	131	0.02%	0.003%
4	2.572	371	383	401	rBV	111642	182963	34.80%	4.292%
5	2.729	429	432	436	rBV	142	173	0.03%	0.004%
6	2.774	440	446	449	rBB	148	174	0.03%	0.004%
7	2.794	449	452	454	rBV	127	112	0.02%	0.003%
8	2.874	475	477	479	rBV	150	98	0.02%	0.002%
9	2.903	483	486	488	rBB	138	96	0.02%	0.002%
10	2.961	501	504	508	rVB	265	206	0.04%	0.005%
11	3.022	519	523	526	rBB	146	149	0.03%	0.003%
12	3.054	527	533	540	rBV4	951	1370	0.26%	0.032%
13	3.189	562	575	591	rBV2	9373	20663	3.93%	0.485%
14	3.334	617	620	624	rBB	139	147	0.03%	0.003%
15	3.356	624	627	630	rBV	123	129	0.02%	0.003%
16	3.398	638	640	643	rBB	135	95	0.02%	0.002%
17	3.427	644	649	651	rBB	139	119	0.02%	0.003%
18	3.745	746	748	751	rBB	144	99	0.02%	0.002%
19	3.884	788	791	794	rBB	124	109	0.02%	0.003%
20	4.636	1010	1025	1054	rVV	49665	132041	25.12%	3.097%
21	4.794	1073	1074	1079	rVB2	383	254	0.05%	0.006%
22	4.819	1080	1082	1084	rBB2	216	103	0.02%	0.002%
23	5.067	1143	1159	1181	rBV	96198	209072	39.77%	4.904%
24	5.186	1194	1196	1200	rVB	255	164	0.03%	0.004%
25	5.247	1212	1215	1219	rBV	275	162	0.03%	0.004%
26	5.363	1247	1251	1252	rBV	248	162	0.03%	0.004%
27	5.729	1341	1365	1385	rBV2	195878	525688	100.00%	12.331%
28	6.250	1513	1527	1543	rBV	184777	345263	65.68%	8.098%
29	6.530	1611	1614	1617	rBB3	538	399	0.08%	0.009%
30	6.694	1651	1665	1685	rBB	121827	233193	44.36%	5.470%
31	6.810	1698	1701	1706	rBB2	250	247	0.05%	0.006%
32	6.883	1722	1724	1726	rBV	148	102	0.02%	0.002%
33	7.047	1773	1775	1778	rVB2	270	154	0.03%	0.004%
34	7.465	1901	1905	1907	rBB	126	110	0.02%	0.003%
35	7.520	1920	1922	1925	rBB	138	96	0.02%	0.002%
36	7.568	1925	1937	1953	rBV2	61630	107702	20.49%	2.526%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046455.D
 Acq On : 17 Dec 2021 04:56
 Operator : SY/MD
 Sample : M5121-10 20X
 Misc : 5.77g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL57

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	7.636	1956	1958	1961	rVB	236	130	0.02%	0.003%
38	7.687	1971	1974	1977	rBB2	289	202	0.04%	0.005%
39	7.745	1989	1992	1995	rBV	154	147	0.03%	0.003%
40	7.797	1999	2008	2012	rBV2	605	791	0.15%	0.019%
41	7.900	2025	2040	2055	rBV	242541	413401	78.64%	9.697%
42	8.086	2095	2098	2101	rBB	147	119	0.02%	0.003%
43	8.182	2117	2128	2141	rBV	43605	73087	13.90%	1.714%
44	8.285	2158	2160	2162	rBV	238	130	0.02%	0.003%
45	8.398	2190	2195	2200	rBB	153	217	0.04%	0.005%
46	8.475	2213	2219	2220	rBV	497	387	0.07%	0.009%
47	8.636	2257	2269	2291	rBV	152529	257181	48.92%	6.032%
48	8.912	2348	2355	2364	rVV	977	1671	0.32%	0.039%
49	8.983	2372	2377	2378	rBV	150	130	0.02%	0.003%
50	9.035	2387	2393	2395	rBV	150	204	0.04%	0.005%
51	9.118	2416	2419	2422	rBB	127	114	0.02%	0.003%
52	9.141	2423	2426	2429	rBB	157	134	0.03%	0.003%
53	9.295	2471	2474	2479	rBV	138	177	0.03%	0.004%
54	9.346	2485	2490	2493	rBB	148	175	0.03%	0.004%
55	9.372	2494	2498	2500	rBV	150	154	0.03%	0.004%
56	9.417	2500	2512	2530	rBV	270115	446724	84.98%	10.478%
57	9.571	2555	2560	2562	rBV	140	142	0.03%	0.003%
58	9.639	2579	2581	2587	rBB	135	163	0.03%	0.004%
59	9.690	2595	2597	2600	rBV	427	308	0.06%	0.007%
60	9.752	2614	2616	2621	rBV	133	159	0.03%	0.004%
61	9.816	2632	2636	2640	rBV	135	188	0.04%	0.004%
62	9.877	2653	2655	2657	rBV	133	95	0.02%	0.002%
63	9.941	2673	2675	2677	rBV	139	97	0.02%	0.002%
64	10.067	2711	2714	2717	rBV	155	162	0.03%	0.004%
65	10.128	2730	2733	2735	rBV	167	130	0.02%	0.003%
66	10.237	2764	2767	2771	rBB	197	175	0.03%	0.004%
67	10.327	2792	2795	2798	rBV	147	158	0.03%	0.004%
68	10.398	2814	2817	2819	rBV	168	134	0.03%	0.003%
69	10.517	2852	2854	2858	rBV	152	169	0.03%	0.004%
70	10.671	2897	2902	2909	rBV3	1048	1350	0.26%	0.032%
71	10.758	2917	2929	2944	rBV	177015	277655	52.82%	6.513%
72	10.887	2966	2969	2970	rBV	189	104	0.02%	0.002%
73	10.970	2990	2995	2997	rBV	153	181	0.03%	0.004%
74	11.009	3003	3007	3009	rBV	144	153	0.03%	0.004%
75	11.192	3058	3064	3068	rBB	172	242	0.05%	0.006%
76	11.211	3068	3070	3072	rBV	138	98	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046455.D
 Acq On : 17 Dec 2021 04:56
 Operator : SY/MD
 Sample : M5121-10 20X
 Misc : 5.77g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL57

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.269	3083	3088	3092	rBV	184	260	0.05%	0.006%
78	11.321	3101	3104	3106	rBV	171	139	0.03%	0.003%
79	11.417	3128	3134	3138	rBV2	527	498	0.09%	0.012%
80	11.459	3138	3147	3150	rBV2	890	1175	0.22%	0.028%
81	11.533	3166	3170	3173	rBV	188	195	0.04%	0.005%
82	11.703	3217	3223	3232	rVB3	794	827	0.16%	0.019%
83	11.813	3244	3257	3273	rBV	304846	470974	89.59%	11.047%
84	12.115	3350	3351	3355	rVB	219	99	0.02%	0.002%
85	12.195	3361	3376	3392	rVB	251534	398200	75.75%	9.340%
86	12.288	3402	3405	3408	rBV	183	186	0.04%	0.004%
87	12.333	3417	3419	3421	rBV2	257	138	0.03%	0.003%
88	12.391	3434	3437	3438	rBV2	260	133	0.03%	0.003%
89	12.520	3475	3477	3479	rBV	214	152	0.03%	0.004%
90	12.607	3501	3504	3505	rBV	460	213	0.04%	0.005%
91	12.665	3518	3522	3531	rVB3	678	814	0.15%	0.019%
92	12.774	3550	3556	3564	rBV2	644	973	0.19%	0.023%
93	13.591	3803	3810	3818	rBV5	1089	1708	0.32%	0.040%
94	14.089	3960	3965	3975	rVB3	2127	3100	0.59%	0.073%
95	14.195	3990	3998	4003	rBV4	1183	1696	0.32%	0.040%
96	15.205	4308	4312	4313	rBV	1263	755	0.14%	0.018%
97	15.414	4369	4377	4384	rVB2	1315	2081	0.40%	0.049%
98	15.446	4384	4387	4389	rBV2	403	265	0.05%	0.006%
99	15.626	4440	4443	4447	rBV3	443	344	0.07%	0.008%
100	15.710	4465	4469	4471	rBV2	335	222	0.04%	0.005%




Sum of corrected areas: 4263298

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046455.D
Acq On : 17 Dec 2021 04:56
Operator : SY/MD
Sample : M5121-10 20X
Misc : 5.77g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL57

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

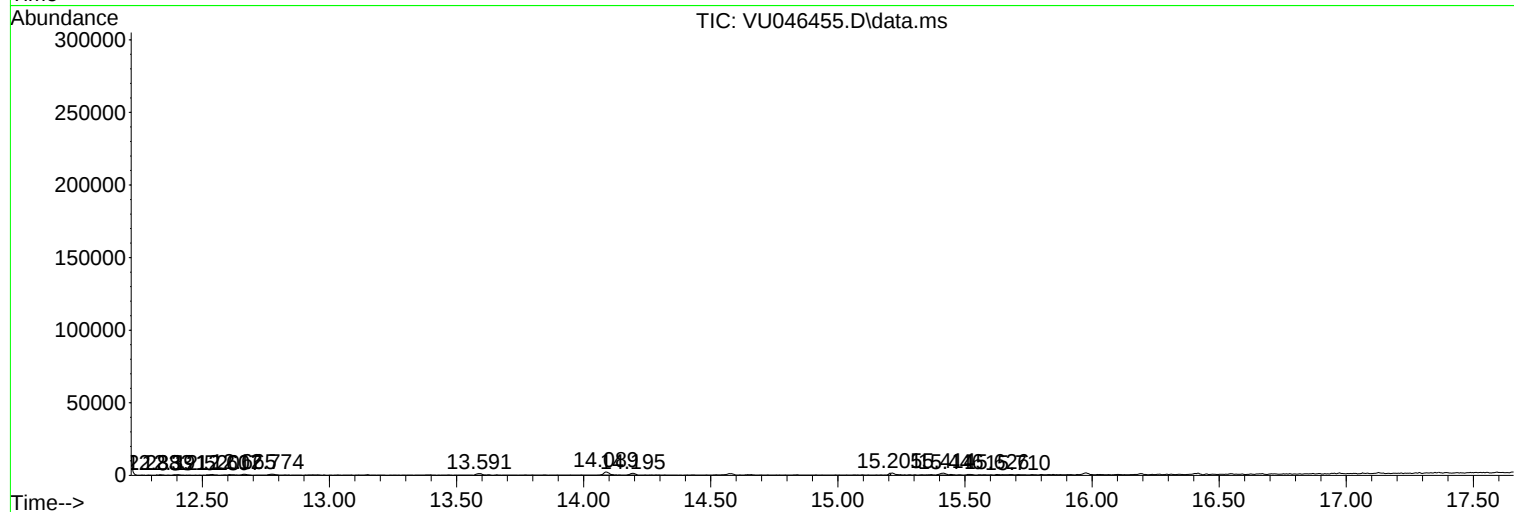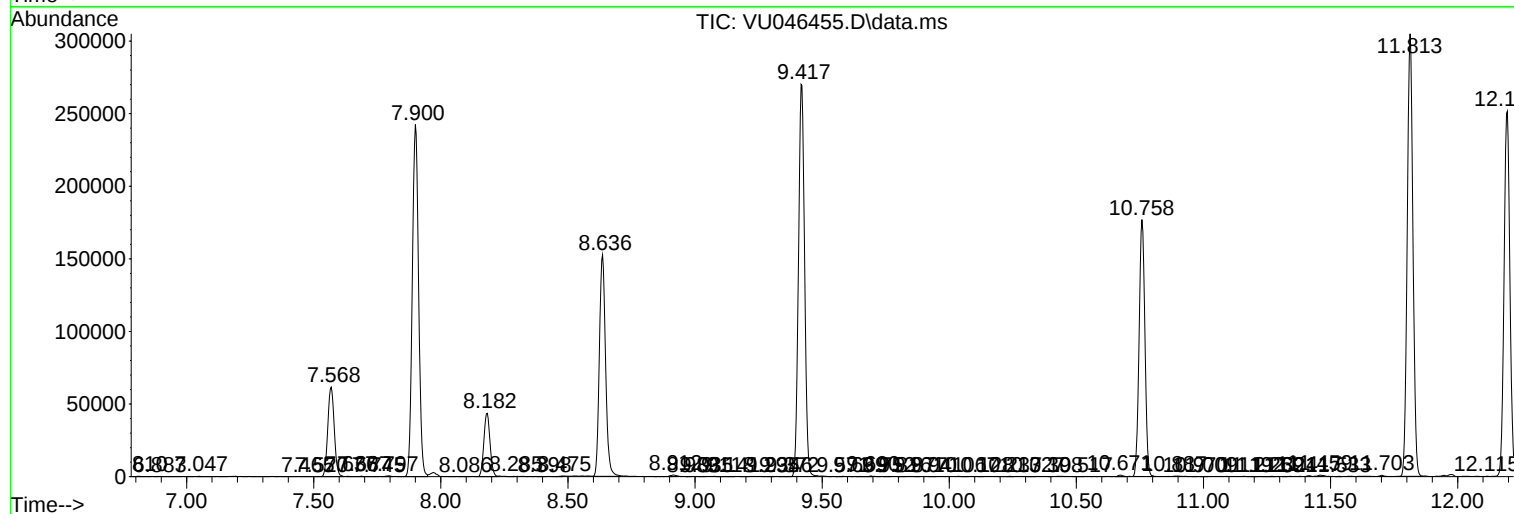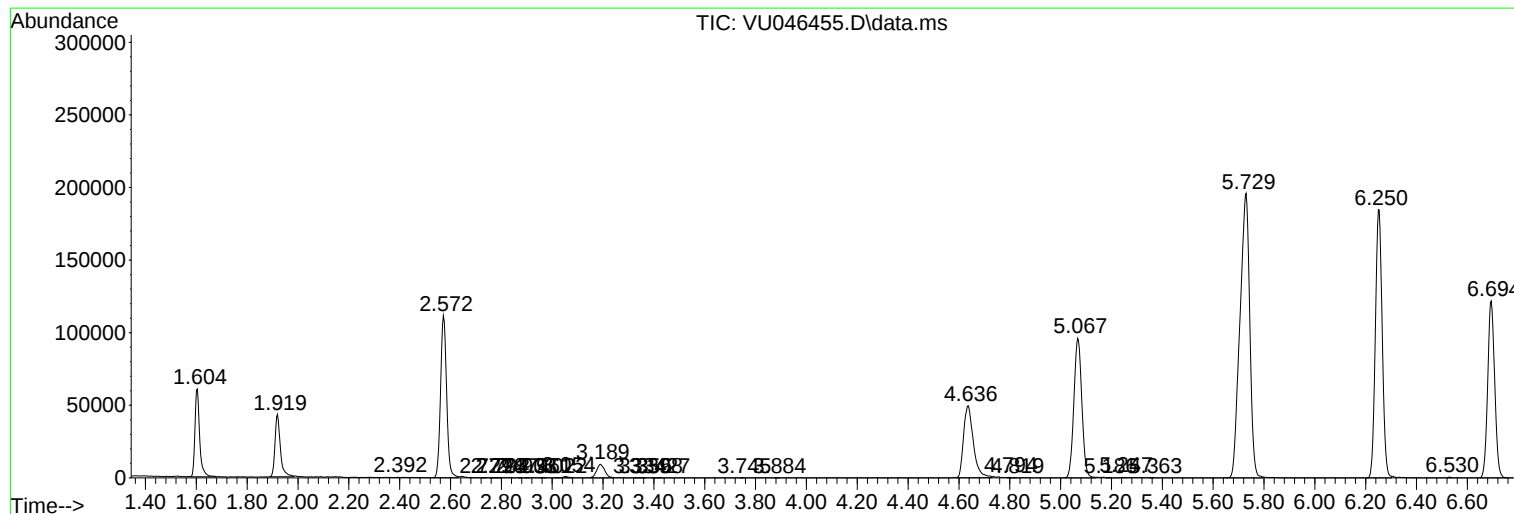

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046455.D
Acq On : 17 Dec 2021 04:56
Operator : SY/MD
Sample : M5121-10 20X
Misc : 5.77g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL57

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046455.D
Acq On : 17 Dec 2021 04:56
Operator : SY/MD
Sample : M5121-10 20X
Misc : 5.77g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL57

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc