

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046457.D
 Acq On : 17 Dec 2021 05:41
 Operator : SY/MD
 Sample : M5121-12 20X
 Misc : 6.35g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL60

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046457.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	73	82	105	rVB	61209	77032	14.31%	1.794%
2	1.919	171	180	198	rBV	43747	62536	11.62%	1.456%
3	2.202	264	268	273	rVB2	251	203	0.04%	0.005%
4	2.247	278	282	287	rVB2	184	127	0.02%	0.003%
5	2.276	288	291	297	rVB2	254	207	0.04%	0.005%
6	2.572	371	383	403	rBV	110861	182319	33.88%	4.246%
7	2.765	438	443	446	rBV	140	189	0.04%	0.004%
8	3.054	526	533	534	rBV3	900	1004	0.19%	0.023%
9	3.189	563	575	590	rBB	4733	10128	1.88%	0.236%
10	3.260	595	597	600	rBV	137	121	0.02%	0.003%
11	3.369	629	631	635	rVB	149	126	0.02%	0.003%
12	3.552	685	688	691	rBB	132	119	0.02%	0.003%
13	3.678	725	727	731	rBB	151	129	0.02%	0.003%
14	4.002	825	828	831	rBB	138	117	0.02%	0.003%
15	4.369	939	942	943	rBV	171	118	0.02%	0.003%
16	4.633	1011	1024	1053	rBV	49327	127839	23.75%	2.977%
17	4.787	1069	1072	1075	rVB2	211	145	0.03%	0.003%
18	4.912	1108	1111	1114	rBB	151	125	0.02%	0.003%
19	5.067	1142	1159	1180	rBV	97643	210713	39.15%	4.907%
20	5.292	1225	1229	1234	rBV	278	279	0.05%	0.006%
21	5.337	1239	1243	1246	rVB2	230	192	0.04%	0.004%
22	5.465	1280	1283	1285	rBV	131	116	0.02%	0.003%
23	5.729	1343	1365	1399	rBV2	197507	538196	100.00%	12.533%
24	6.250	1514	1527	1552	rBV	185967	347529	64.57%	8.093%
25	6.465	1591	1594	1597	rBV	157	147	0.03%	0.003%
26	6.485	1597	1600	1603	rVB	158	137	0.03%	0.003%
27	6.533	1613	1615	1618	rVB2	418	304	0.06%	0.007%
28	6.694	1648	1665	1687	rBB	121358	235594	43.77%	5.486%
29	6.890	1723	1726	1729	rBB	155	131	0.02%	0.003%
30	7.044	1771	1774	1776	rVB2	301	183	0.03%	0.004%
31	7.189	1813	1819	1822	rBV	349	376	0.07%	0.009%
32	7.372	1873	1876	1879	rBB	157	125	0.02%	0.003%
33	7.568	1924	1937	1955	rBV	66012	110788	20.59%	2.580%
34	7.729	1984	1987	1990	rVB	185	146	0.03%	0.003%
35	7.790	2001	2006	2010	rBB	439	431	0.08%	0.010%
36	7.899	2025	2040	2055	rBV	246898	419230	77.90%	9.763%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046457.D
 Acq On : 17 Dec 2021 05:41
 Operator : SY/MD
 Sample : M5121-12 20X
 Misc : 6.35g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL60

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	7.973	2058	2063	2073	rVB4	3127	4746	0.88%	0.111%
38	8.099	2100	2102	2105	rBV	130	121	0.02%	0.003%
39	8.182	2116	2128	2145	rBV	44315	73589	13.67%	1.714%
40	8.266	2151	2154	2157	rBV2	240	179	0.03%	0.004%
41	8.301	2161	2165	2169	rBB2	261	230	0.04%	0.005%
42	8.353	2176	2181	2185	rBB2	214	157	0.03%	0.004%
43	8.378	2186	2189	2192	rBB	145	120	0.02%	0.003%
44	8.436	2205	2207	2210	rBV	135	117	0.02%	0.003%
45	8.475	2213	2219	2224	rVV2	389	535	0.10%	0.012%
46	8.523	2231	2234	2238	rVV2	243	287	0.05%	0.007%
47	8.636	2256	2269	2287	rBV	155262	257997	47.94%	6.008%
48	8.816	2322	2325	2328	rVB	165	137	0.03%	0.003%
49	8.845	2331	2334	2336	rBV	161	132	0.02%	0.003%
50	8.915	2349	2356	2364	rBB2	1068	1521	0.28%	0.035%
51	8.983	2373	2377	2380	rBV	159	175	0.03%	0.004%
52	9.311	2476	2479	2484	rBV	151	198	0.04%	0.005%
53	9.417	2498	2512	2531	rBV	273608	453720	84.30%	10.566%
54	9.481	2531	2532	2538	rVB2	398	371	0.07%	0.009%
55	9.767	2615	2621	2624	rBB	186	221	0.04%	0.005%
56	9.851	2643	2647	2648	rBV	154	130	0.02%	0.003%
57	9.886	2655	2658	2660	rBV	143	129	0.02%	0.003%
58	9.935	2670	2673	2676	rBV	148	149	0.03%	0.003%
59	10.089	2718	2721	2724	rBV	157	149	0.03%	0.003%
60	10.147	2735	2739	2745	rBV	200	284	0.05%	0.007%
61	10.218	2759	2761	2765	rBV	161	168	0.03%	0.004%
62	10.626	2884	2888	2892	rBV	178	221	0.04%	0.005%
63	10.674	2896	2903	2909	rVB4	1378	1784	0.33%	0.042%
64	10.703	2909	2912	2915	rBV	179	171	0.03%	0.004%
65	10.758	2916	2929	2945	rVB	175158	277386	51.54%	6.460%
66	10.835	2950	2953	2955	rBV	145	123	0.02%	0.003%
67	10.864	2958	2962	2965	rVV	176	157	0.03%	0.004%
68	10.896	2968	2972	2980	rVB	384	489	0.09%	0.011%
69	11.256	3080	3084	3092	rBV	173	353	0.07%	0.008%
70	11.456	3139	3146	3156	rVB4	1029	1551	0.29%	0.036%
71	11.578	3180	3184	3190	rVB	335	372	0.07%	0.009%
72	11.697	3215	3221	3227	rVB3	676	722	0.13%	0.017%
73	11.812	3245	3257	3274	rVV	311571	476414	88.52%	11.094%
74	11.944	3291	3298	3301	rBV2	594	795	0.15%	0.019%
75	11.970	3302	3306	3308	rBV4	726	599	0.11%	0.014%
76	12.018	3317	3321	3325	rBV	159	211	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046457.D
 Acq On : 17 Dec 2021 05:41
 Operator : SY/MD
 Sample : M5121-12 20X
 Misc : 6.35g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL60

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	12.105	3343	3348	3353	rBV	244	172	0.03%	0.004%
78	12.195	3363	3376	3391	rBV	253693	401015	74.51%	9.339%
79	12.501	3468	3471	3477	rBV	99	116	0.02%	0.003%
80	12.642	3511	3515	3519	rVB	227	202	0.04%	0.005%
81	12.777	3549	3557	3562	rVB3	714	1086	0.20%	0.025%
82	13.584	3803	3808	3812	rBV2	228	219	0.04%	0.005%
83	14.095	3960	3967	3974	rBV2	344	505	0.09%	0.012%
84	14.581	4108	4118	4125	rBV2	850	1366	0.25%	0.032%
85	15.317	4342	4347	4351	rVB2	248	205	0.04%	0.005%
86	15.340	4351	4354	4356	rBV	162	122	0.02%	0.003%
87	15.372	4360	4364	4371	rVB	261	263	0.05%	0.006%
88	15.443	4384	4386	4393	rBV2	279	297	0.06%	0.007%
89	15.523	4408	4411	4415	rBV2	137	119	0.02%	0.003%
90	15.571	4424	4426	4431	rVB2	206	121	0.02%	0.003%
91	15.597	4431	4434	4436	rBV	205	154	0.03%	0.004%
92	16.002	4557	4560	4561	rBV2	270	144	0.03%	0.003%
93	16.105	4590	4592	4596	rBV	213	175	0.03%	0.004%
94	16.198	4615	4621	4626	rVB6	903	837	0.16%	0.019%
95	16.291	4645	4650	4653	rBV3	387	332	0.06%	0.008%
96	16.333	4661	4663	4668	rVB2	239	128	0.02%	0.003%
97	16.532	4723	4725	4733	rVB8	1028	1091	0.20%	0.025%
98	16.664	4762	4766	4771	rBV7	711	624	0.12%	0.015%
99	16.905	4839	4841	4843	rBV3	453	223	0.04%	0.005%
100	17.529	5033	5035	5039	rBV4	836	532	0.10%	0.012%




Sum of corrected areas: 4294159

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046457.D
Acq On : 17 Dec 2021 05:41
Operator : SY/MD
Sample : M5121-12 20X
Misc : 6.35g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL60

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

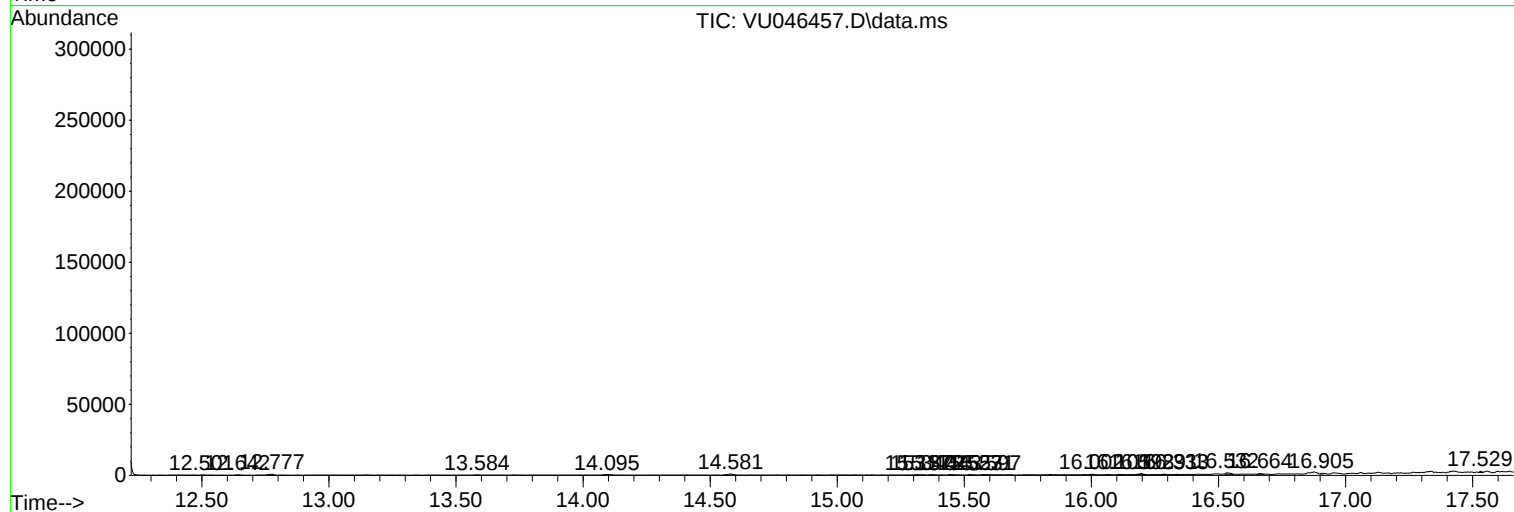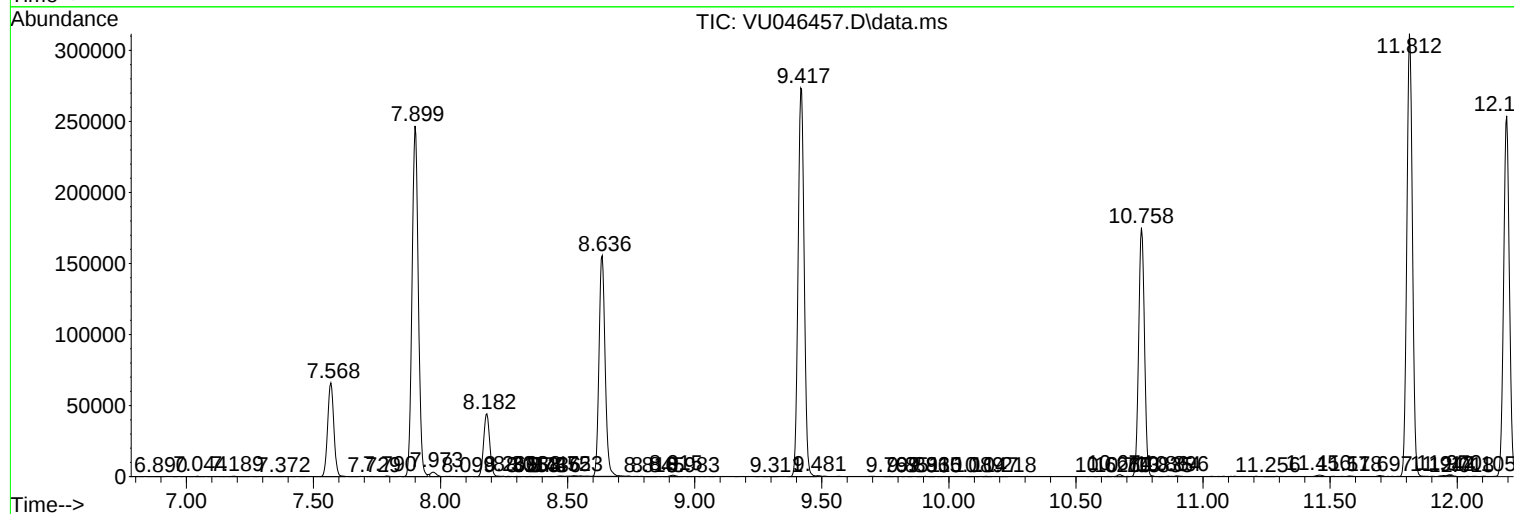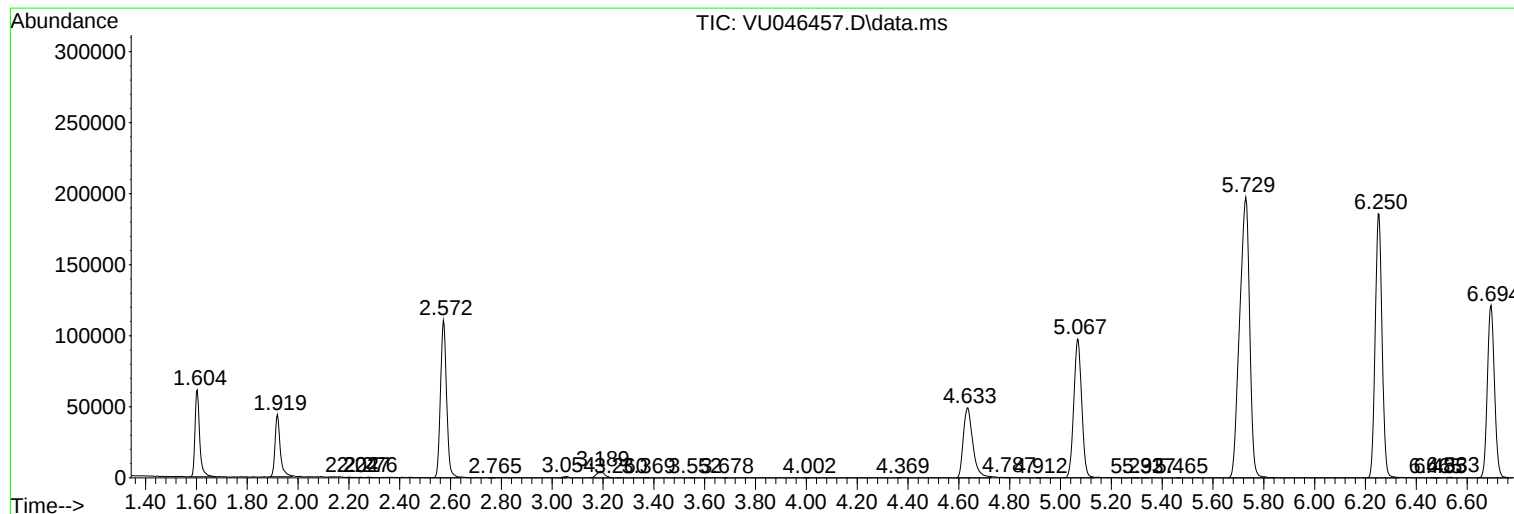

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046457.D
Acq On : 17 Dec 2021 05:41
Operator : SY/MD
Sample : M5121-12 20X
Misc : 6.35g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL60

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046457.D
Acq On : 17 Dec 2021 05:41
Operator : SY/MD
Sample : M5121-12 20X
Misc : 6.35g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL60

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc