

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046458.D
 Acq On : 17 Dec 2021 06:04
 Operator : SY/MD
 Sample : M5121-14 20X
 Misc : 4.91g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL64

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M

Title : VOC Analysis

Signal : TIC: VU046458.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	101	rBV	53995	67338	13.90%	1.766%
2	1.919	171	180	197	rBV	40424	58252	12.02%	1.528%
3	2.572	372	383	405	rBV	93639	154476	31.88%	4.052%
4	2.793	448	452	454	rBV	179	171	0.04%	0.004%
5	3.051	526	532	542	rBB3	1260	1917	0.40%	0.050%
6	3.137	555	559	563	rBV	196	229	0.05%	0.006%
7	3.189	563	575	592	rVB	9842	22509	4.65%	0.590%
8	3.472	659	663	668	rBB	147	164	0.03%	0.004%
9	3.620	706	709	712	rBB	140	120	0.02%	0.003%
10	3.742	745	747	751	rBB	139	119	0.02%	0.003%
11	4.134	867	869	873	rBB	129	112	0.02%	0.003%
12	4.401	947	952	955	rBB	129	138	0.03%	0.004%
13	4.636	1010	1025	1051	rBV2	50329	134852	27.83%	3.537%
14	4.787	1070	1072	1077	rVB2	278	210	0.04%	0.006%
15	4.874	1096	1099	1101	rBV	144	122	0.03%	0.003%
16	5.067	1144	1159	1180	rBV	90650	195631	40.37%	5.131%
17	5.137	1180	1181	1185	rVB	472	176	0.04%	0.005%
18	5.295	1228	1230	1233	rVV2	379	256	0.05%	0.007%
19	5.314	1233	1236	1242	rVB2	285	316	0.07%	0.008%
20	5.729	1344	1365	1388	rBV2	176590	484581	100.00%	12.710%
21	5.845	1400	1401	1405	rVB2	262	140	0.03%	0.004%
22	6.250	1513	1527	1551	rBV	160735	301419	62.20%	7.906%
23	6.424	1578	1581	1584	rBB	124	111	0.02%	0.003%
24	6.536	1611	1616	1619	rBB2	356	302	0.06%	0.008%
25	6.694	1651	1665	1684	rBB	115242	219537	45.30%	5.758%
26	7.189	1811	1819	1824	rBB2	378	598	0.12%	0.016%
27	7.507	1915	1918	1922	rBB	131	134	0.03%	0.004%
28	7.568	1925	1937	1949	rBV	58216	99860	20.61%	2.619%
29	7.684	1970	1973	1977	rBV2	227	186	0.04%	0.005%
30	7.787	1998	2005	2006	rBV	834	777	0.16%	0.020%
31	7.899	2026	2040	2055	rBV	204899	350616	72.35%	9.196%
32	8.182	2117	2128	2143	rBV	40507	68584	14.15%	1.799%
33	8.250	2147	2149	2152	rBB	236	138	0.03%	0.004%
34	8.279	2153	2158	2159	rBV2	231	173	0.04%	0.005%
35	8.308	2164	2167	2169	rBV2	251	203	0.04%	0.005%
36	8.446	2207	2210	2212	rBV	130	110	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046458.D
 Acq On : 17 Dec 2021 06:04
 Operator : SY/MD
 Sample : M5121-14 20X
 Misc : 4.91g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL64

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	8.468	2212	2217	2218	rBV	227	199	0.04%	0.005%
38	8.481	2218	2221	2225	rVV2	323	258	0.05%	0.007%
39	8.578	2249	2251	2256	rVB2	246	186	0.04%	0.005%
40	8.636	2256	2269	2292	rBV	151794	255865	52.80%	6.711%
41	8.777	2310	2313	2315	rBV2	240	144	0.03%	0.004%
42	8.806	2319	2322	2324	rBB	163	111	0.02%	0.003%
43	8.825	2325	2328	2332	rBB	173	159	0.03%	0.004%
44	8.915	2349	2356	2362	rBV4	2652	3900	0.80%	0.102%
45	8.973	2370	2374	2377	rBV	186	197	0.04%	0.005%
46	9.028	2387	2391	2395	rBB	157	155	0.03%	0.004%
47	9.054	2396	2399	2403	rBV	167	189	0.04%	0.005%
48	9.160	2426	2432	2437	rBV	147	275	0.06%	0.007%
49	9.240	2455	2457	2460	rBV	164	140	0.03%	0.004%
50	9.301	2471	2476	2480	rBB	150	151	0.03%	0.004%
51	9.420	2499	2513	2532	rBV	230441	378291	78.07%	9.922%
52	9.530	2544	2547	2550	rBB	155	129	0.03%	0.003%
53	9.562	2554	2557	2559	rBV	156	132	0.03%	0.003%
54	9.578	2559	2562	2565	rVB	185	149	0.03%	0.004%
55	9.623	2573	2576	2580	rBV	151	176	0.04%	0.005%
56	9.684	2592	2595	2596	rBV	168	115	0.02%	0.003%
57	9.719	2602	2606	2609	rBB	156	151	0.03%	0.004%
58	9.787	2625	2627	2632	rVB	152	146	0.03%	0.004%
59	9.829	2637	2640	2644	rBV	171	182	0.04%	0.005%
60	9.874	2650	2654	2657	rBV	154	153	0.03%	0.004%
61	9.938	2671	2674	2675	rBV	155	111	0.02%	0.003%
62	10.095	2719	2723	2726	rBB	144	143	0.03%	0.004%
63	10.118	2726	2730	2733	rBB	164	165	0.03%	0.004%
64	10.147	2734	2739	2742	rBB	156	154	0.03%	0.004%
65	10.182	2742	2750	2753	rBV	161	286	0.06%	0.008%
66	10.266	2773	2776	2778	rVB	186	121	0.02%	0.003%
67	10.292	2781	2784	2786	rBV	153	137	0.03%	0.004%
68	10.562	2864	2868	2875	rBV	160	284	0.06%	0.007%
69	10.674	2896	2903	2910	rVV3	645	898	0.19%	0.024%
70	10.706	2910	2913	2916	rVV	179	154	0.03%	0.004%
71	10.758	2917	2929	2945	rVB	168924	268461	55.40%	7.041%
72	10.822	2946	2949	2952	rBB	166	132	0.03%	0.003%
73	10.851	2955	2958	2960	rBV	191	151	0.03%	0.004%
74	10.890	2967	2970	2971	rBV	191	135	0.03%	0.004%
75	10.976	2992	2997	3003	rBV	195	334	0.07%	0.009%
76	11.246	3076	3081	3083	rBV	160	159	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046458.D
 Acq On : 17 Dec 2021 06:04
 Operator : SY/MD
 Sample : M5121-14 20X
 Misc : 4.91g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL64

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.291	3093	3095	3098	rVB2	270	153	0.03%	0.004%
78	11.317	3098	3103	3105	rBV	165	183	0.04%	0.005%
79	11.455	3135	3146	3147	rBV2	384	546	0.11%	0.014%
80	11.584	3182	3186	3189	rBV	179	203	0.04%	0.005%
81	11.690	3215	3219	3221	rBV	324	260	0.05%	0.007%
82	11.748	3233	3237	3243	rVB	159	128	0.03%	0.003%
83	11.812	3245	3257	3276	rVB	249582	387640	79.99%	10.167%
84	11.941	3294	3297	3300	rBV2	152	128	0.03%	0.003%
85	11.973	3304	3307	3316	rVB3	551	485	0.10%	0.013%
86	12.195	3364	3376	3392	rBV	215175	340389	70.24%	8.928%
87	12.774	3549	3556	3563	rVV2	548	837	0.17%	0.022%
88	13.214	3688	3693	3698	rBV	86	113	0.02%	0.003%
89	13.999	3931	3937	3942	rBV	166	202	0.04%	0.005%
90	14.578	4108	4117	4125	rVB2	869	1428	0.29%	0.037%
91	15.330	4347	4351	4353	rBV	181	159	0.03%	0.004%
92	15.410	4374	4376	4379	rVV2	237	141	0.03%	0.004%
93	15.433	4381	4383	4388	rVV2	229	196	0.04%	0.005%
94	15.455	4388	4390	4392	rVV2	232	132	0.03%	0.003%
95	15.478	4393	4397	4403	rVB2	205	208	0.04%	0.005%
96	15.578	4425	4428	4433	rBV2	208	247	0.05%	0.006%
97	15.764	4480	4486	4490	rBV2	251	360	0.07%	0.009%
98	16.584	4738	4741	4744	rBV2	319	196	0.04%	0.005%
99	16.848	4821	4823	4825	rBV	281	153	0.03%	0.004%
100	16.928	4845	4848	4850	rBV	432	237	0.05%	0.006%




Sum of corrected areas: 3812679

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046458.D
Acq On : 17 Dec 2021 06:04
Operator : SY/MD
Sample : M5121-14 20X
Misc : 4.91g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL64

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

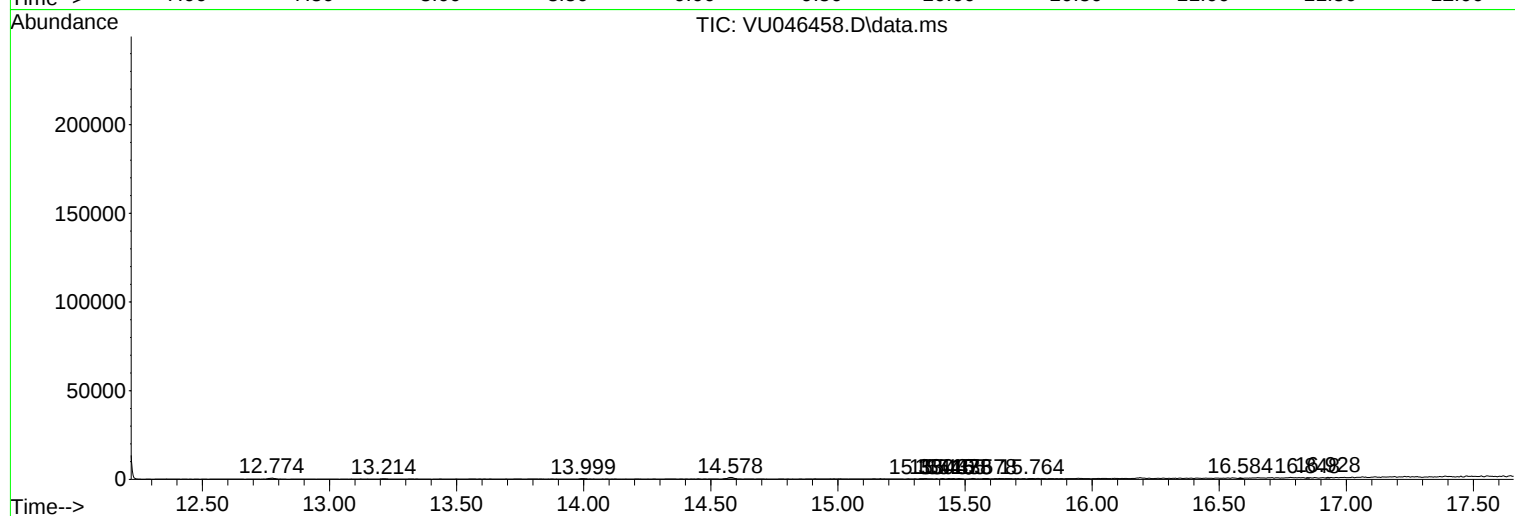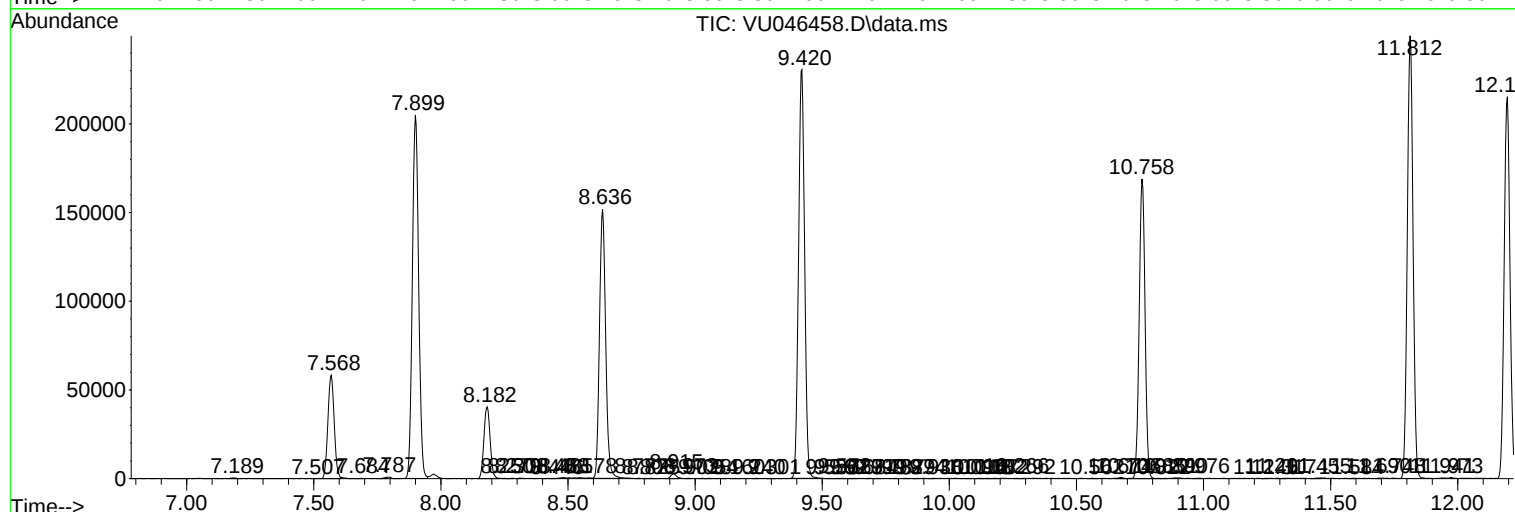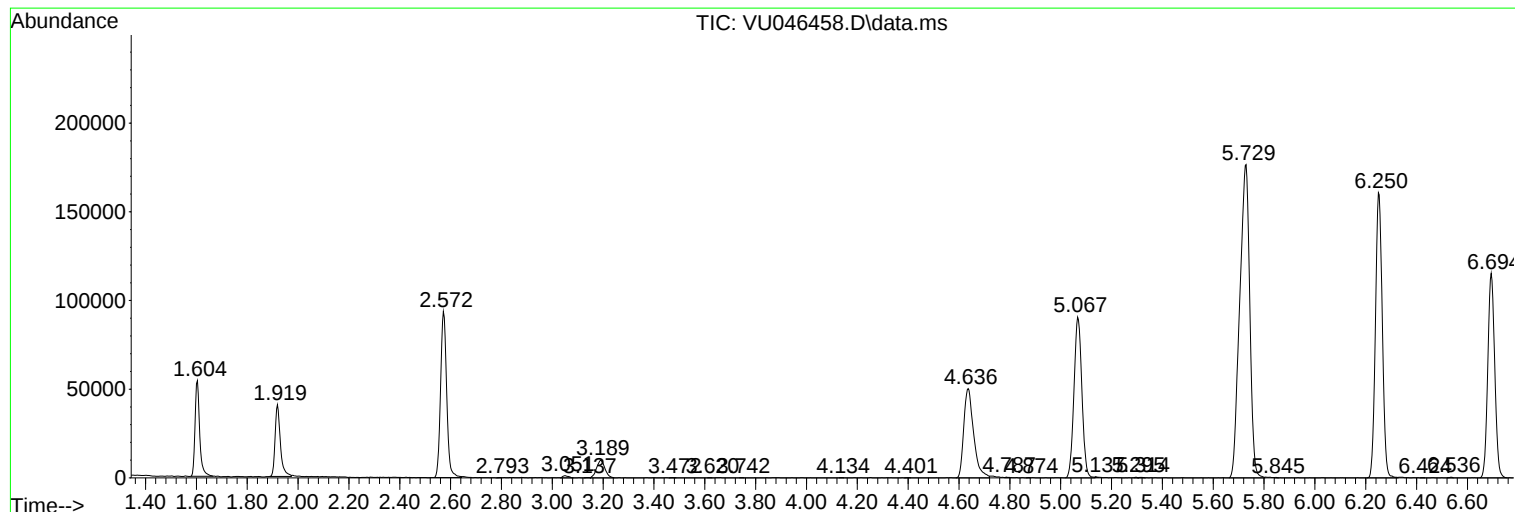

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046458.D
Acq On : 17 Dec 2021 06:04
Operator : SY/MD
Sample : M5121-14 20X
Misc : 4.91g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL64

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046458.D
Acq On : 17 Dec 2021 06:04
Operator : SY/MD
Sample : M5121-14 20X
Misc : 4.91g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL64

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------