

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046459.D
 Acq On : 17 Dec 2021 06:27
 Operator : SY/MD
 Sample : M5121-15 20X
 Misc : 7.20g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046459.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	103	rVB	59380	74066	14.21%	1.757%
2	1.919	172	180	197	rBV	43224	61499	11.80%	1.459%
3	2.571	371	383	401	rBV	106828	176133	33.80%	4.179%
4	2.777	444	447	450	rBV	121	132	0.03%	0.003%
5	2.854	467	471	474	rBV	158	176	0.03%	0.004%
6	2.983	506	511	515	rBB	129	136	0.03%	0.003%
7	3.054	524	533	540	rBB4	903	1538	0.30%	0.036%
8	3.086	540	543	546	rBB	134	117	0.02%	0.003%
9	3.192	561	576	593	rVV2	8711	18996	3.65%	0.451%
10	3.276	597	602	605	rBB	155	149	0.03%	0.004%
11	3.314	610	614	617	rBB	140	116	0.02%	0.003%
12	3.498	667	671	673	rBB	127	113	0.02%	0.003%
13	3.633	709	713	716	rBV	128	161	0.03%	0.004%
14	3.887	790	792	795	rBV	129	112	0.02%	0.003%
15	4.636	1010	1025	1051	rBV	51853	136640	26.22%	3.242%
16	4.774	1066	1068	1074	rVB2	215	150	0.03%	0.004%
17	4.803	1074	1077	1082	rVB2	264	214	0.04%	0.005%
18	4.825	1082	1084	1087	rVB	282	174	0.03%	0.004%
19	4.845	1088	1090	1092	rBV	244	135	0.03%	0.003%
20	5.067	1143	1159	1179	rBV	94985	205357	39.41%	4.872%
21	5.176	1191	1193	1196	rVB	397	216	0.04%	0.005%
22	5.205	1200	1202	1207	rBB	247	188	0.04%	0.004%
23	5.240	1210	1213	1215	rBB	229	112	0.02%	0.003%
24	5.253	1215	1217	1221	rBV	228	160	0.03%	0.004%
25	5.298	1224	1231	1234	rBV	343	385	0.07%	0.009%
26	5.430	1268	1272	1275	rBB	145	144	0.03%	0.003%
27	5.729	1344	1365	1394	rBV2	191327	521111	100.00%	12.364%
28	6.253	1514	1528	1550	rBV	177912	335750	64.43%	7.966%
29	6.375	1564	1566	1569	rVB2	248	143	0.03%	0.003%
30	6.526	1609	1613	1614	rBV2	490	298	0.06%	0.007%
31	6.694	1651	1665	1682	rBV	119038	228881	43.92%	5.431%
32	6.767	1685	1688	1691	rVB	331	196	0.04%	0.005%
33	7.144	1803	1805	1810	rBB	130	137	0.03%	0.003%
34	7.568	1923	1937	1953	rBV	61551	106820	20.50%	2.534%
35	7.722	1979	1985	1987	rBV	144	195	0.04%	0.005%
36	7.780	1998	2003	2004	rBV	559	437	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046459.D
 Acq On : 17 Dec 2021 06:27
 Operator : SY/MD
 Sample : M5121-15 20X
 Misc : 7.20g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	7.899	2027	2040	2056	rBV	236192	403239	77.38%	9.568%
38	8.182	2117	2128	2142	rBV	43078	71258	13.67%	1.691%
39	8.237	2142	2145	2150	rVB	336	304	0.06%	0.007%
40	8.301	2160	2165	2169	rBV2	240	218	0.04%	0.005%
41	8.417	2199	2201	2206	rBV	161	175	0.03%	0.004%
42	8.468	2210	2217	2218	rBV	248	248	0.05%	0.006%
43	8.526	2234	2235	2240	rBV	225	145	0.03%	0.003%
44	8.636	2257	2269	2294	rBV	157526	261653	50.21%	6.208%
45	8.832	2326	2330	2332	rBV	136	143	0.03%	0.003%
46	8.867	2338	2341	2347	rBV	194	248	0.05%	0.006%
47	8.912	2348	2355	2364	rVB3	1778	2716	0.52%	0.064%
48	8.992	2376	2380	2383	rBB	146	146	0.03%	0.003%
49	9.031	2388	2392	2394	rBV	150	153	0.03%	0.004%
50	9.108	2414	2416	2419	rBV	130	115	0.02%	0.003%
51	9.214	2446	2449	2451	rBV	143	119	0.02%	0.003%
52	9.308	2475	2478	2480	rBV	139	120	0.02%	0.003%
53	9.343	2484	2489	2491	rBB	124	109	0.02%	0.003%
54	9.369	2494	2497	2500	rBV	142	145	0.03%	0.003%
55	9.420	2500	2513	2533	rBV	263659	431871	82.88%	10.247%
56	9.545	2550	2552	2555	rBB	161	109	0.02%	0.003%
57	9.584	2562	2564	2568	rBV	120	126	0.02%	0.003%
58	9.674	2587	2592	2594	rBV	138	142	0.03%	0.003%
59	9.690	2594	2597	2601	rVV2	232	224	0.04%	0.005%
60	9.716	2603	2605	2609	rVB2	261	190	0.04%	0.005%
61	9.742	2609	2613	2618	rBV	145	222	0.04%	0.005%
62	9.825	2636	2639	2642	rBB	166	144	0.03%	0.003%
63	9.944	2672	2676	2679	rBV	149	175	0.03%	0.004%
64	10.025	2695	2701	2704	rVB2	291	349	0.07%	0.008%
65	10.118	2728	2730	2734	rVB2	296	183	0.04%	0.004%
66	10.250	2766	2771	2778	rVB2	969	1170	0.22%	0.028%
67	10.349	2799	2802	2811	rVB2	363	484	0.09%	0.011%
68	10.401	2811	2818	2821	rBB2	461	469	0.09%	0.011%
69	10.423	2821	2825	2830	rBV	152	235	0.05%	0.006%
70	10.472	2836	2840	2842	rBV	148	127	0.02%	0.003%
71	10.549	2861	2864	2867	rBV2	204	152	0.03%	0.004%
72	10.671	2895	2902	2909	rVV2	1444	1831	0.35%	0.043%
73	10.758	2917	2929	2944	rBV	174861	276621	53.08%	6.563%
74	10.864	2958	2962	2964	rBV2	258	235	0.05%	0.006%
75	11.063	3018	3024	3026	rBV	409	390	0.07%	0.009%
76	11.121	3037	3042	3045	rBV4	754	646	0.12%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
 Data File : VU046459.D
 Acq On : 17 Dec 2021 06:27
 Operator : SY/MD
 Sample : M5121-15 20X
 Misc : 7.20g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGL65

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.208	3068	3069	3073	rVB	265	123	0.02%	0.003%
78	11.317	3097	3103	3106	rBV3	951	837	0.16%	0.020%
79	11.372	3115	3120	3121	rBV3	924	677	0.13%	0.016%
80	11.417	3128	3134	3141	rBV5	3102	3897	0.75%	0.092%
81	11.574	3176	3183	3189	rBV4	1336	1729	0.33%	0.041%
82	11.642	3197	3204	3210	rVB3	784	975	0.19%	0.023%
83	11.700	3214	3222	3227	rBV5	1971	2933	0.56%	0.070%
84	11.812	3245	3257	3271	rBV	299127	463789	89.00%	11.004%
85	11.944	3287	3298	3301	rBV4	1717	2730	0.52%	0.065%
86	12.195	3358	3376	3394	rBV	246319	395589	75.91%	9.386%
87	12.269	3394	3399	3405	rVB3	533	647	0.12%	0.015%
88	12.388	3431	3436	3437	rBV2	776	647	0.12%	0.015%
89	12.777	3548	3557	3562	rVB	911	1210	0.23%	0.029%
90	12.832	3572	3574	3577	rVB3	633	248	0.05%	0.006%
91	12.947	3608	3610	3614	rVB	579	294	0.06%	0.007%
92	13.143	3667	3671	3672	rBV2	342	240	0.05%	0.006%
93	13.343	3731	3733	3737	rBV2	262	139	0.03%	0.003%
94	13.465	3769	3771	3776	rVB2	395	316	0.06%	0.007%
95	13.587	3803	3809	3817	rVB5	1709	2506	0.48%	0.059%
96	13.626	3817	3821	3825	rVB2	330	264	0.05%	0.006%
97	14.192	3991	3997	4005	rBV4	2059	2867	0.55%	0.068%
98	14.259	4015	4018	4020	rBV2	321	163	0.03%	0.004%
99	15.211	4308	4314	4321	rBV4	2063	2691	0.52%	0.064%
100	15.455	4385	4390	4394	rBV3	463	492	0.09%	0.012%




Sum of corrected areas: 4214639

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046459.D
Acq On : 17 Dec 2021 06:27
Operator : SY/MD
Sample : M5121-15 20X
Misc : 7.20g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL65

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

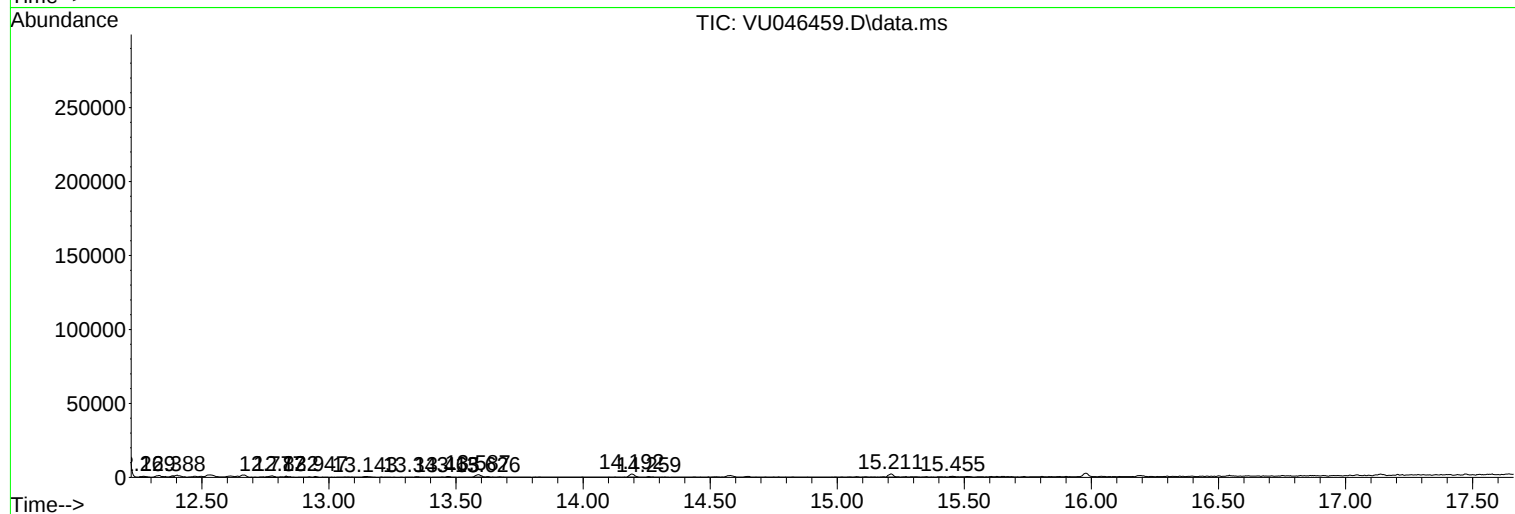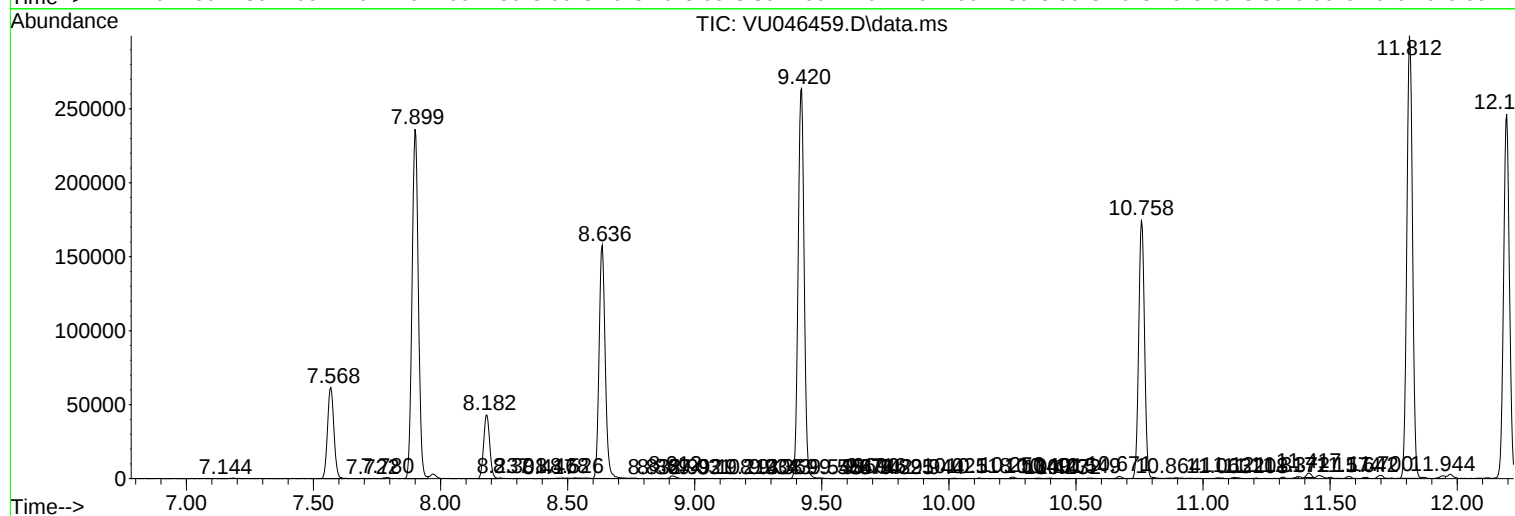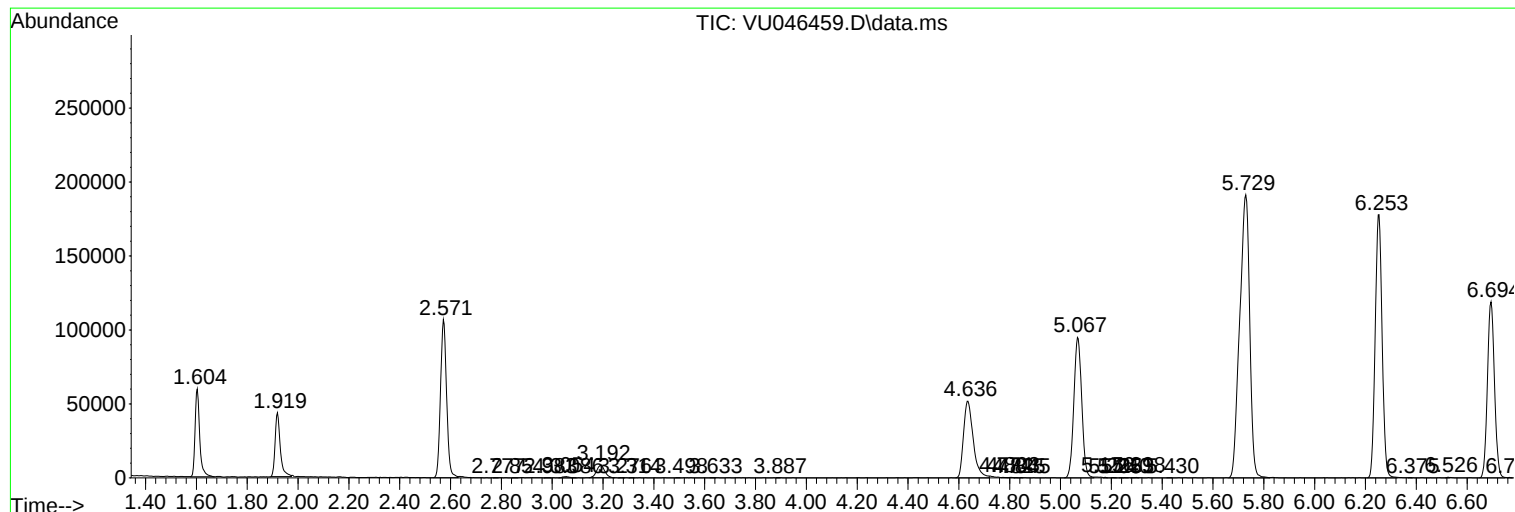

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046459.D
Acq On : 17 Dec 2021 06:27
Operator : SY/MD
Sample : M5121-15 20X
Misc : 7.20g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL65

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121621\
Data File : VU046459.D
Acq On : 17 Dec 2021 06:27
Operator : SY/MD
Sample : M5121-15 20X
Misc : 7.20g/5.0mL/100ul/5.0mL/MSVOA_U/MEOH
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGL65

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc